


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
Data File : BF132688.D
Acq On : 08 Mar 2023 13:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 09 16:26:19 2023

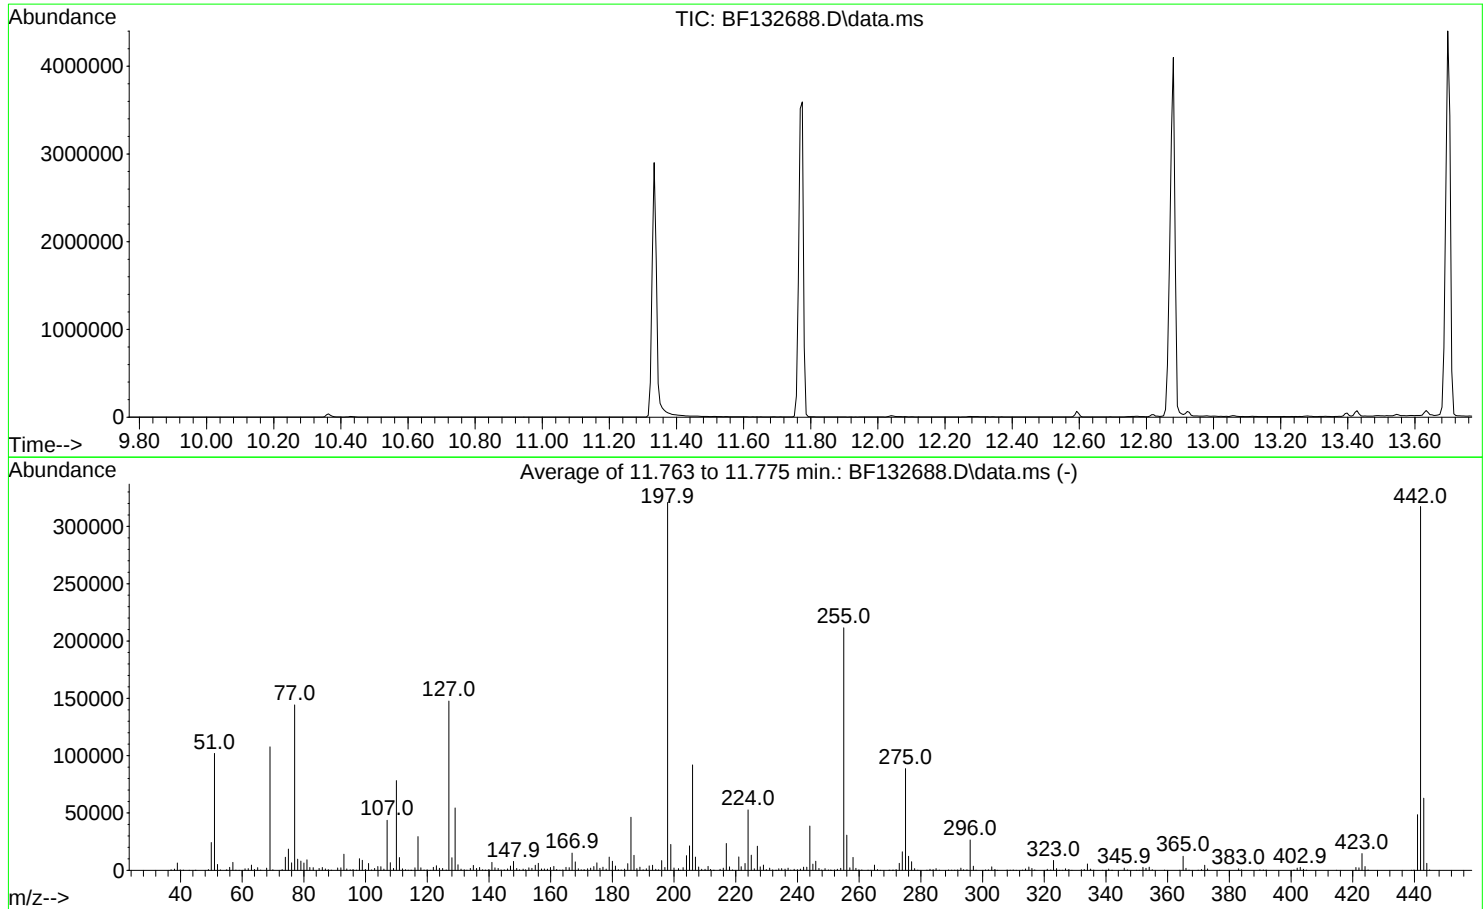

AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	101997	PASS
68	69	0.00	2	1.7	1851	PASS
69	198	0.00	100	33.5	107656	PASS
70	69	0.00	2	0.5	559	PASS
127	198	10	80	46.0	147563	PASS
197	198	0.00	2	0.8	2478	PASS
198	198	100	100	100.0	320917	PASS
199	198	5	9	7.0	22518	PASS
275	198	10	60	27.6	88715	PASS
365	198	1	100	3.8	12165	PASS
441	198	0.01	100	15.1	48558	PASS
442	442	50	100	100.0	317387	PASS
443	442	15	24	19.8	62955	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/8/2023	BNA_F	<u>BF132688.D</u>
Compound Name	Response	Retention Time
DDT	867026	13.698
DDD	18721	13.427
DDE	2419	13.057
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21140	888166	2.38

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
Data File : BF132688.D
Acq On : 08 Mar 2023 13:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 09 04:57:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 13:42:31 2023
Response via : Initial Calibration

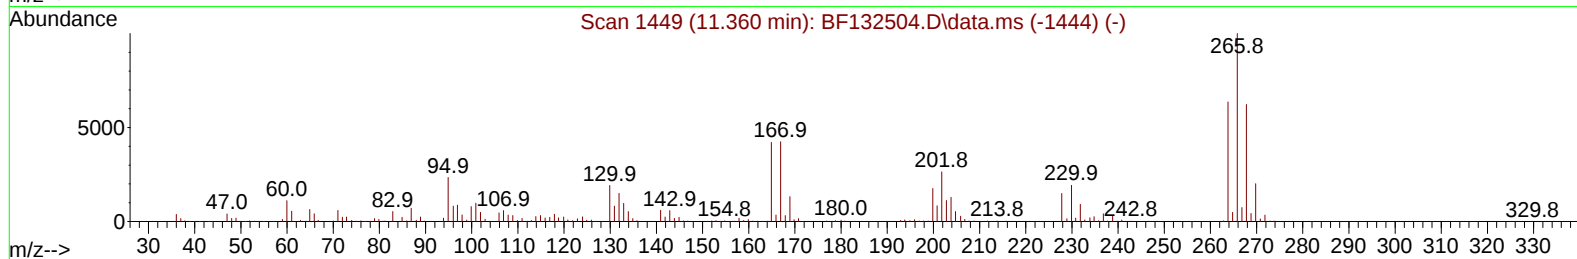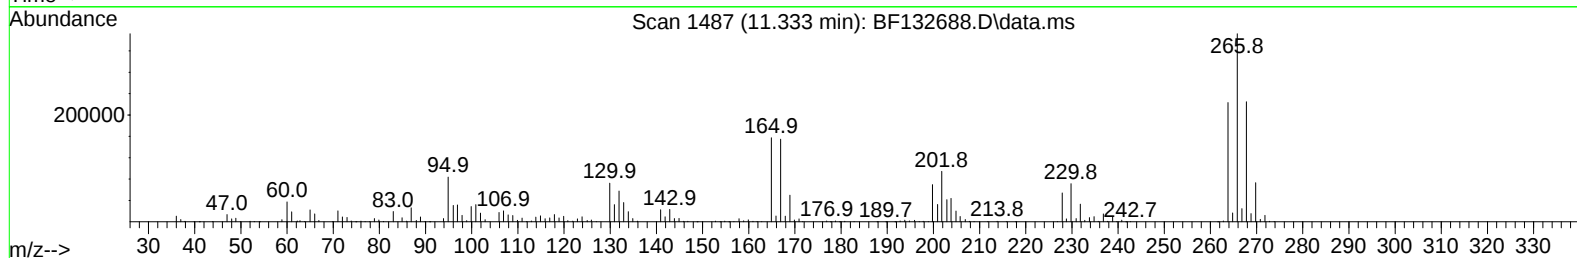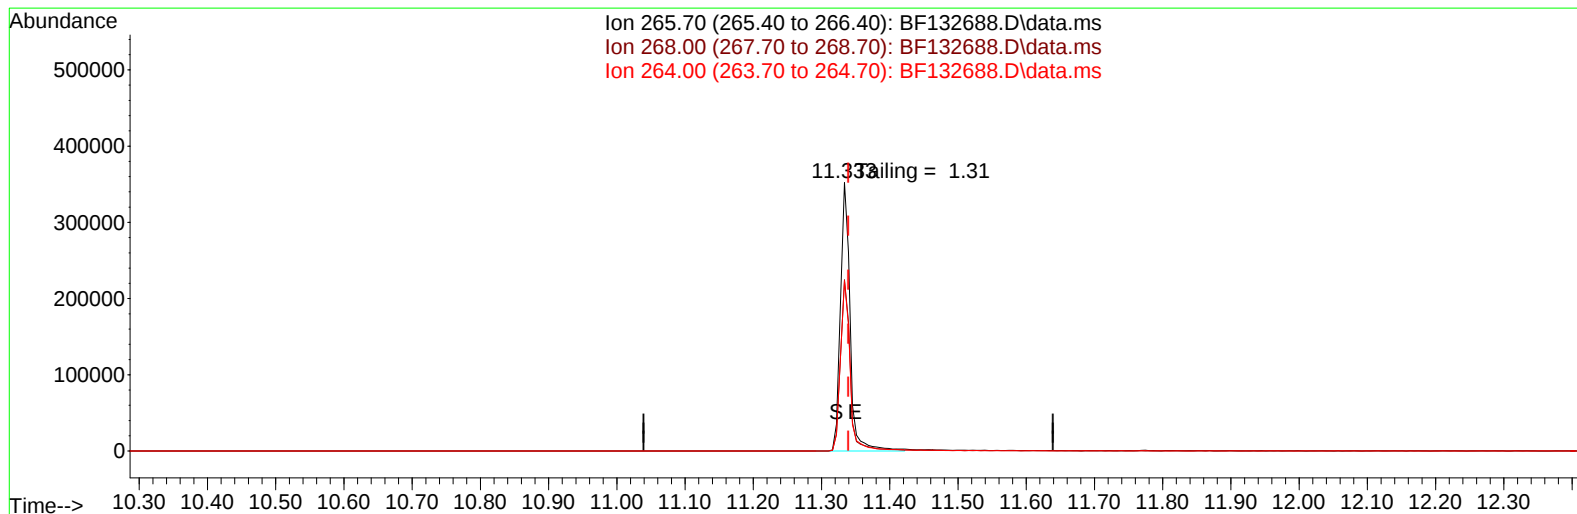

TIC: BF132688.D\data.ms

(70) Pentachlorophenol (C)

11.333min (-0.006) 304594.52 ng




response 347275

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.81
264.00	63.60	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
 Data File : BF132688.D
 Acq On : 08 Mar 2023 13:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 09 04:57:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 13:42:31 2023
 Response via : Initial Calibration

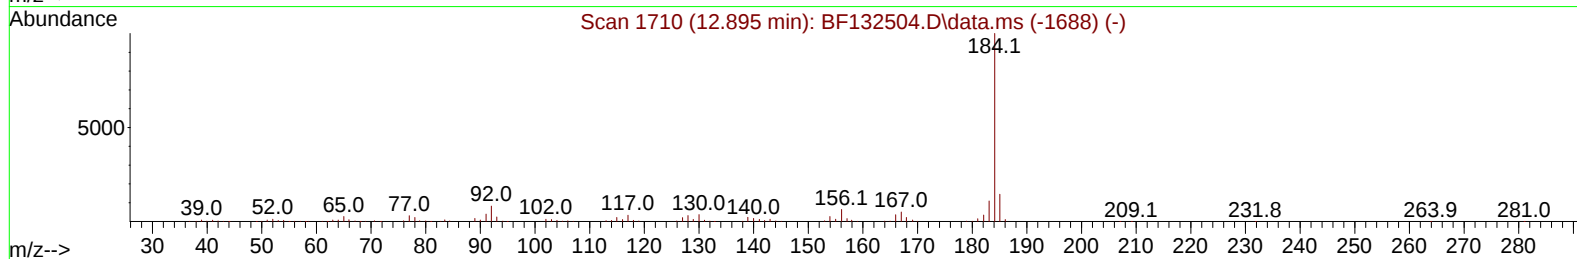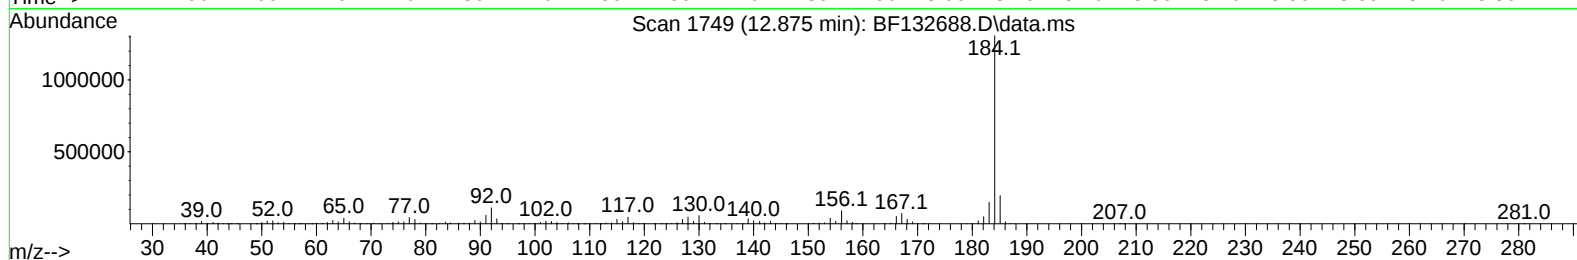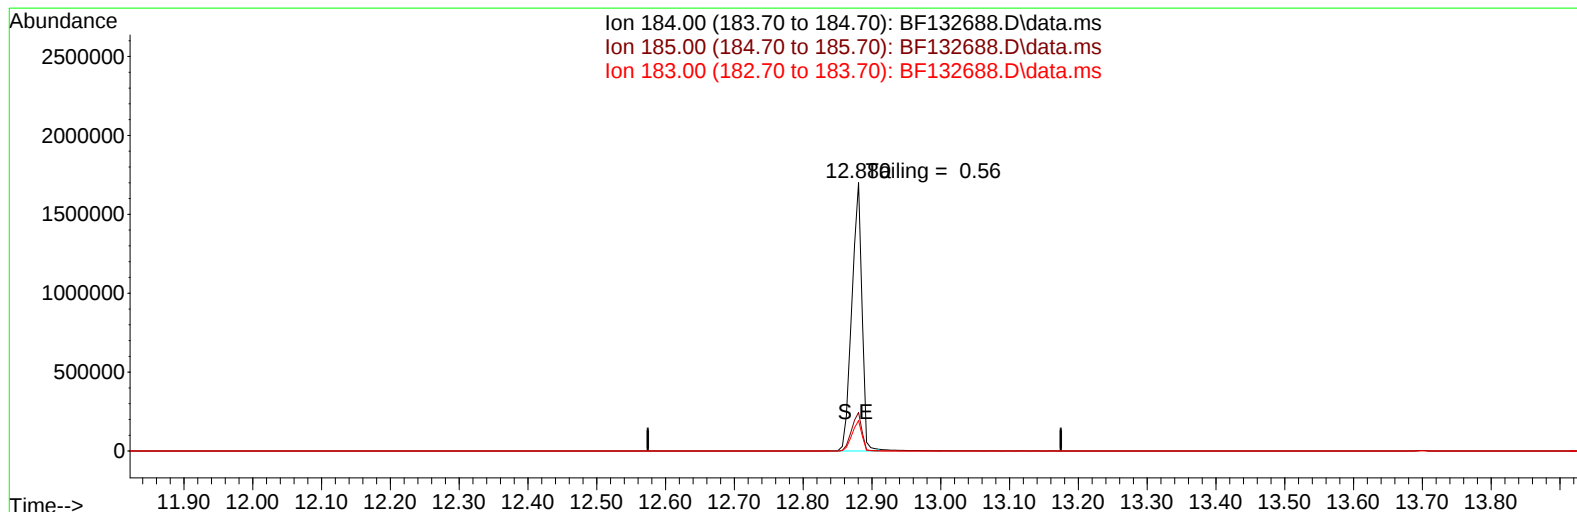

TIC: BF132688.D\data.ms

(77) Benzidine

12.875min (-12.875) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.60	0.00#
183.00	10.90	0.00#
0.00	0.00	0.00