
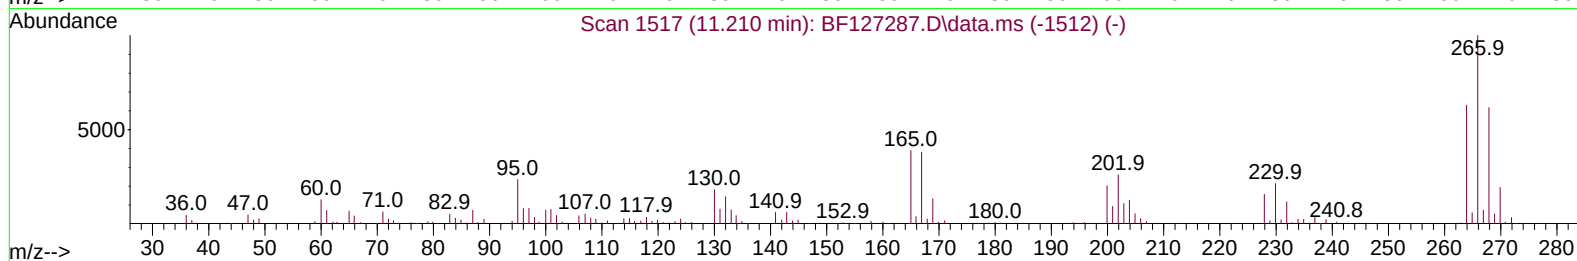
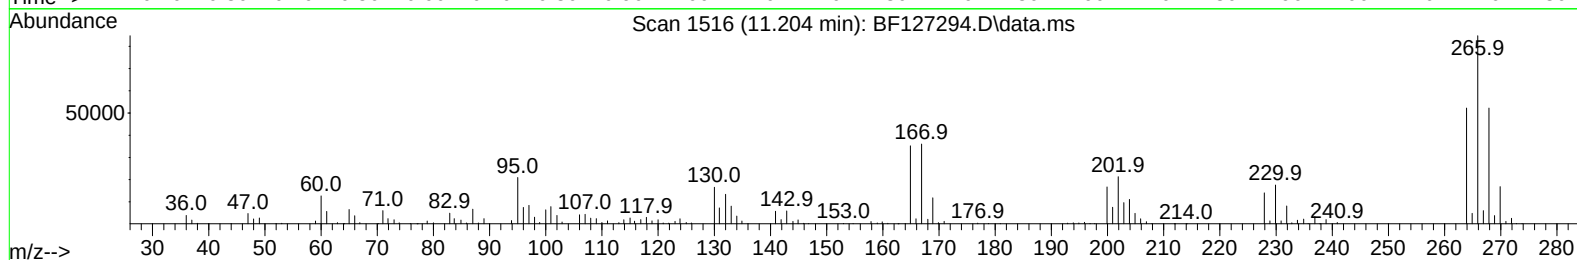


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
Data File : BF127294.D
Acq On : 11 Mar 2022 10:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 12:33:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

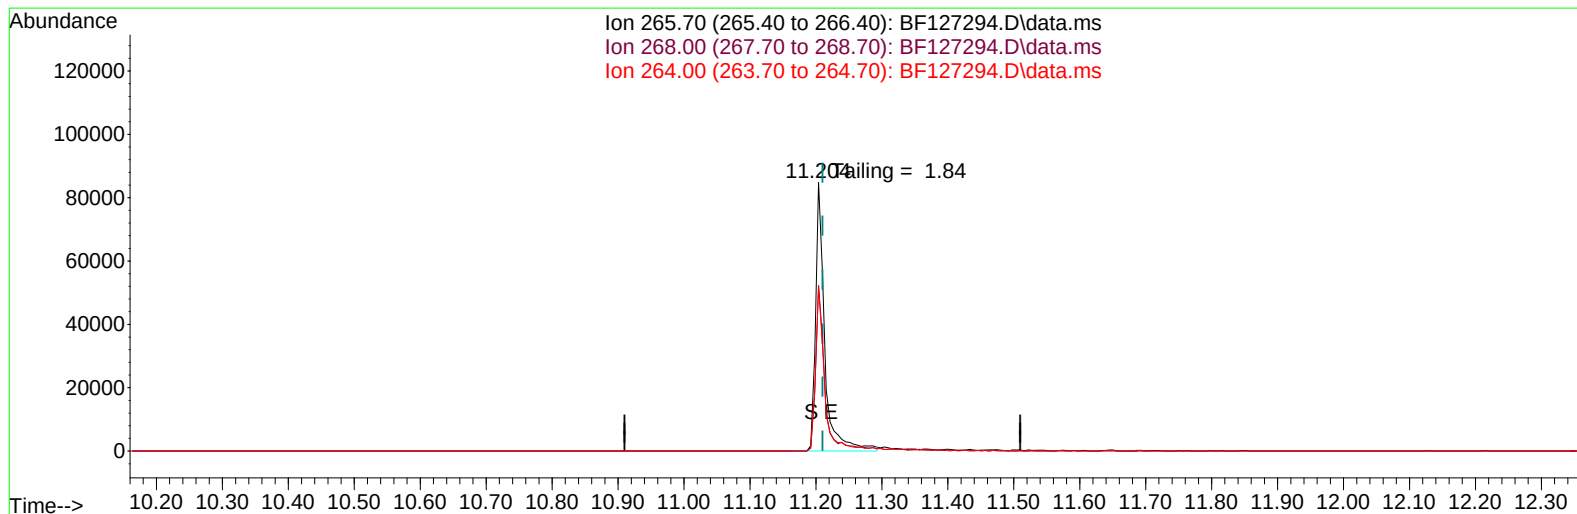

TIC: BF127294.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.006) 32607.23 ng

response 85614

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	61.60
264.00	63.00	61.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
Data File : BF127294.D
Acq On : 11 Mar 2022 10:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 12:33:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

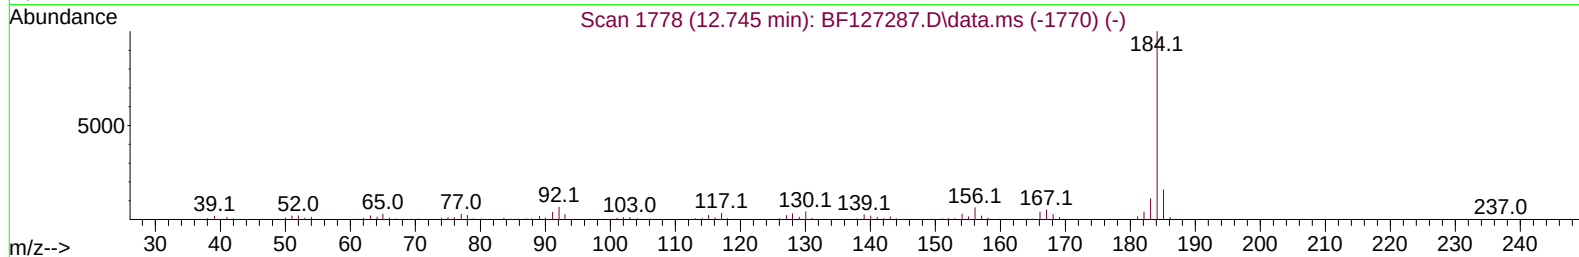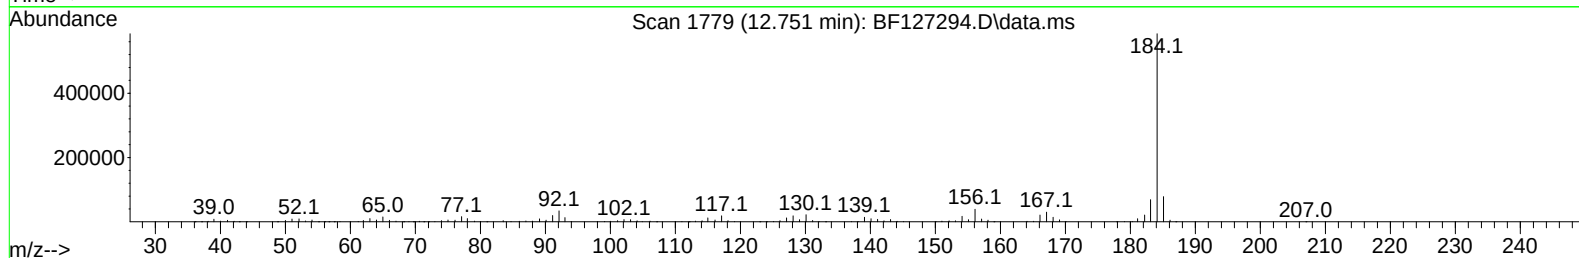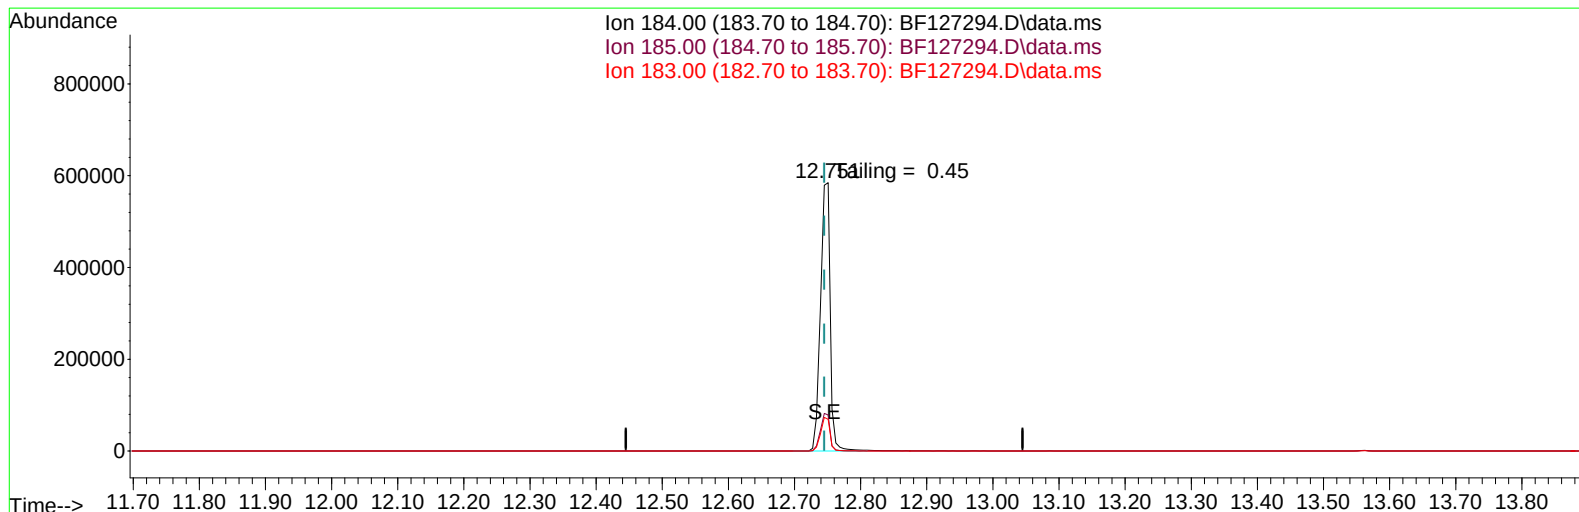

TIC: BF127294.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 599832

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.41
183.00	10.20	11.82
0.00	0.00	0.00