

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
 Data File : BF127296.D
 Acq On : 11 Mar 2022 11:22
 Operator : CG\JU
 Sample : PB143161BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143161BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127296.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	542	547	550	rBV	3195499	3263027	84.43%	14.125%
2	6.504	711	717	720	rBV	2868652	3337263	86.35%	14.446%
3	6.869	775	779	782	rBV	727607	636653	16.47%	2.756%
4	7.434	869	875	878	rBV	1941933	2283612	59.09%	9.885%
5	8.151	992	997	1000	rBV	782844	706582	18.28%	3.059%
6	9.228	1174	1180	1183	rBV	3420747	3474878	89.91%	15.042%
7	9.910	1290	1296	1299	rBV	967289	855465	22.14%	3.703%
8	10.704	1426	1431	1434	rBV	2289037	2185350	56.55%	9.460%
9	11.398	1545	1549	1553	rBV	994817	887166	22.96%	3.840%
10	12.992	1815	1820	1823	rBV	3999950	3864647	100.00%	16.729%
11	14.045	1995	1999	2003	rBV	927077	801533	20.74%	3.470%
12	15.533	2247	2252	2262	rBV	522963	646187	16.72%	2.797%
13	17.262	2533	2546	2561	rVB3	34333	159335	4.12%	0.690%




Sum of corrected areas: 23101698

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
Data File : BF127296.D
Acq On : 11 Mar 2022 11:22
Operator : CG\JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

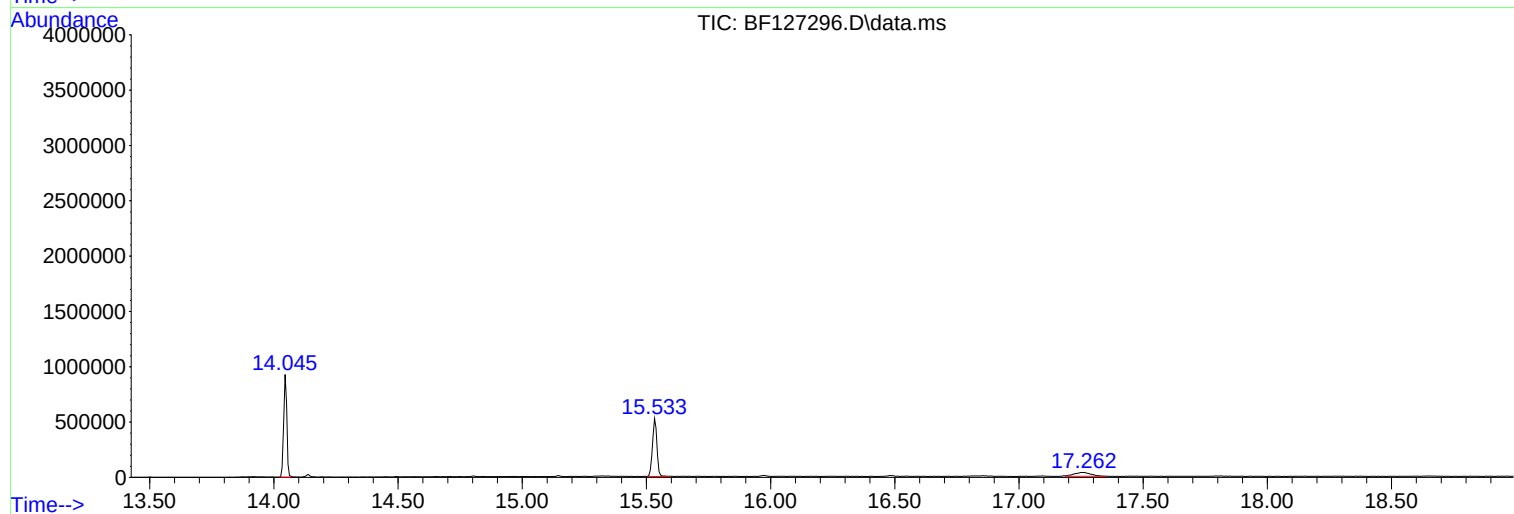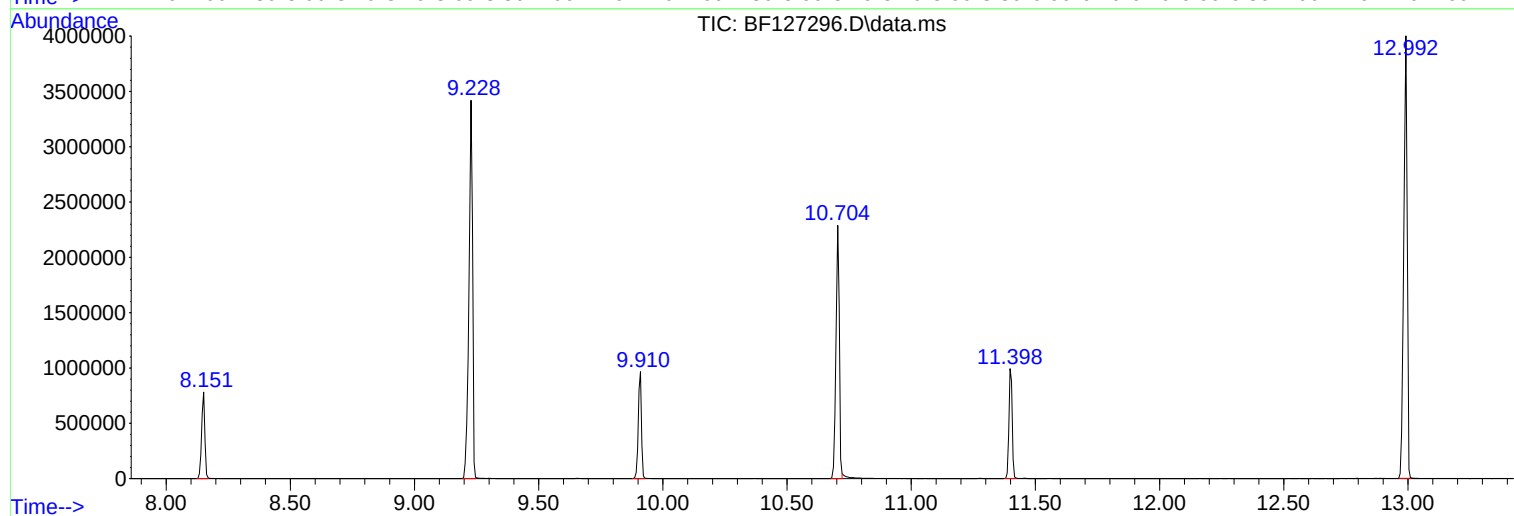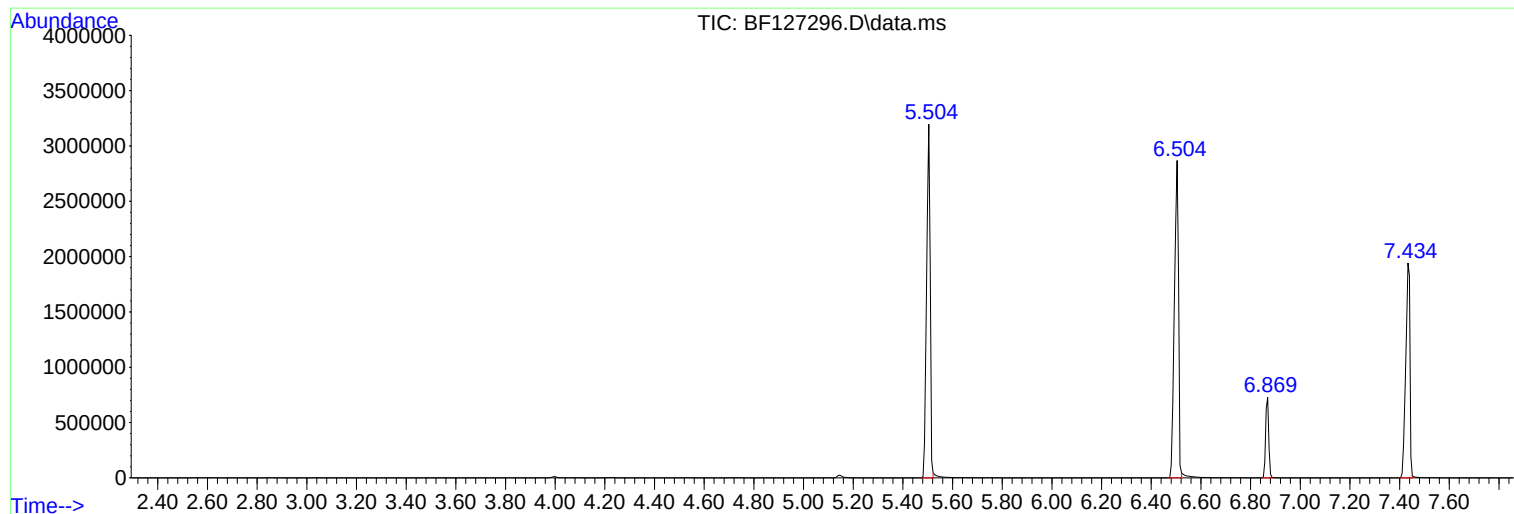

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
Data File : BF127296.D
Acq On : 11 Mar 2022 11:22
Operator : CG\JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143161BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (1,1'-Biphenyl)-4,4'-diamin... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.262	4.93 ng	159335	Perylene-d12	15.533

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			(1,1'-Biphenyl)-4,4'-diamine, N,...	360	C26H20N2	006311-48-4	83
2			Benzaldehyde, 4-hydroxy-3,5-dime...	360	C18H20N2O6	014414-32-5	52
3			1,10-Phenanthroline, 2,9-dimethy...	360	C26H20N2	004733-39-5	52
4			N,N'-di-2-Naphthyl-p-phenylenedi...	360	C26H20N2	000093-46-9	47
5			Ethene, 1-(anthracen-9-yl)-2-(4-...	360	C27H20O	1000163-55-1	47

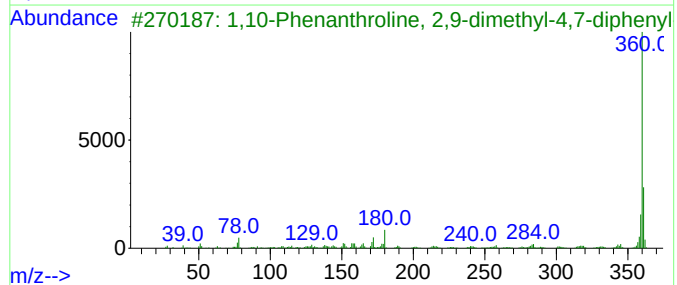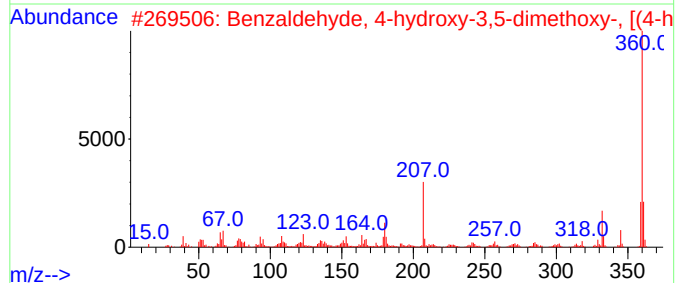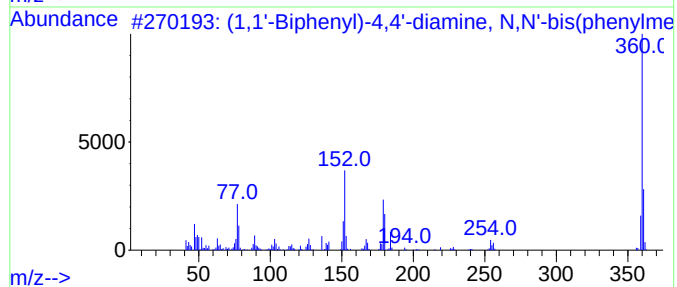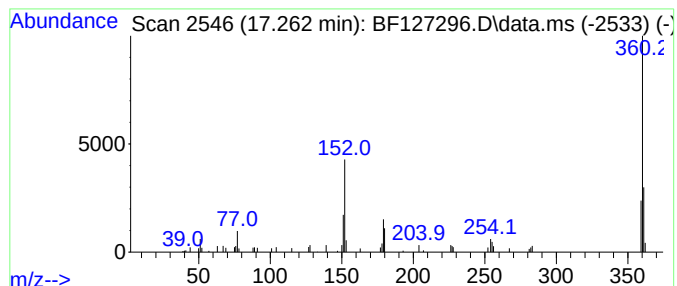

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
Data File : BF127296.D
Acq On : 11 Mar 2022 11:22
Operator : CG\JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(1,1'-Biphenyl)...	17.262	4.9	ng	159335	6	15.533	646187	20.0