

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
 Data File : BF127302.D
 Acq On : 11 Mar 2022 16:22
 Operator : CG\JU
 Sample : PB143171BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143171BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	543	548	551	rBV	3451032	3707186	78.55%	13.119%
2	6.504	711	717	720	rBV	3076942	3902447	82.69%	13.810%
3	6.869	775	779	782	rBV	801921	759483	16.09%	2.688%
4	7.434	869	875	878	rBV	2133557	2737546	58.01%	9.688%
5	8.151	991	997	1000	rBV	987839	995617	21.10%	3.523%
6	9.228	1173	1180	1183	rBV	4076939	4551592	96.45%	16.107%
7	9.910	1290	1296	1299	rBV	1223766	1161064	24.60%	4.109%
8	10.704	1424	1431	1434	rBV	2769503	2762781	58.54%	9.777%
9	11.398	1543	1549	1553	rBV	1356047	1179968	25.00%	4.176%
10	12.992	1814	1820	1823	rBV	4269043	4719250	100.00%	16.701%
11	14.045	1995	1999	2003	rBV	1146913	995359	21.09%	3.522%
12	15.533	2247	2252	2263	rBV	642458	785505	16.64%	2.780%




Sum of corrected areas: 28257798

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
Data File : BF127302.D
Acq On : 11 Mar 2022 16:22
Operator : CG\JU
Sample : PB143171BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

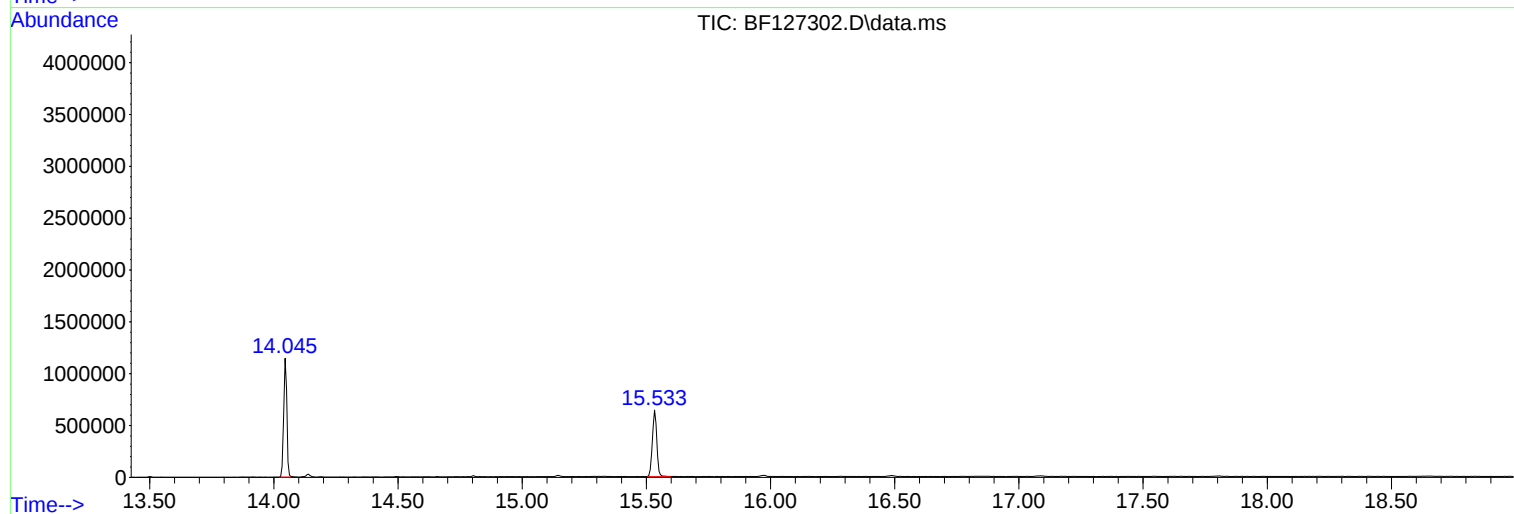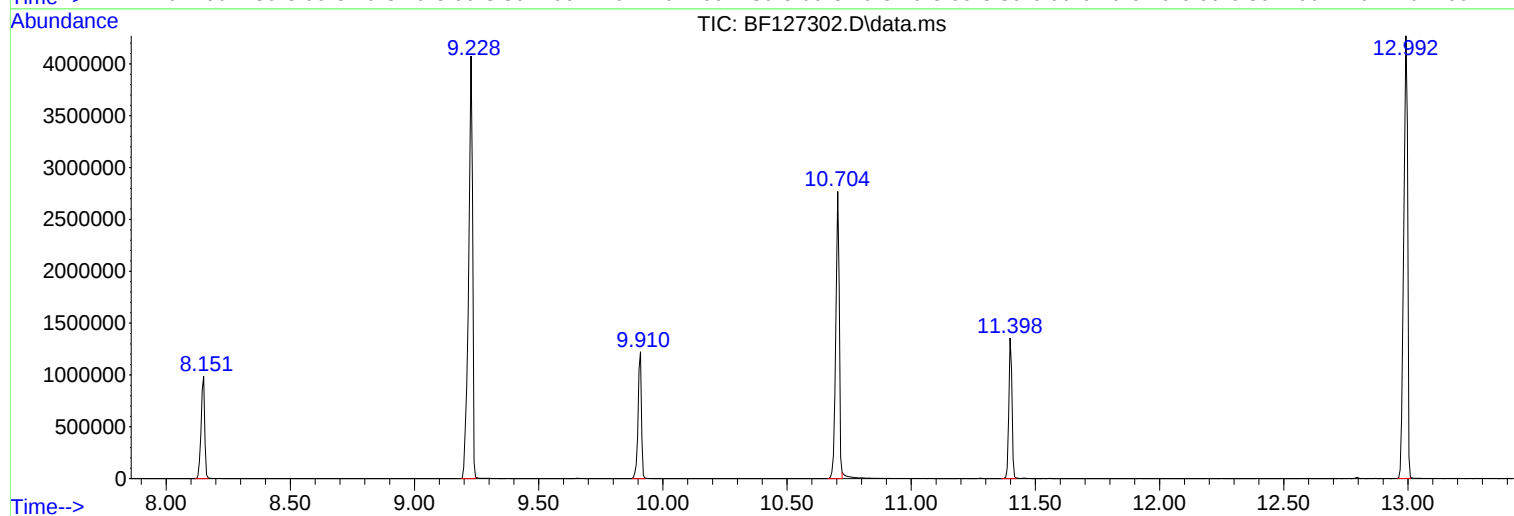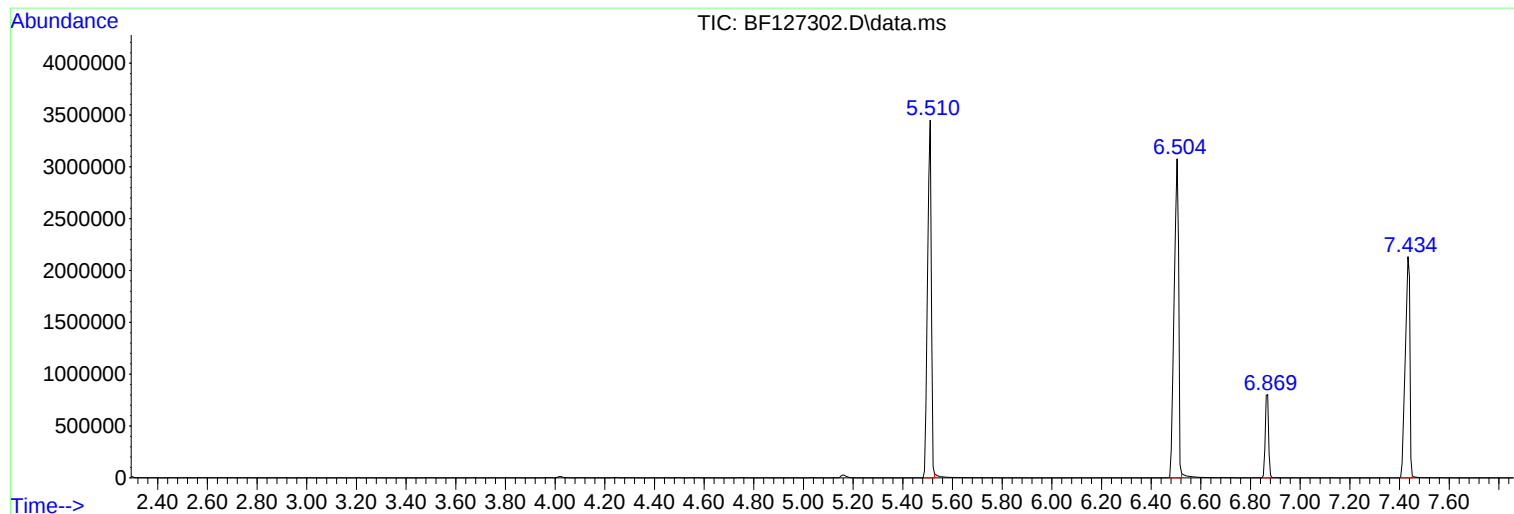

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
Data File : BF127302.D
Acq On : 11 Mar 2022 16:22
Operator : CG\JU
Sample : PB143171BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
Data File : BF127302.D
Acq On : 11 Mar 2022 16:22
Operator : CG\JU
Sample : PB143171BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------