
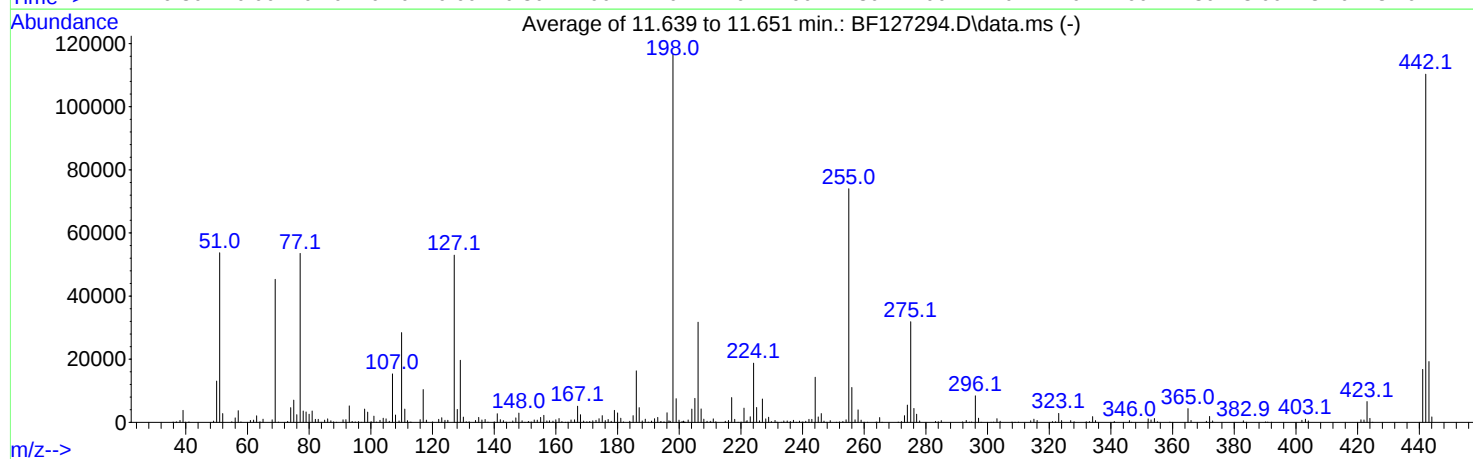


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
 Data File : BF127294.D
 Acq On : 11 Mar 2022 10:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 10 16:51:53 2022

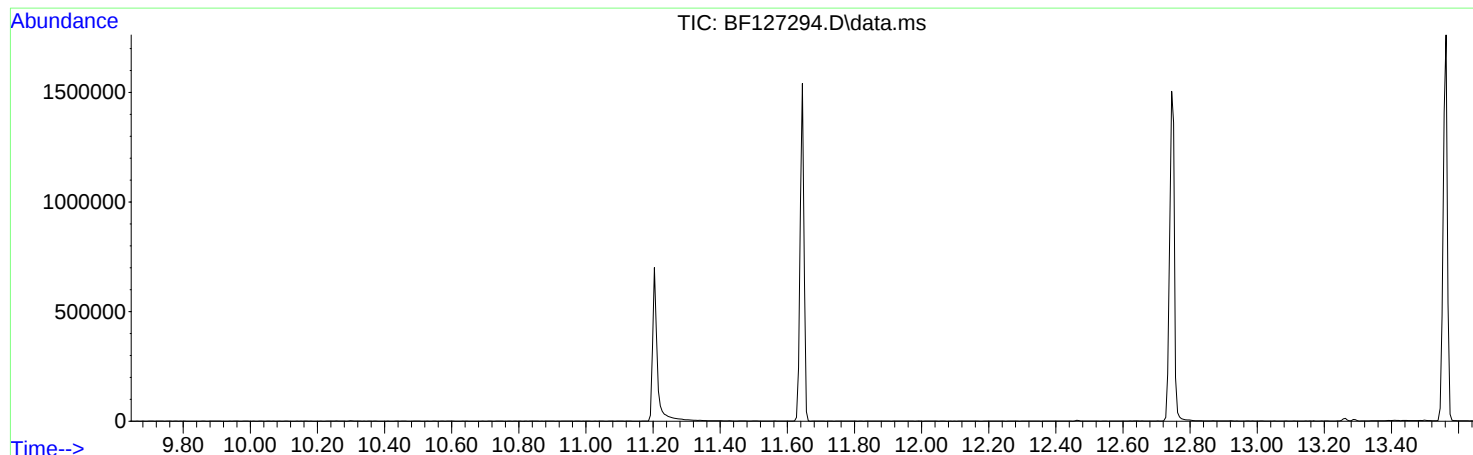




AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	53720	PASS
68	69	0.00	2	1.8	802	PASS
69	198	0.00	100	38.9	45320	PASS
70	69	0.00	2	0.3	124	PASS
127	198	10	80	45.5	52997	PASS
197	198	0.00	2	0.4	511	PASS
198	198	100	100	100.0	116544	PASS
199	198	5	9	6.4	7506	PASS
275	198	10	60	27.3	31867	PASS
365	198	1	100	3.8	4373	PASS
441	198	0.01	100	14.4	16772	PASS
442	442	50	100	100.0	110315	PASS
443	442	15	24	17.5	19291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
Data File : BF127294.D
Acq On : 11 Mar 2022 10:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 11 12:33:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

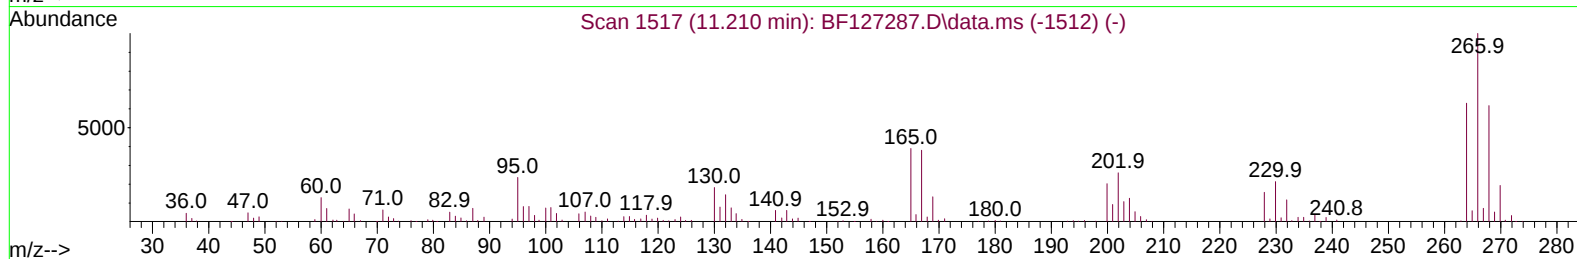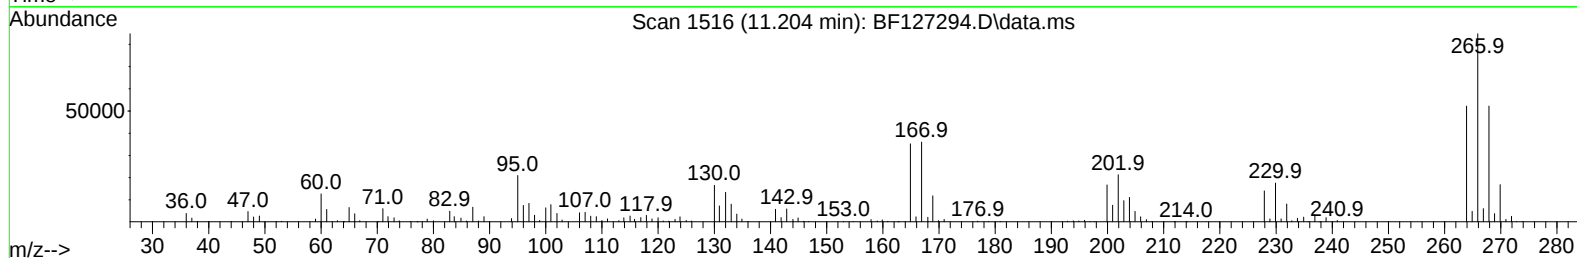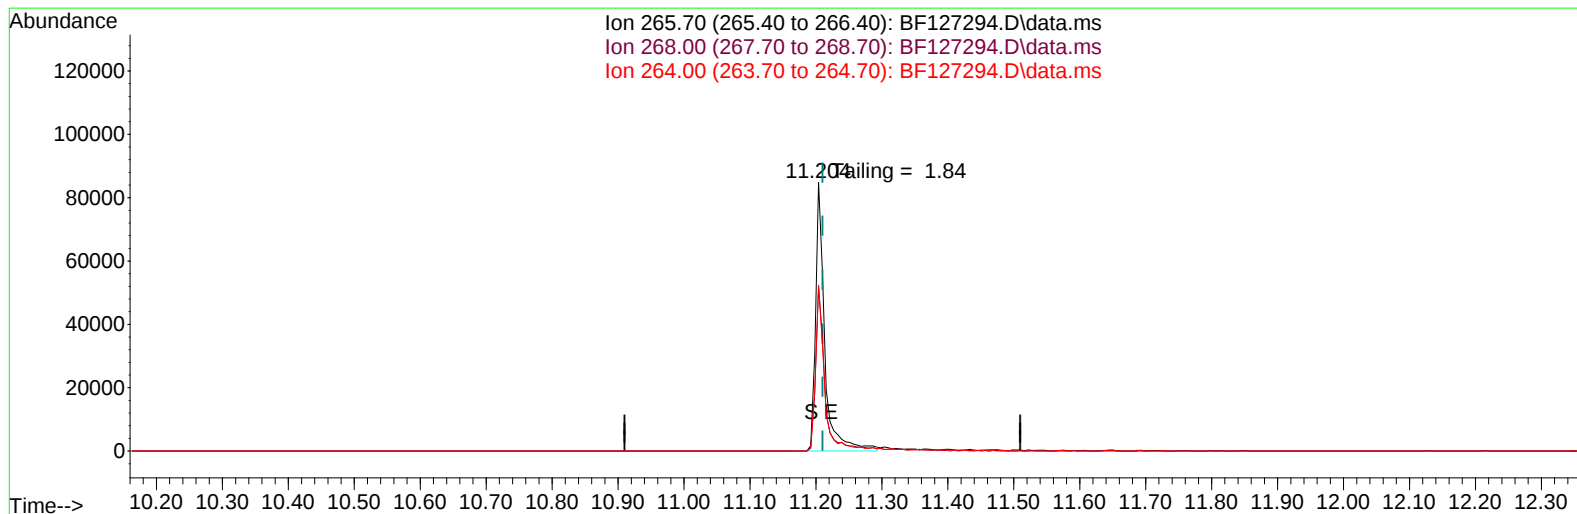

TIC: BF127294.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 32607.23 ng




response 85614

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	61.60
264.00	63.00	61.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031122\
 Data File : BF127294.D
 Acq On : 11 Mar 2022 10:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 11 12:33:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 10 16:51:53 2022
 Response via : Initial Calibration

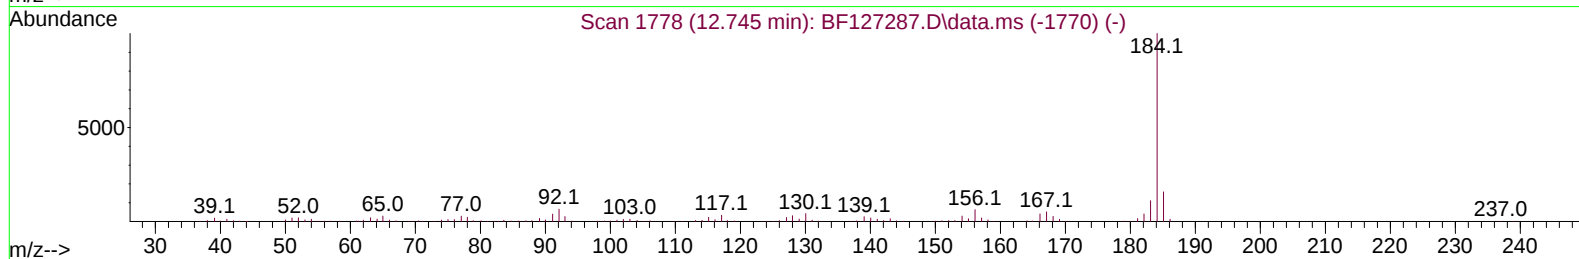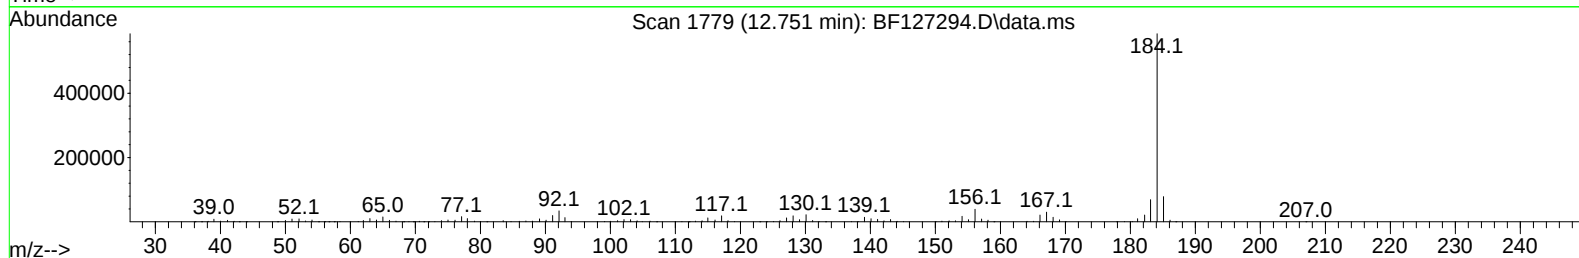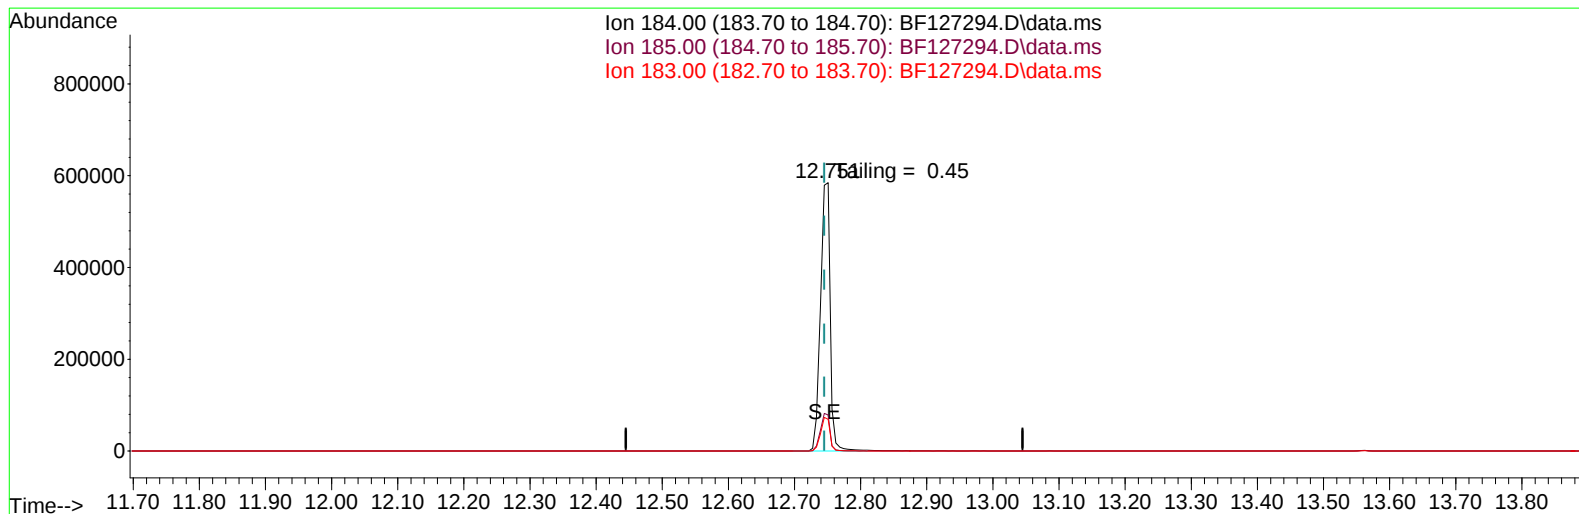

TIC: BF127294.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 599832

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.41
183.00	10.20	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/11/2022	BNA_F	<u>BF127294.D</u>
Compound Name	Response	Retention Time
DDT	307010	13.56
DDD	2714	13.26
DDE	164	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2878	309888	0.93

Instrument :
BNA_F
ClientSampleId :
DFTPP