

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
 Data File : BF127360.D
 Acq On : 16 Mar 2022 21:26
 Operator : CG\JU
 Sample : N1951-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BLIND-DUPLICATE

Quant Time: Mar 17 02:36:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 10 16:51:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.863	152	81564	20.000	ng	0.00
21) Naphthalene-d8	8.151	136	302736	20.000	ng	# 0.00
39) Acenaphthene-d10	9.904	164	177884	20.000	ng	-0.01
64) Phenanthrene-d10	11.398	188	321139	20.000	ng	# 0.00
76) Chrysene-d12	14.045	240	219203	20.000	ng	# 0.00
86) Perylene-d12	15.527	264	189639	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.487	112	520276	102.542	ng	0.00
7) Phenol-d6	6.498	99	721135	103.318	ng	0.00
23) Nitrobenzene-d5	7.433	82	481660	65.706	ng	0.00
42) 2,4,6-Tribromophenol	10.698	330	192802	100.685	ng	-0.01
45) 2-Fluorobiphenyl	9.222	172	853353	67.823	ng	-0.01
79) Terphenyl-d14	12.986	244	958317	75.281	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127360.D
Acq On : 16 Mar 2022 21:26
Operator : CG\JU
Sample : N1951-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BLIND-DUPLICATE

Quant Time: Mar 17 02:36:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration




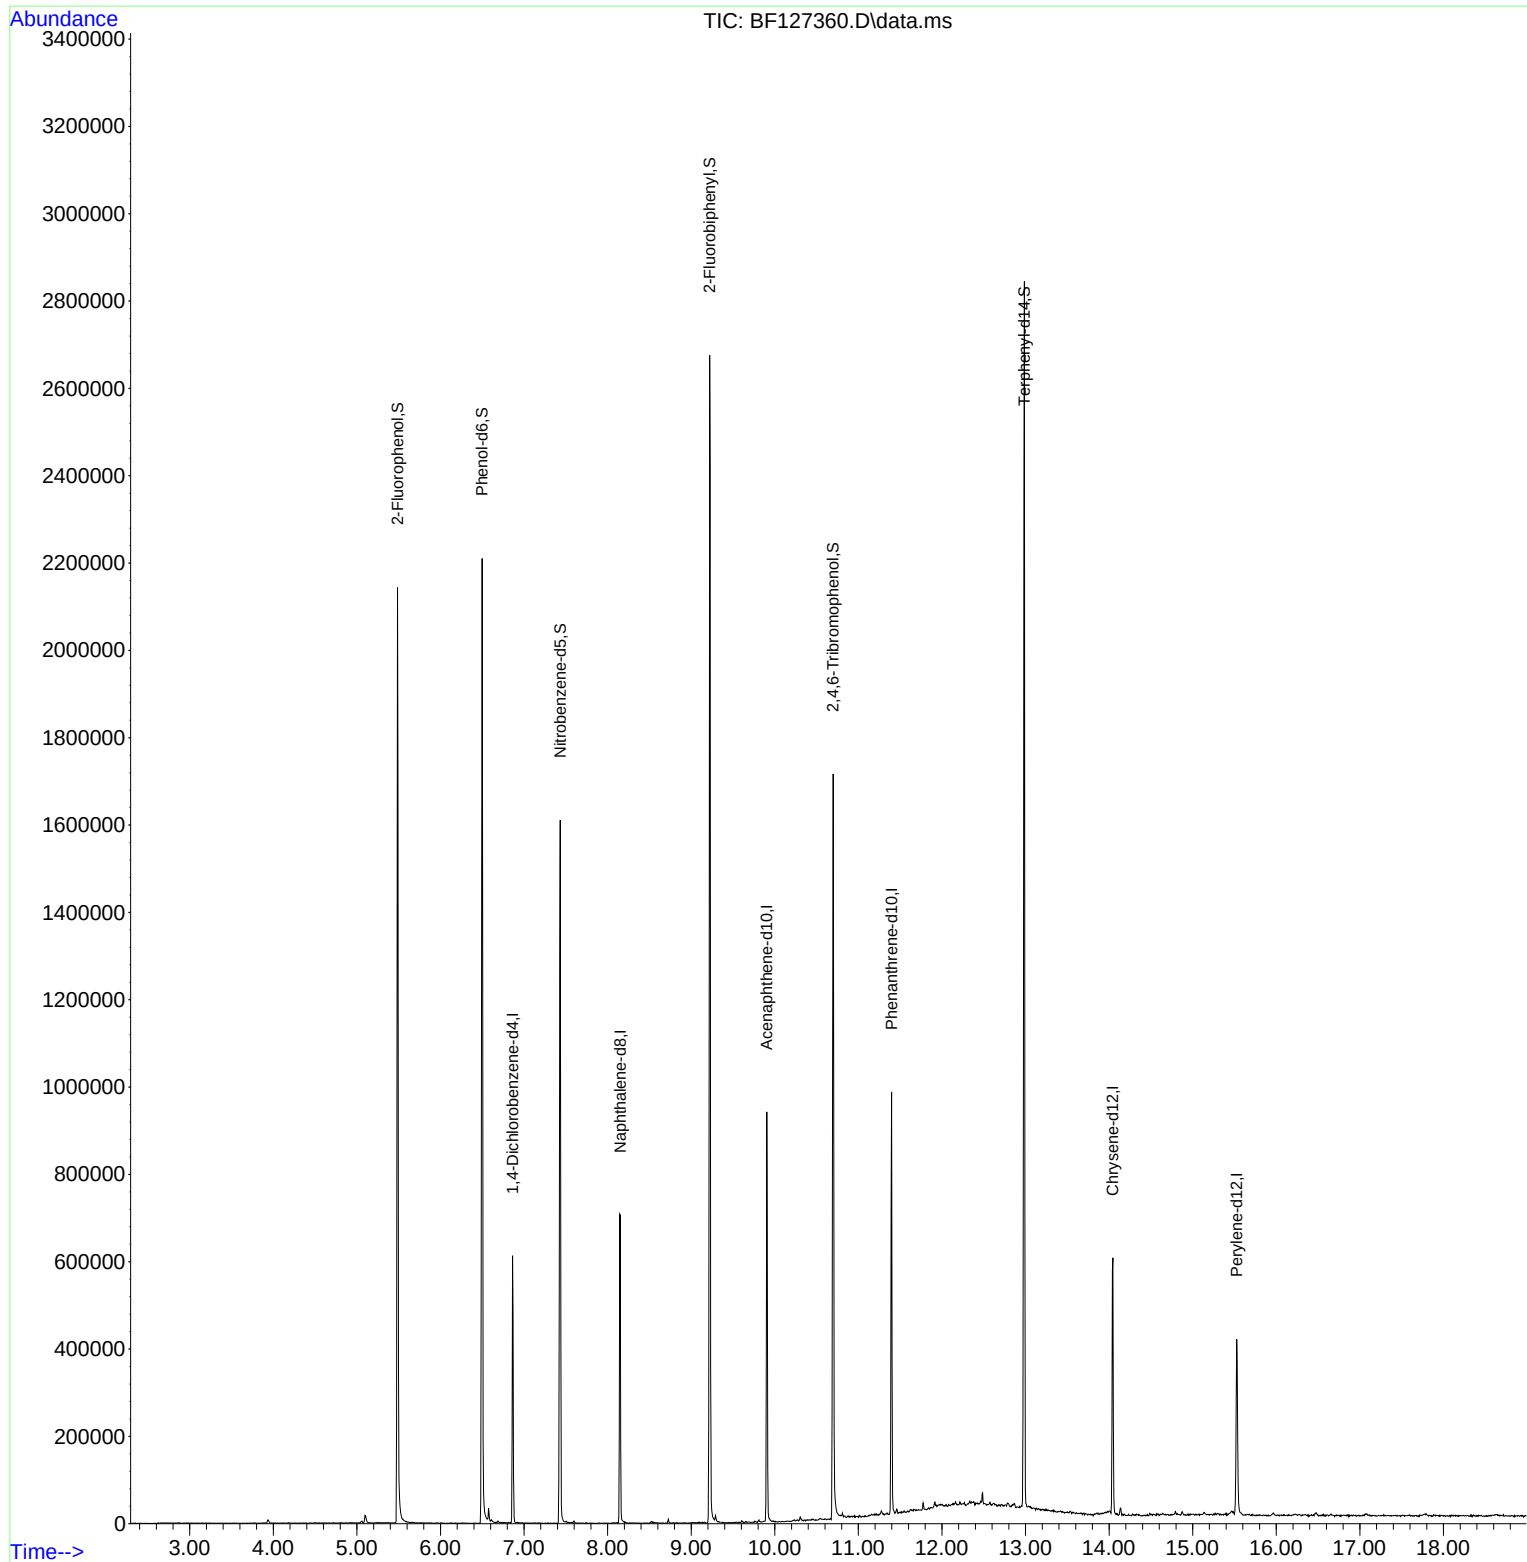


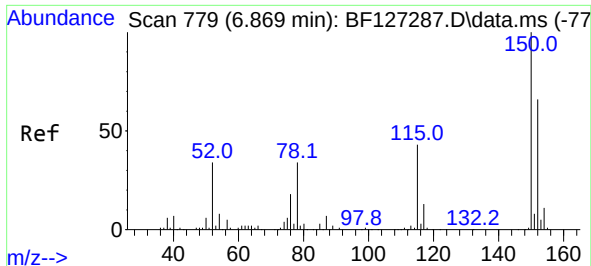

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.863 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26




Instrument :
BNA_F
ClientSampleId :
BLIND-DUPLICATE


Tgt Ion:152 Resp: 81564
Ion Ratio Lower Upper
152 100
150 145.6 128.1 192.1
115 64.3 56.7 85.1

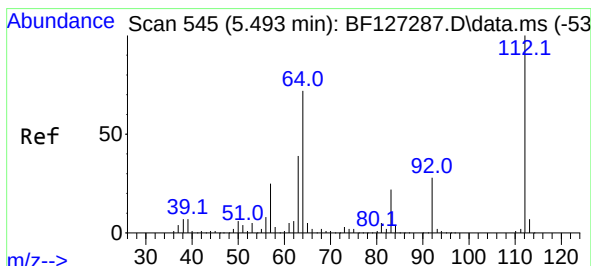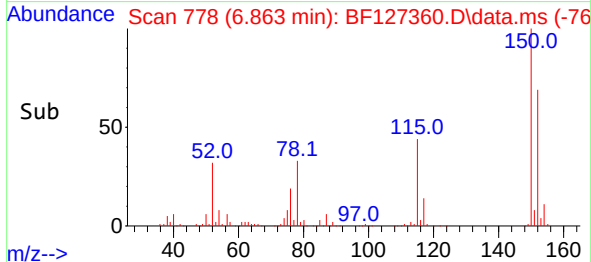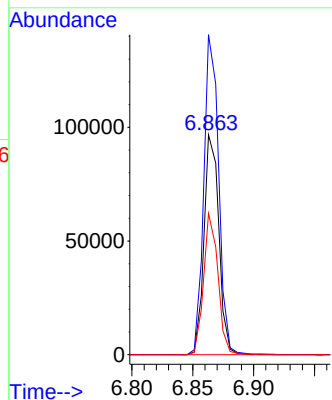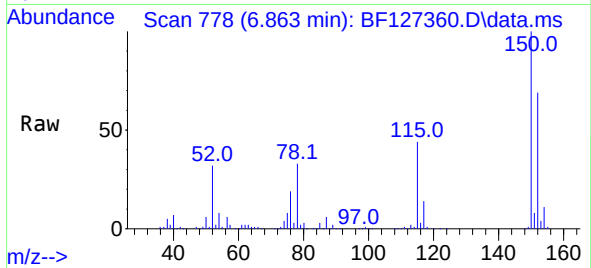

#5
2-Fluorophenol
Concen: 102.542 ng
RT: 5.487 min Scan# 544
Delta R.T. -0.006 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26

Tgt Ion:112 Resp: 520276
Ion Ratio Lower Upper
112 100
64 75.4 49.5 74.3#
63 39.4 23.9 35.9#


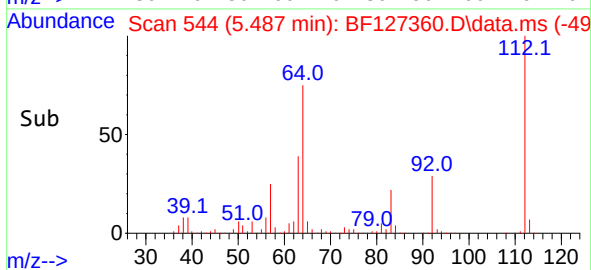
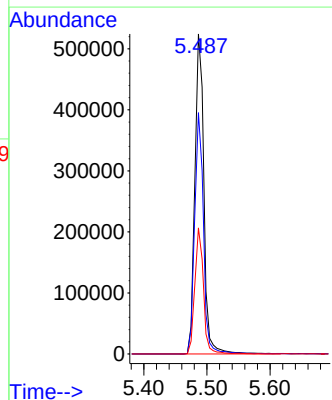
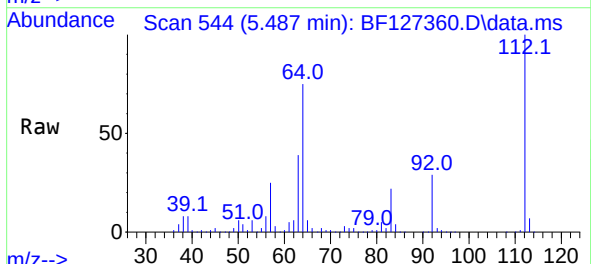


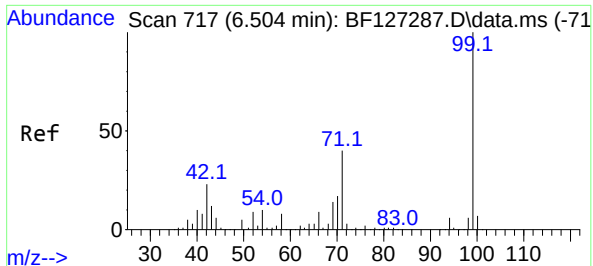

#7
Phenol-d6
Concen: 103.318 ng
RT: 6.498 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26




Instrument :
BNA_F
ClientSampleId :
BLIND-DUPLICATE


Tgt Ion: 99 Resp: 721135
Ion Ratio Lower Upper
99 100
42 22.3 14.2 21.4#
71 37.4 24.3 36.5#

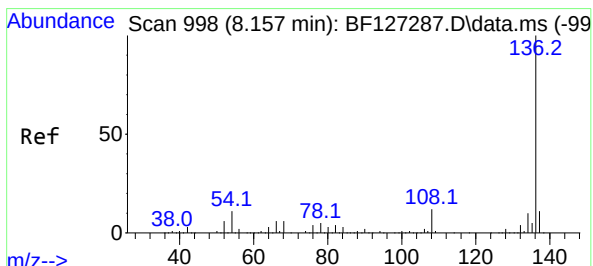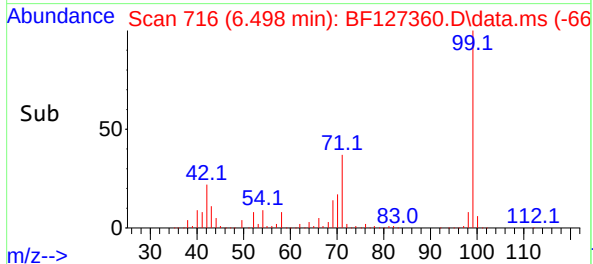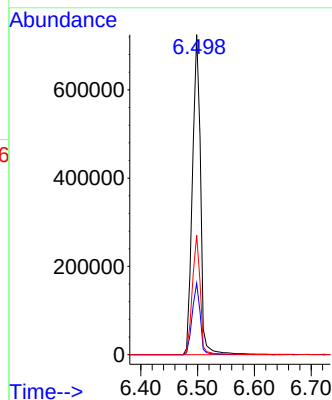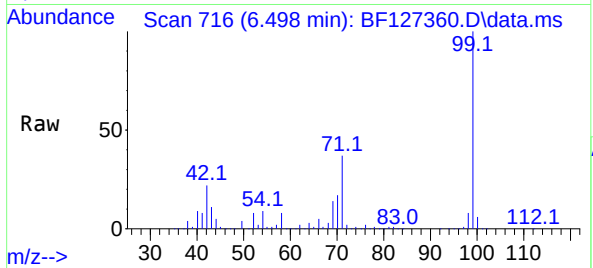

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.151 min Scan# 997
Delta R.T. -0.006 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26

Tgt Ion: 136 Resp: 302736
Ion Ratio Lower Upper
136 100
137 10.2 8.6 13.0
54 10.1 7.8 11.6
68 6.0 6.3 9.5#


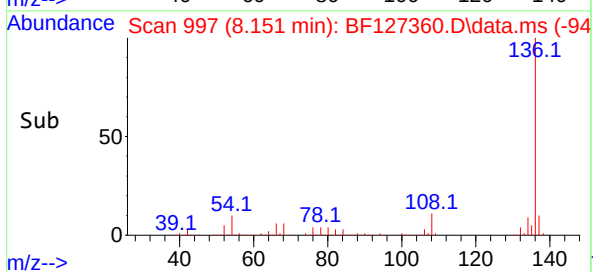
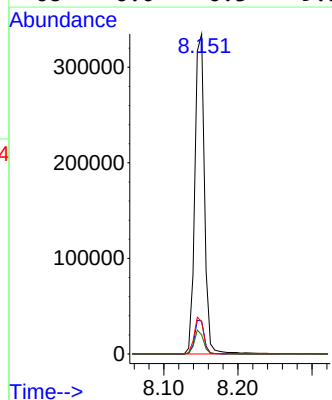
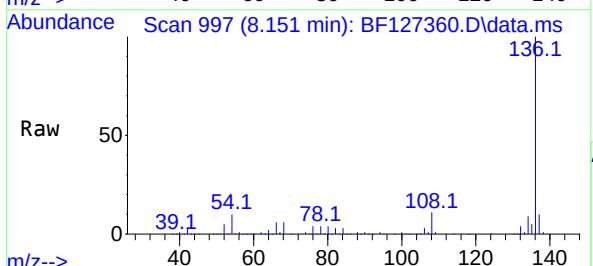


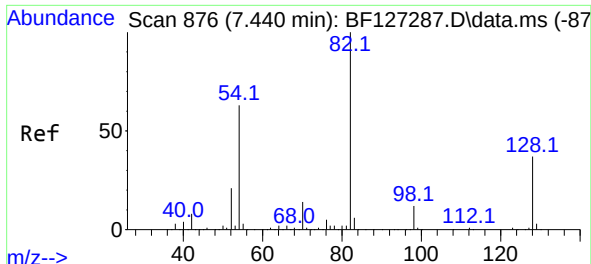

#23
Nitrobenzene-d5
Concen: 65.706 ng
RT: 7.433 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26




Instrument :
BNA_F
ClientSampleId :
BLIND-DUPLICATE


Tgt Ion: 82 Resp: 481660
Ion Ratio Lower Upper
82 100
128 38.4 32.7 49.1
54 60.1 41.7 62.5

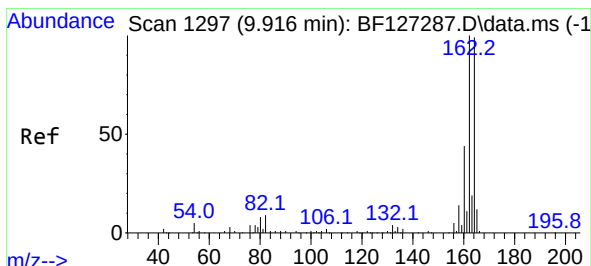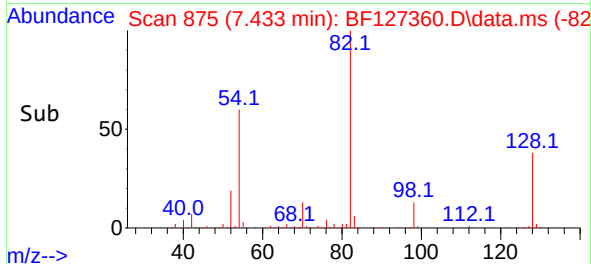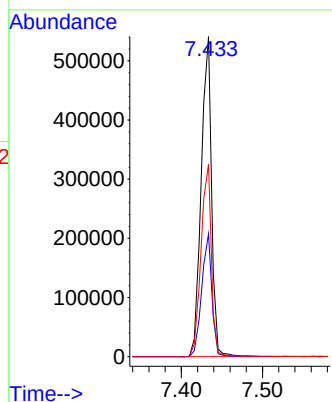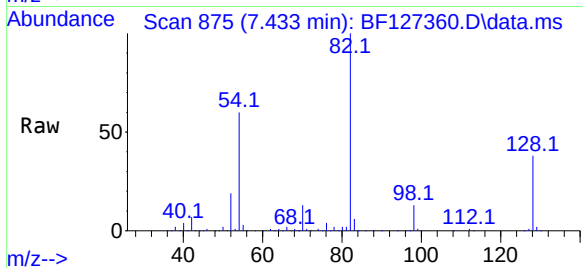

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.904 min Scan# 1295
Delta R.T. -0.012 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26

Tgt Ion: 164 Resp: 177884
Ion Ratio Lower Upper
164 100
162 98.4 81.4 122.0
160 42.3 36.6 54.8

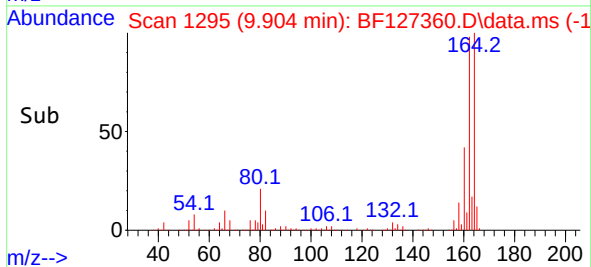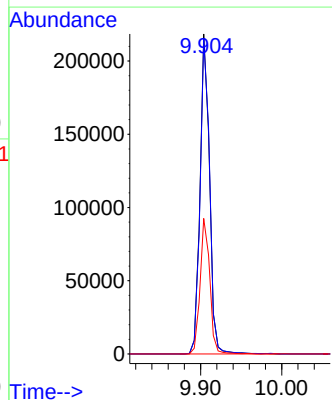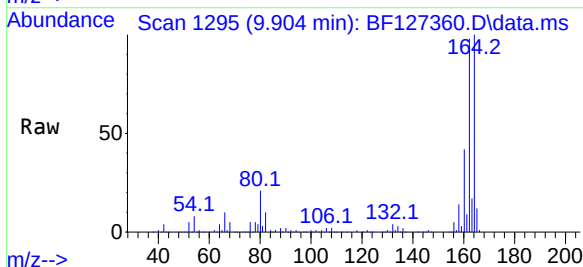

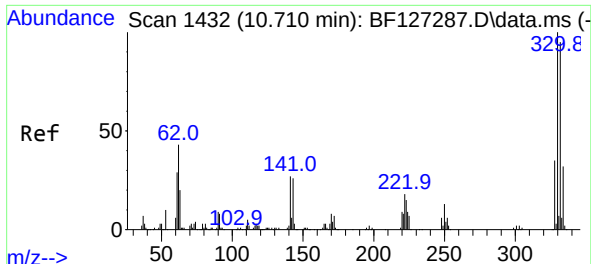

#42

2,4,6-Tribromophenol

Concen: 100.685 ng

RT: 10.698 min Scan# 1430

Delta R.T. -0.012 min

Lab File: BF127360.D


Acq: 16 Mar 2022 21:26

Instrument :

BNA_F

ClientSampleId :

BLIND-DUPLICATE

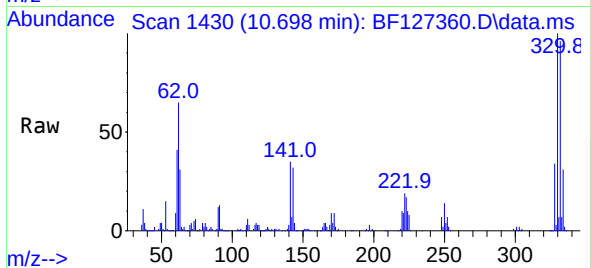




Tgt Ion:330 Resp: 192802

Ion Ratio Lower Upper

330 100

332 97.2 76.0 114.0

141 33.3 30.1 45.1

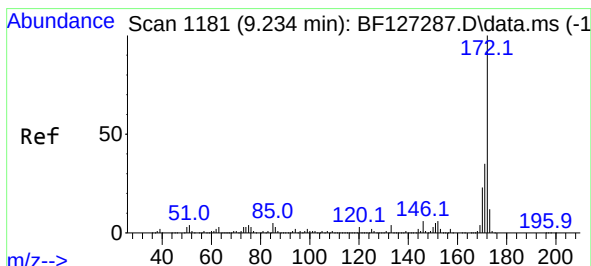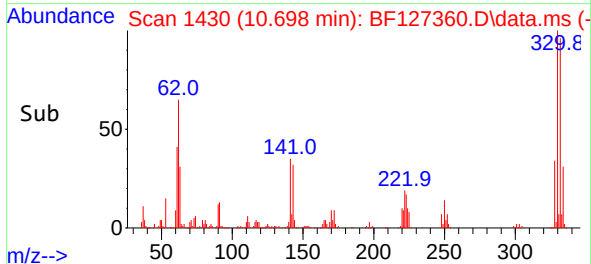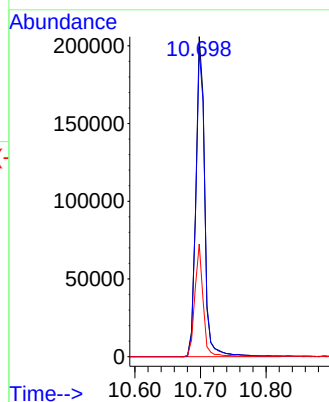

#45

2-Fluorobiphenyl

Concen: 67.823 ng

RT: 9.222 min Scan# 1179

Delta R.T. -0.012 min

Lab File: BF127360.D

Acq: 16 Mar 2022 21:26




Tgt Ion:172 Resp: 853353


Ion Ratio Lower Upper

172 100

171 34.6 28.3 42.5

170 23.2 19.0 28.6


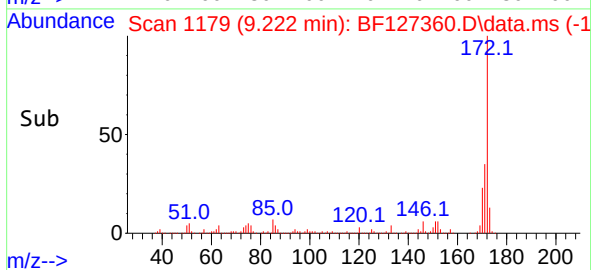
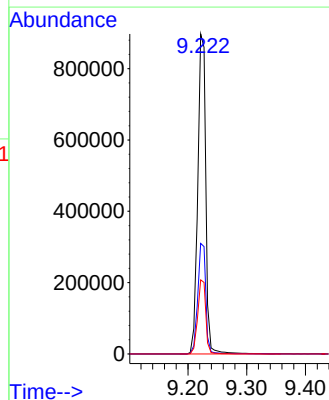
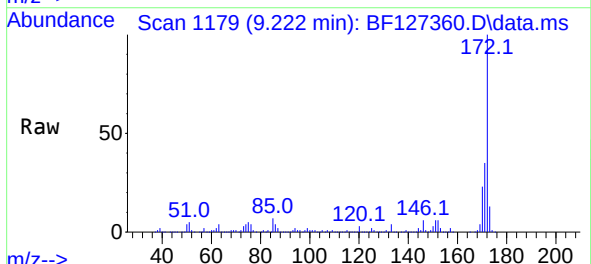


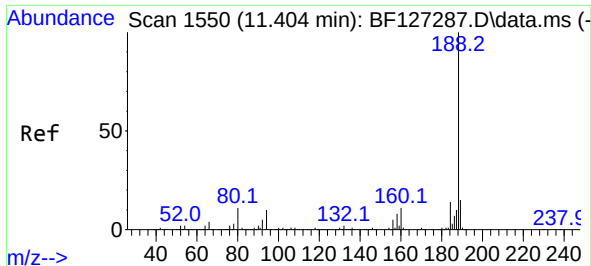

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.398 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26




Instrument :
BNA_F
ClientSampleId :
BLIND-DUPLICATE


Tgt Ion:188 Resp: 321139
Ion Ratio Lower Upper
188 100
94 9.1 10.1 15.1#
80 9.7 11.8 17.6#

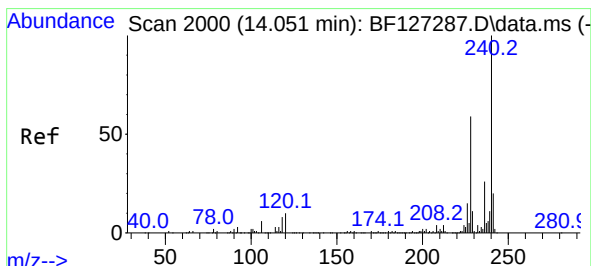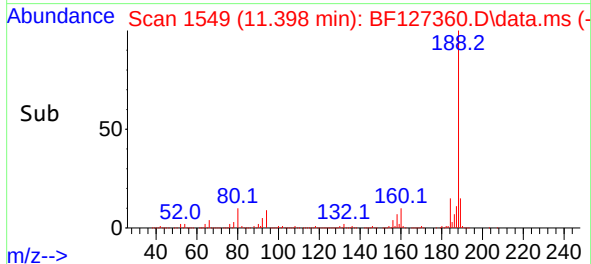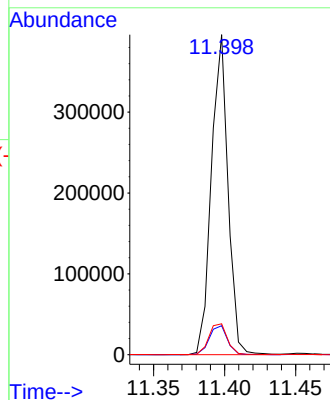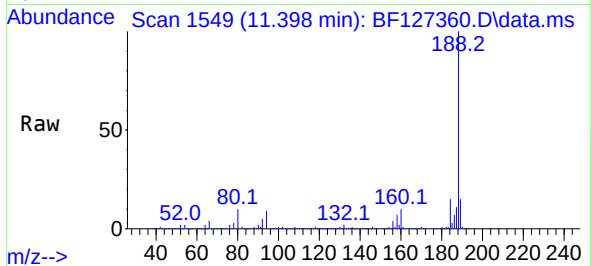

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.045 min Scan# 1999
Delta R.T. -0.006 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26


Tgt Ion:240 Resp: 219203
Ion Ratio Lower Upper
240 100
120 8.1 14.4 21.6#
236 24.6 20.5 30.7

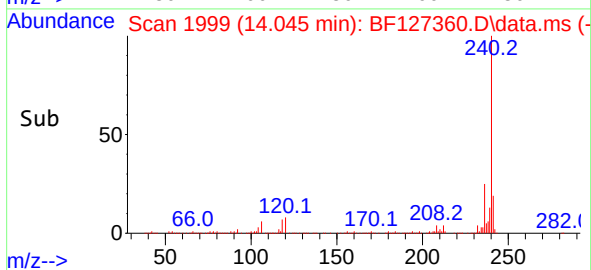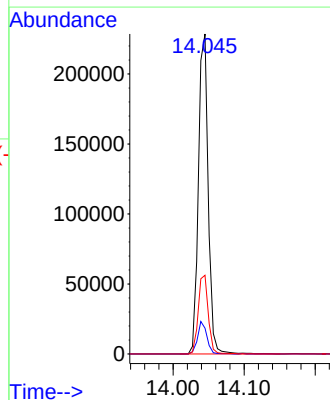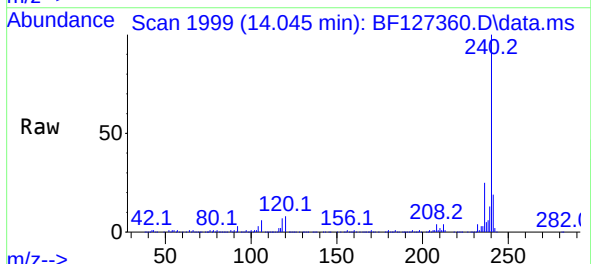



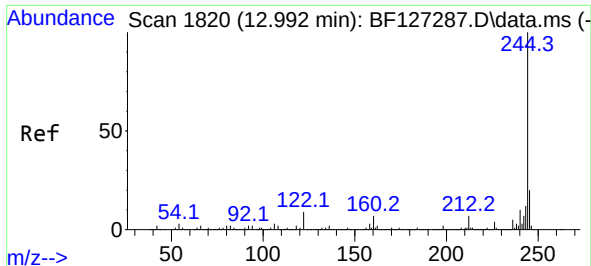


#79
Terphenyl-d14
Concen: 75.281 ng
RT: 12.986 min Scan# 1819
Delta R.T. -0.006 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26

Instrument :
BNA_F
ClientSampleId :
BLIND-DUPLICATE

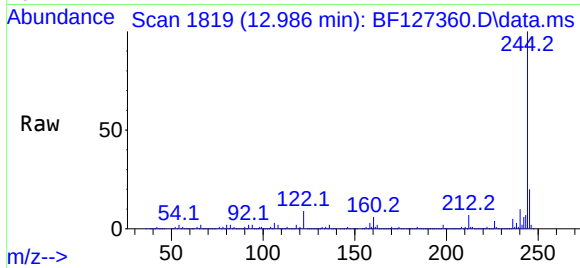

Tgt Ion:244 Resp: 958317
Ion Ratio Lower Upper
244 100
212 6.9 5.0 7.4
122 8.6 13.3 19.9#

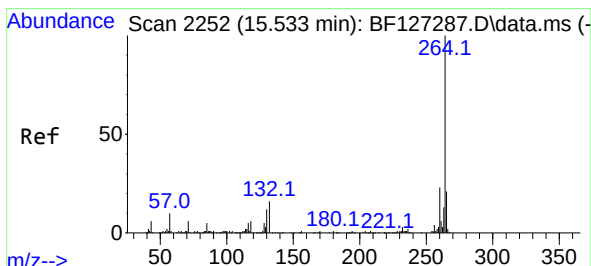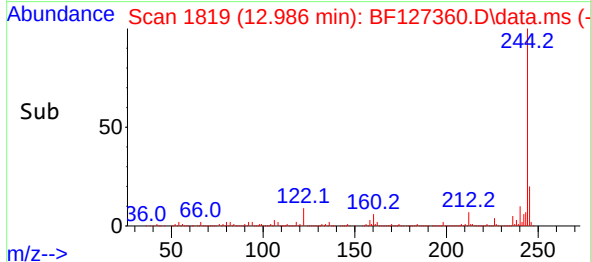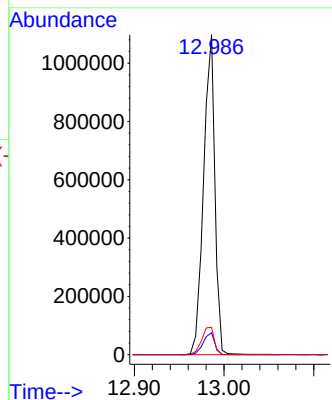

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.527 min Scan# 2251
Delta R.T. -0.006 min
Lab File: BF127360.D
Acq: 16 Mar 2022 21:26

Tgt Ion:264 Resp: 189639
Ion Ratio Lower Upper
264 100
260 23.9 19.2 28.8
265 21.7 17.4 26.2

