

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
 Data File : BF127353.D
 Acq On : 16 Mar 2022 18:01
 Operator : CG\JU
 Sample : N1951-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DB-8-(30-35)-3-12-22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	540	545	548	rBV	2323291	2065144	93.80%	14.424%
2	6.504	712	717	727	rBV	1911561	2037786	92.56%	14.233%
3	6.581	727	730	732	rVB	31674	24700	1.12%	0.173%
4	6.863	775	778	782	rBV	477049	374728	17.02%	2.617%
5	7.434	870	875	878	rBV	1484212	1355883	61.59%	9.470%
6	8.145	993	996	1000	rBV	561724	479877	21.80%	3.352%
7	9.228	1174	1180	1183	rBV	2352493	2201626	100.00%	15.378%
8	9.904	1291	1295	1299	rBV	638624	514731	23.38%	3.595%
9	10.216	1344	1348	1355	rBV4	12958	33173	1.51%	0.232%
10	10.698	1426	1430	1434	rBV	1487903	1477647	67.12%	10.321%
11	11.398	1545	1549	1552	rBV	729736	585451	26.59%	4.089%
12	11.916	1634	1637	1642	rVB4	34957	41303	1.88%	0.288%
13	12.486	1732	1734	1736	rVB3	29233	26164	1.19%	0.183%
14	12.986	1814	1819	1822	rVB	2450828	2123166	96.44%	14.830%
15	13.863	1965	1968	1971	rVB	24397	30133	1.37%	0.210%
16	13.904	1971	1975	1979	rVB	39651	41002	1.86%	0.286%
17	14.039	1995	1998	2003	rBV	446589	428876	19.48%	2.996%
18	14.133	2011	2014	2018	rVB	36209	35126	1.60%	0.245%
19	14.292	2036	2041	2050	rVB6	17297	45004	2.04%	0.314%
20	14.792	2121	2126	2131	rVB7	16818	32453	1.47%	0.227%
21	15.527	2246	2251	2256	rBV	290592	362966	16.49%	2.535%

Sum of corrected areas: 14316939

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127353.D
Acq On : 16 Mar 2022 18:01
Operator : CG\JU
Sample : N1951-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-8-(30-35)-3-12-22










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown14.292 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.292	2.10 ng	45004	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptadecane, 2,6,10,15-tetramethyl-	296	C21H44	054833-48-6	43
2			Decane, 6-ethyl-2-methyl-	184	C13H28	062108-21-8	43
3			Undecane, 5-ethyl-5-propyl-	226	C16H34	002755-07-9	43
4			Oxalic acid, 6-ethyloct-3-yl pro...	272	C15H28O4	1000309-34-0	43
5			Sulfurous acid, butyl decyl ester	278	C14H30O3S	1000309-17-7	43

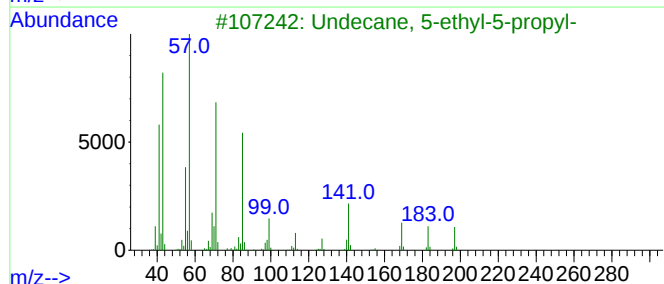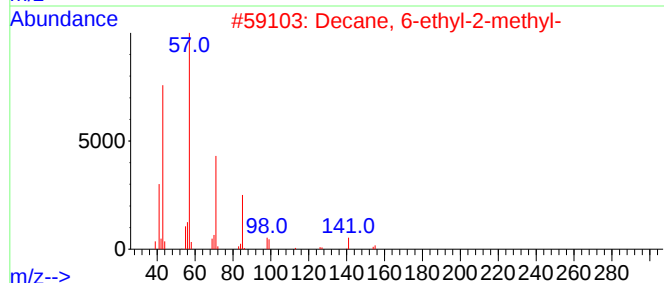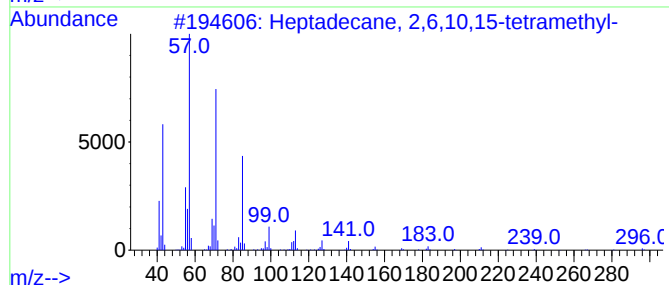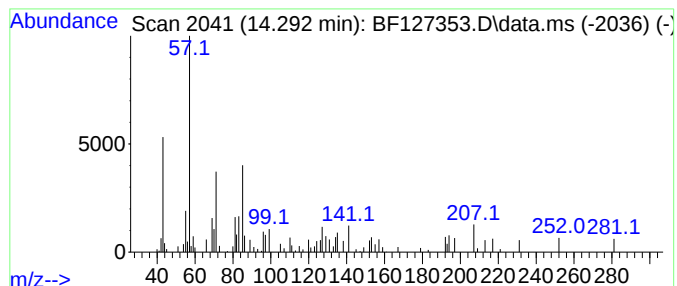

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127353.D
Acq On : 16 Mar 2022 18:01
Operator : CG\JU
Sample : N1951-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-8-(30-35)-3-12-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown14.292	14.292	2.1	ng	45004	5	14.045	428876	20.0