

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
 Data File : BF127358.D
 Acq On : 16 Mar 2022 20:27
 Operator : CG\JU
 Sample : N1951-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DB-15-(20-25)-3-12-22

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	540	544	562	rBV	1981853	1839327	89.29%	12.779%
2	6.498	712	716	719	rBV	2055013	1844075	89.52%	12.812%
3	6.863	775	778	782	rBV	633873	527784	25.62%	3.667%
4	7.434	870	875	878	rBV	1332742	1245869	60.48%	8.656%
5	8.145	993	996	1000	rBV	758436	674188	32.73%	4.684%
6	9.222	1175	1179	1182	rBV	2398195	2059955	100.00%	14.312%
7	9.904	1292	1295	1304	rVB	1030371	799375	38.81%	5.554%
8	10.698	1426	1430	1444	rBV	1535780	1386458	67.31%	9.633%
9	11.398	1545	1549	1552	rBV	989232	841698	40.86%	5.848%
10	12.980	1814	1818	1822	rBV	2168235	1986318	96.43%	13.800%
11	13.957	1977	1984	1986	rBV6	14636	31676	1.54%	0.220%
12	14.045	1995	1999	2012	rVB	616169	611105	29.67%	4.246%
13	15.527	2246	2251	2261	rBV	412637	545324	26.47%	3.789%




Sum of corrected areas: 14393152

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127358.D
Acq On : 16 Mar 2022 20:27
Operator : CG\JU
Sample : N1951-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-15-(20-25)-3-12-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

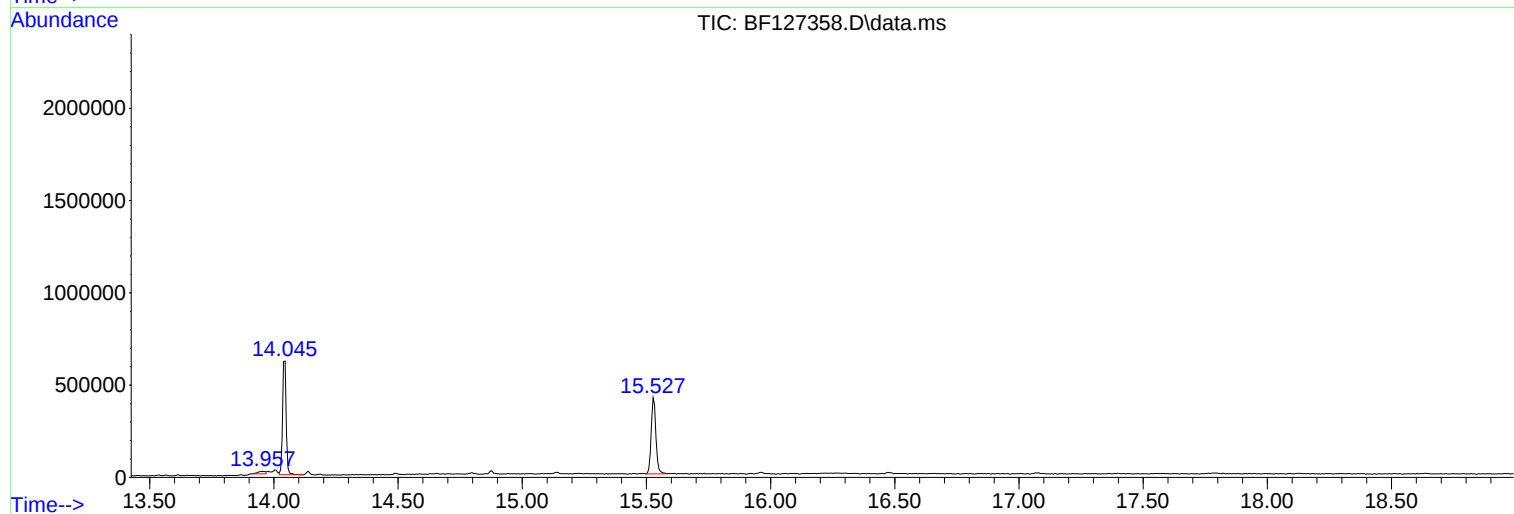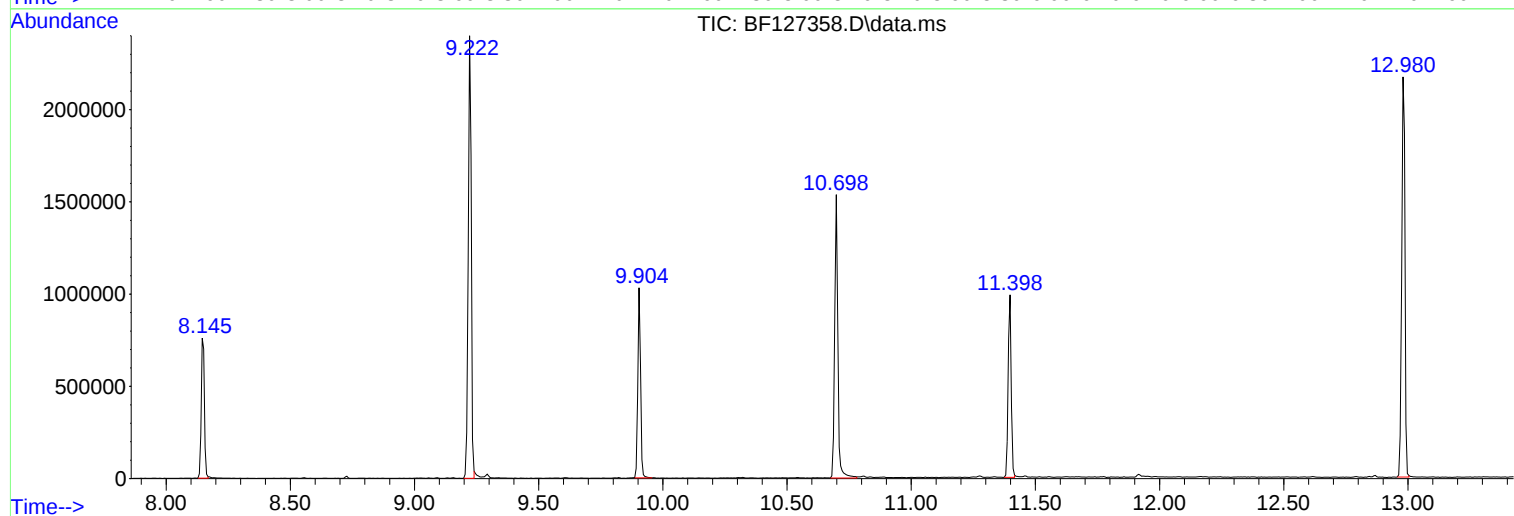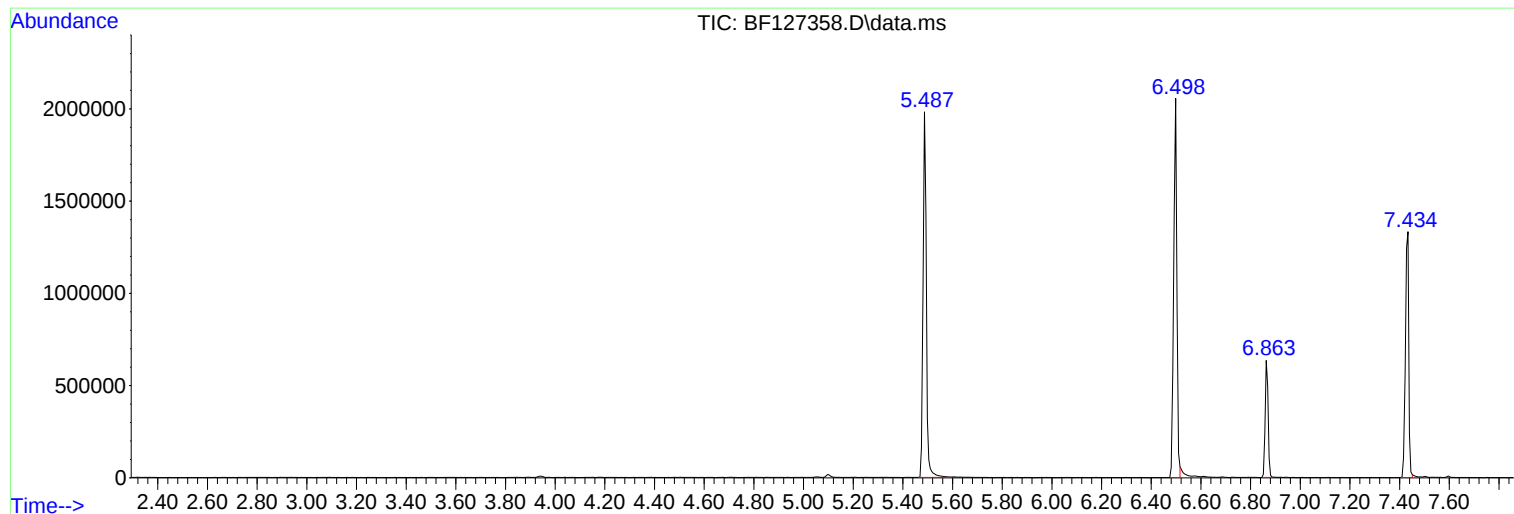

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127358.D
Acq On : 16 Mar 2022 20:27
Operator : CG\JU
Sample : N1951-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-15-(20-25)-3-12-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127358.D
Acq On : 16 Mar 2022 20:27
Operator : CG\JU
Sample : N1951-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-15-(20-25)-3-12-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------