

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
 Data File : BF127364.D
 Acq On : 16 Mar 2022 23:21
 Operator : CG\JU
 Sample : N1951-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DB-14-(20-25)-3-12-22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	540	544	561	rBV	1882510	1815250	90.94%	14.447%
2	6.498	712	716	719	rBV	1854538	1697269	85.03%	13.508%
3	6.863	775	778	782	rBV	484758	398050	19.94%	3.168%
4	7.434	870	875	878	rBV	1218181	1124086	56.32%	8.947%
5	8.145	993	996	1000	rBV	538764	484801	24.29%	3.858%
6	9.222	1175	1179	1182	rBV	2382373	1996056	100.00%	15.886%
7	9.904	1292	1295	1299	rBV	739283	599559	30.04%	4.772%
8	10.698	1426	1430	1442	rBV	1431091	1273733	63.81%	10.138%
9	11.398	1545	1549	1557	rBV	784130	664055	33.27%	5.285%
10	12.980	1814	1818	1821	rBV	1907416	1656075	82.97%	13.181%
11	14.039	1995	1998	2004	rVB	478650	455754	22.83%	3.627%
12	15.527	2246	2251	2260	rBV2	310086	399843	20.03%	3.182%




Sum of corrected areas: 12564531

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127364.D
Acq On : 16 Mar 2022 23:21
Operator : CG\JU
Sample : N1951-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-14-(20-25)-3-12-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

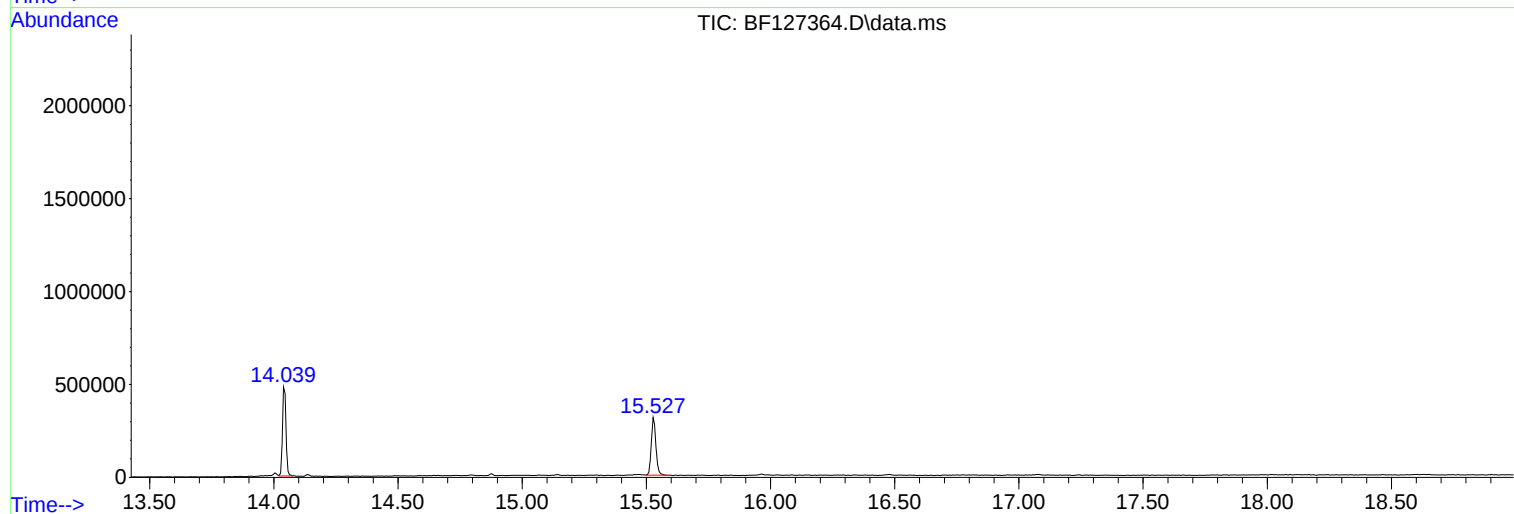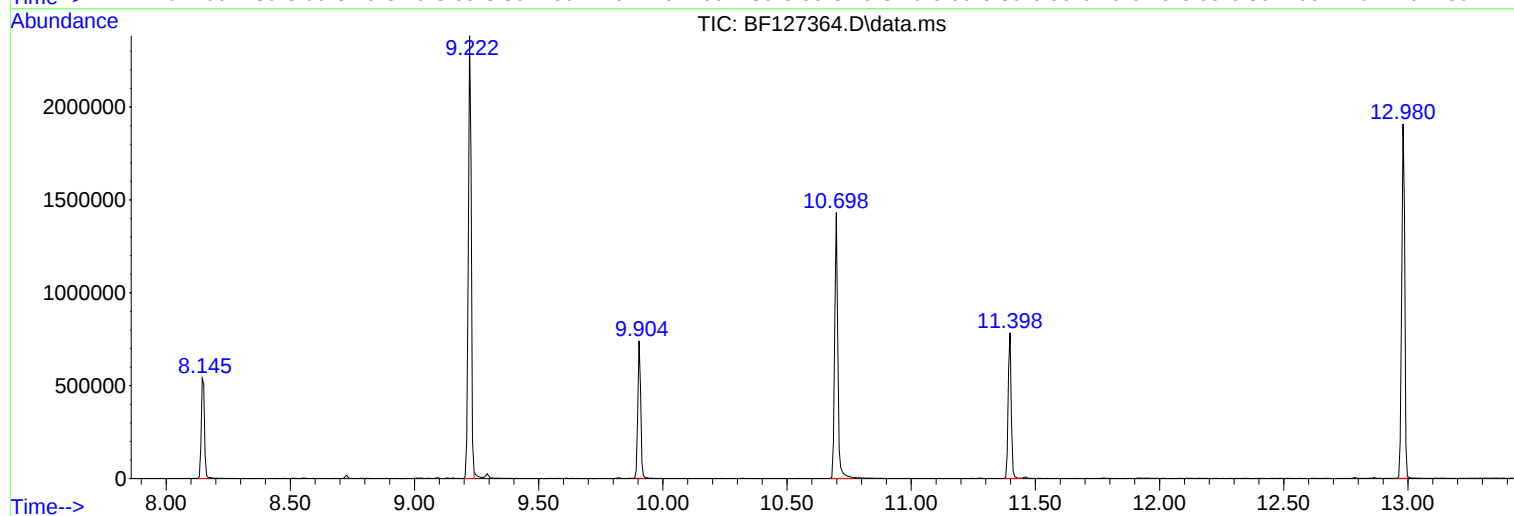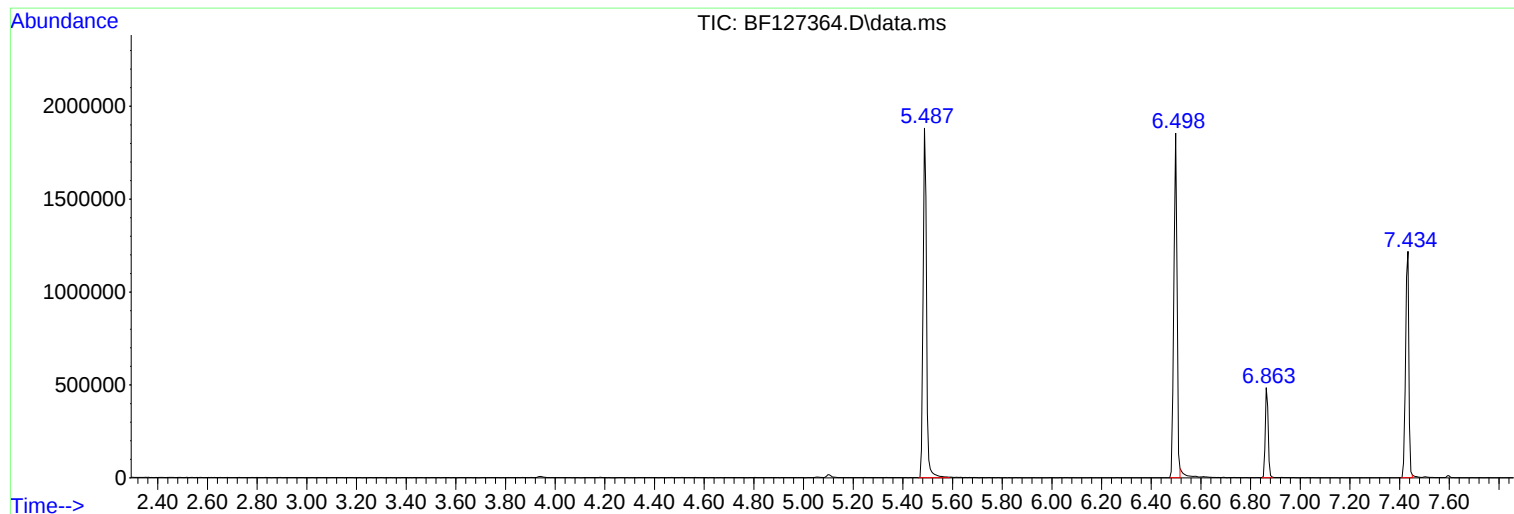

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127364.D
Acq On : 16 Mar 2022 23:21
Operator : CG\JU
Sample : N1951-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-14-(20-25)-3-12-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127364.D
Acq On : 16 Mar 2022 23:21
Operator : CG\JU
Sample : N1951-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DB-14-(20-25)-3-12-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------