
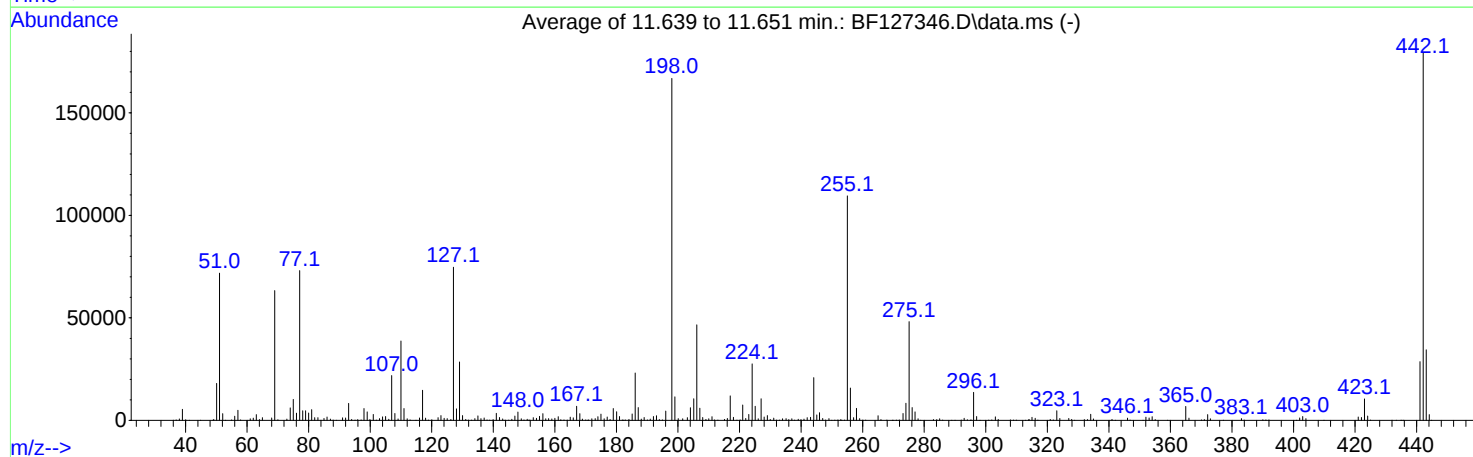


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
 Data File : BF127346.D
 Acq On : 16 Mar 2022 12:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 10 16:51:53 2022

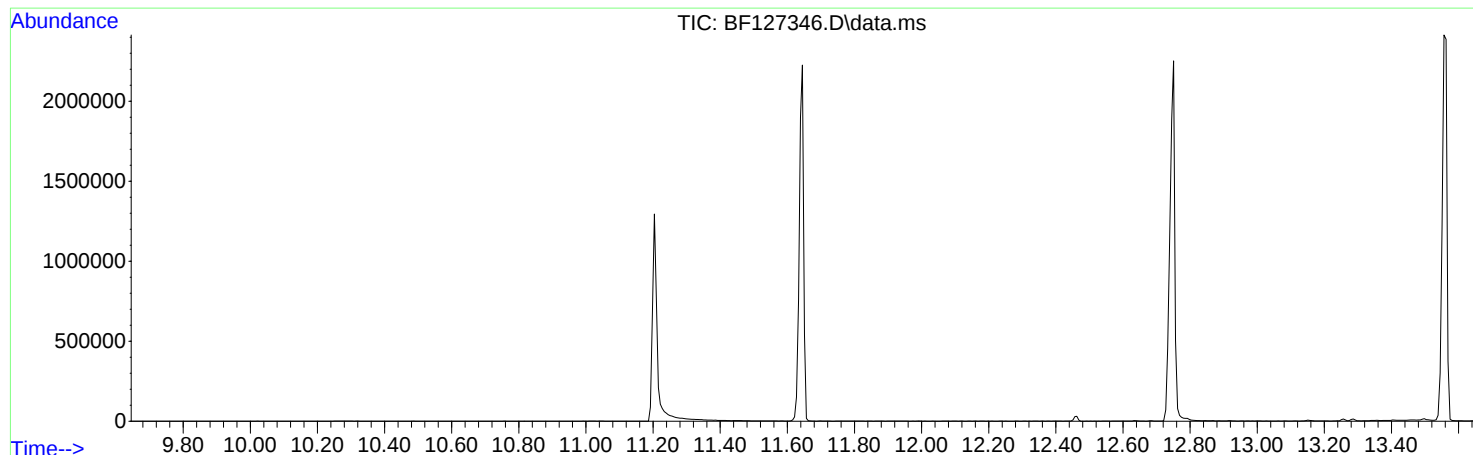




AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	71824	PASS
68	69	0.00	2	1.8	1158	PASS
69	198	0.00	100	37.9	63284	PASS
70	69	0.00	2	0.5	286	PASS
127	198	10	80	44.8	74685	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	166832	PASS
199	198	5	9	6.9	11466	PASS
275	198	10	60	28.9	48163	PASS
365	198	1	100	4.1	6773	PASS
441	198	0.01	100	17.2	28629	PASS
442	442	50	100	100.0	179453	PASS
443	442	15	24	19.2	34397	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\
Data File : BF127346.D
Acq On : 16 Mar 2022 12:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 17 04:07:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

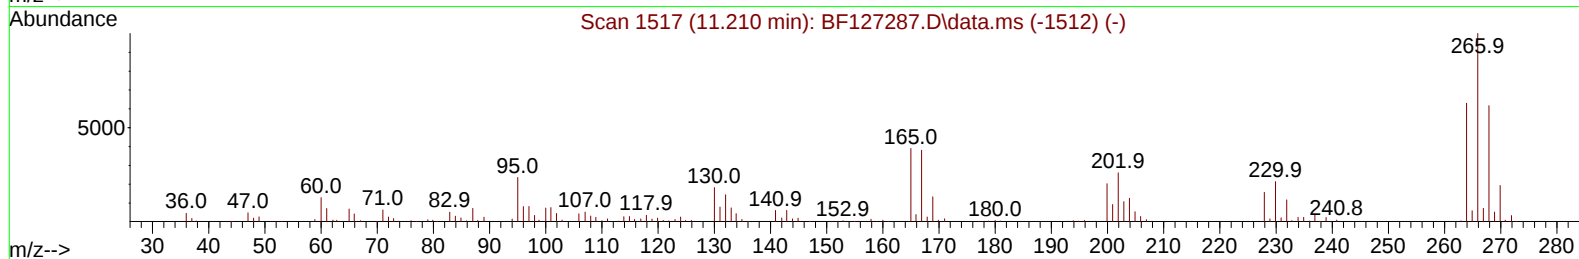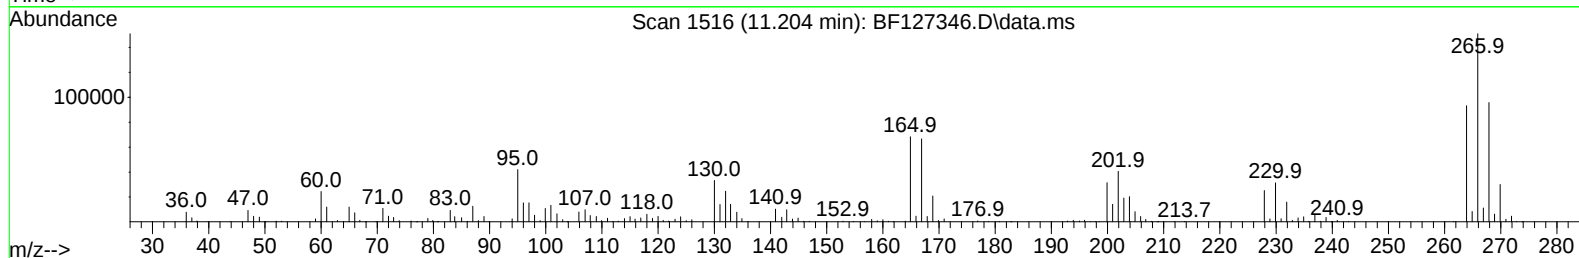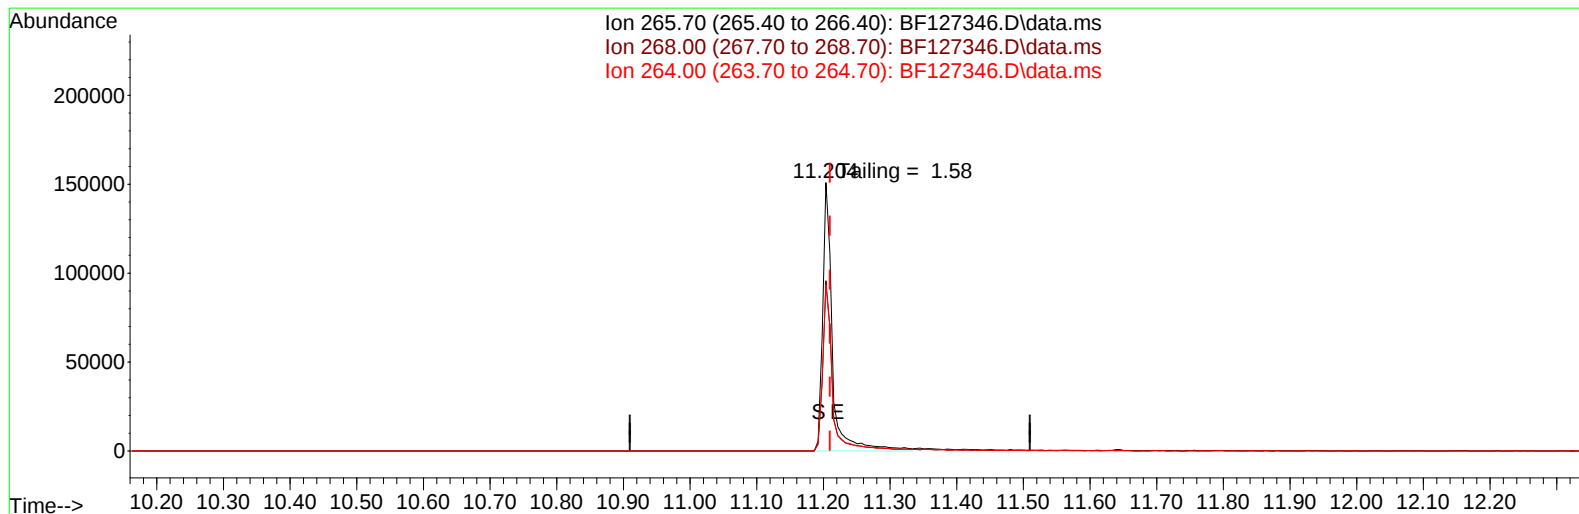

TIC: BF127346.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 35060.17 ng




response 154168

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	63.42
264.00	63.00	61.77
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031622\  
Data File : BF127346.D  
Acq On    : 16 Mar 2022  12:22  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 17 04:07:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

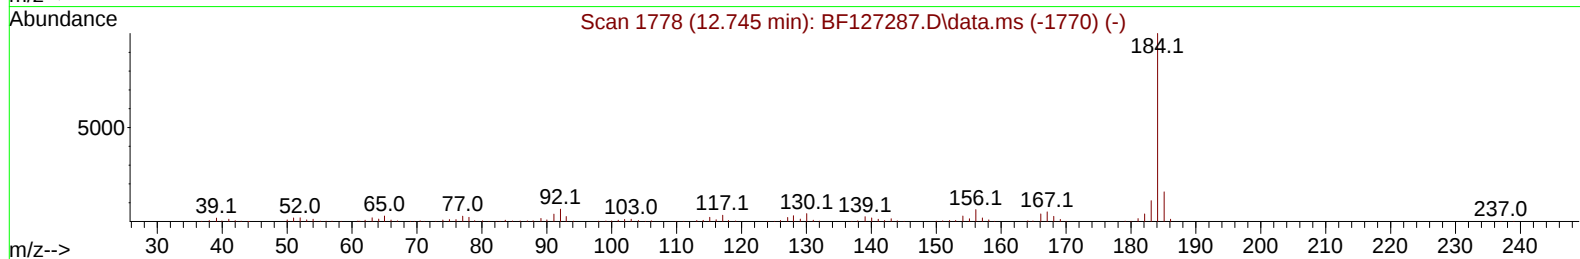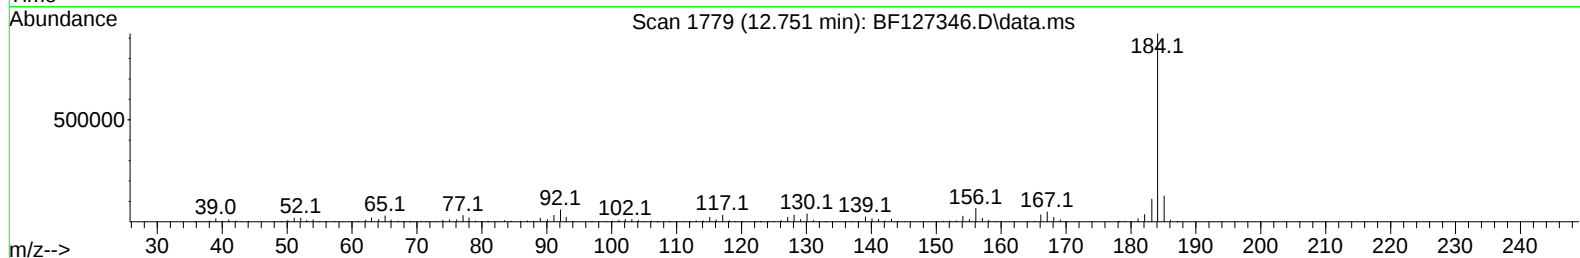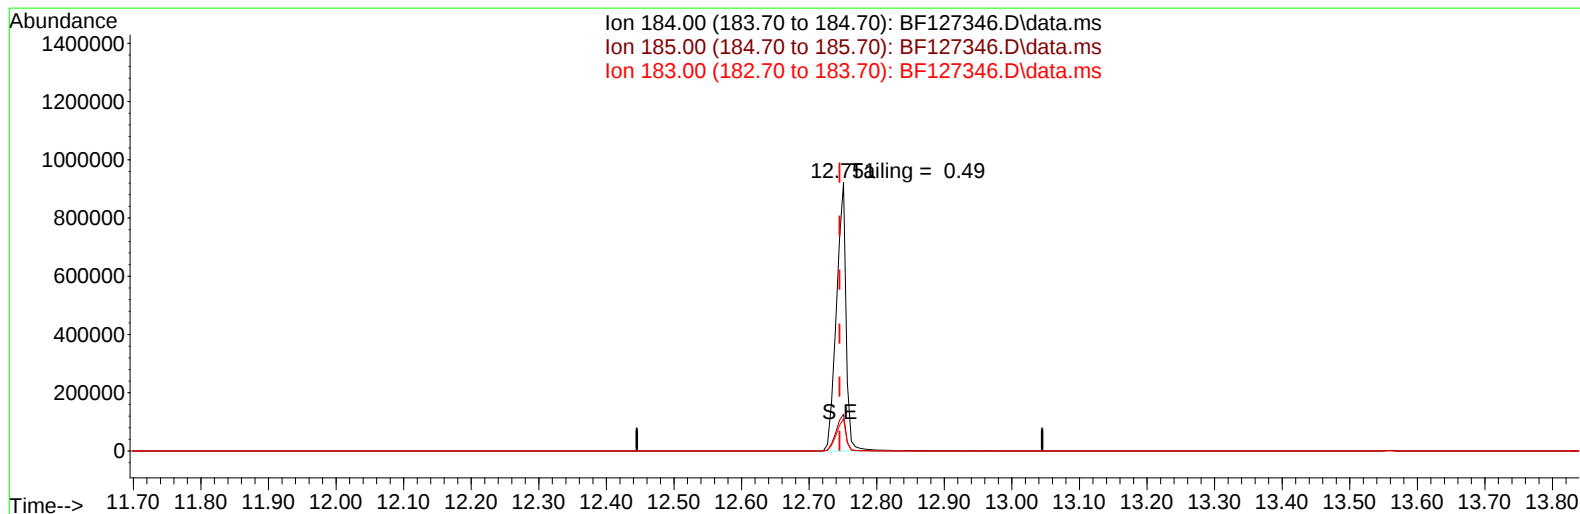

TIC: BF127346.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response **914569**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.72
183.00	10.20	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/16/2022	BNA_F	<u>BF127346.D</u>
Compound Name	Response	Retention Time
DDT	475793	13.562
DDD	5731	13.257
DDE	300	12.915
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6031	481824	1.25

Instrument :
BNA_F
ClientSampleId :
DFTPP