


Benzaldehyde


Response Ratio

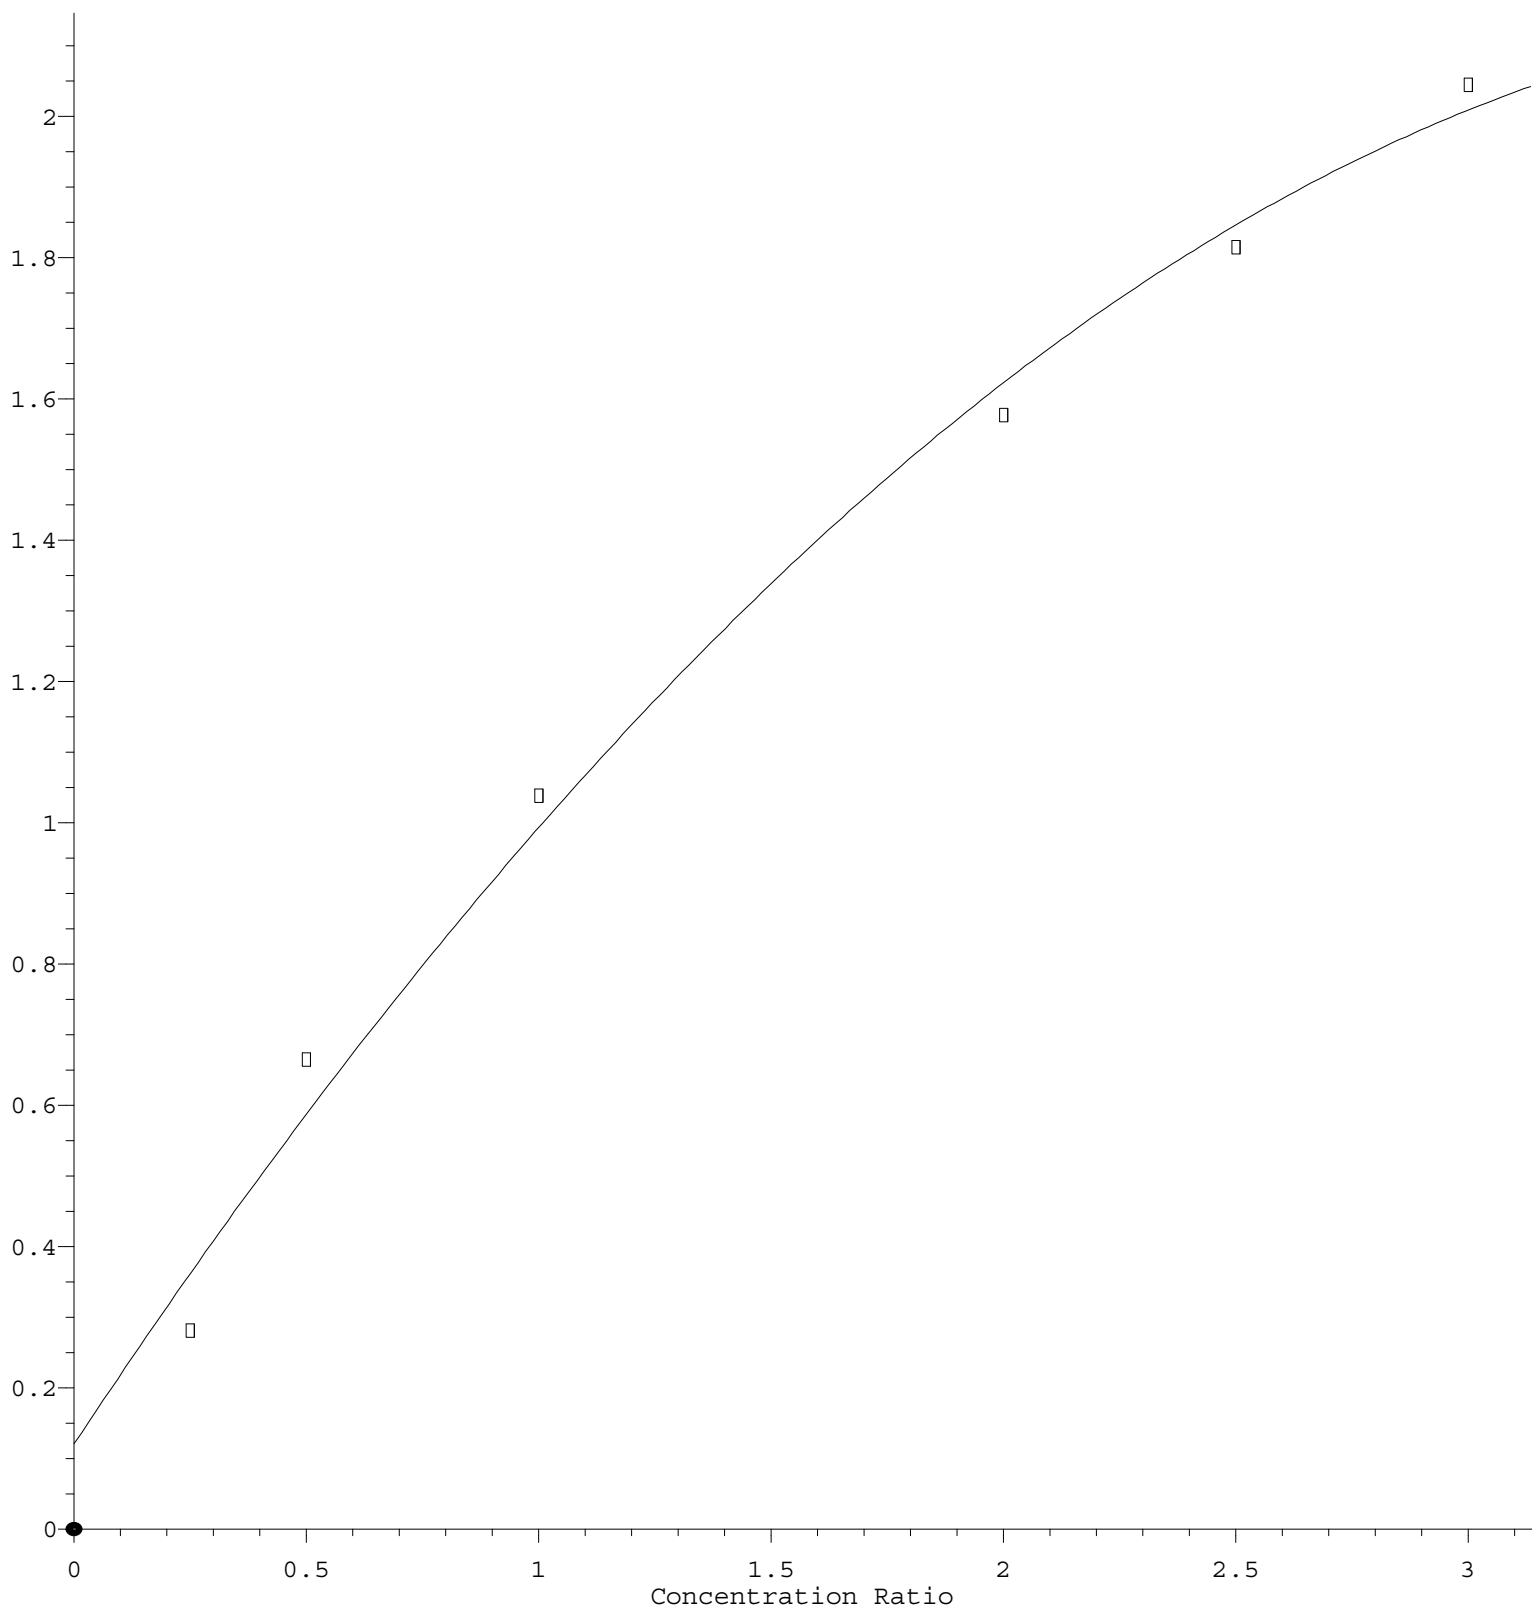

$R = -1.217e-001 A^2 + 9.944e-001 A + 1.206e-001$
Coef of Det (r^2) = 0.992100 Curve Fit: Quadratic
Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031721.M
Calibration Table Last Updated: Thu Mar 18 02:38:45 2021

Phenol


Response Ratio

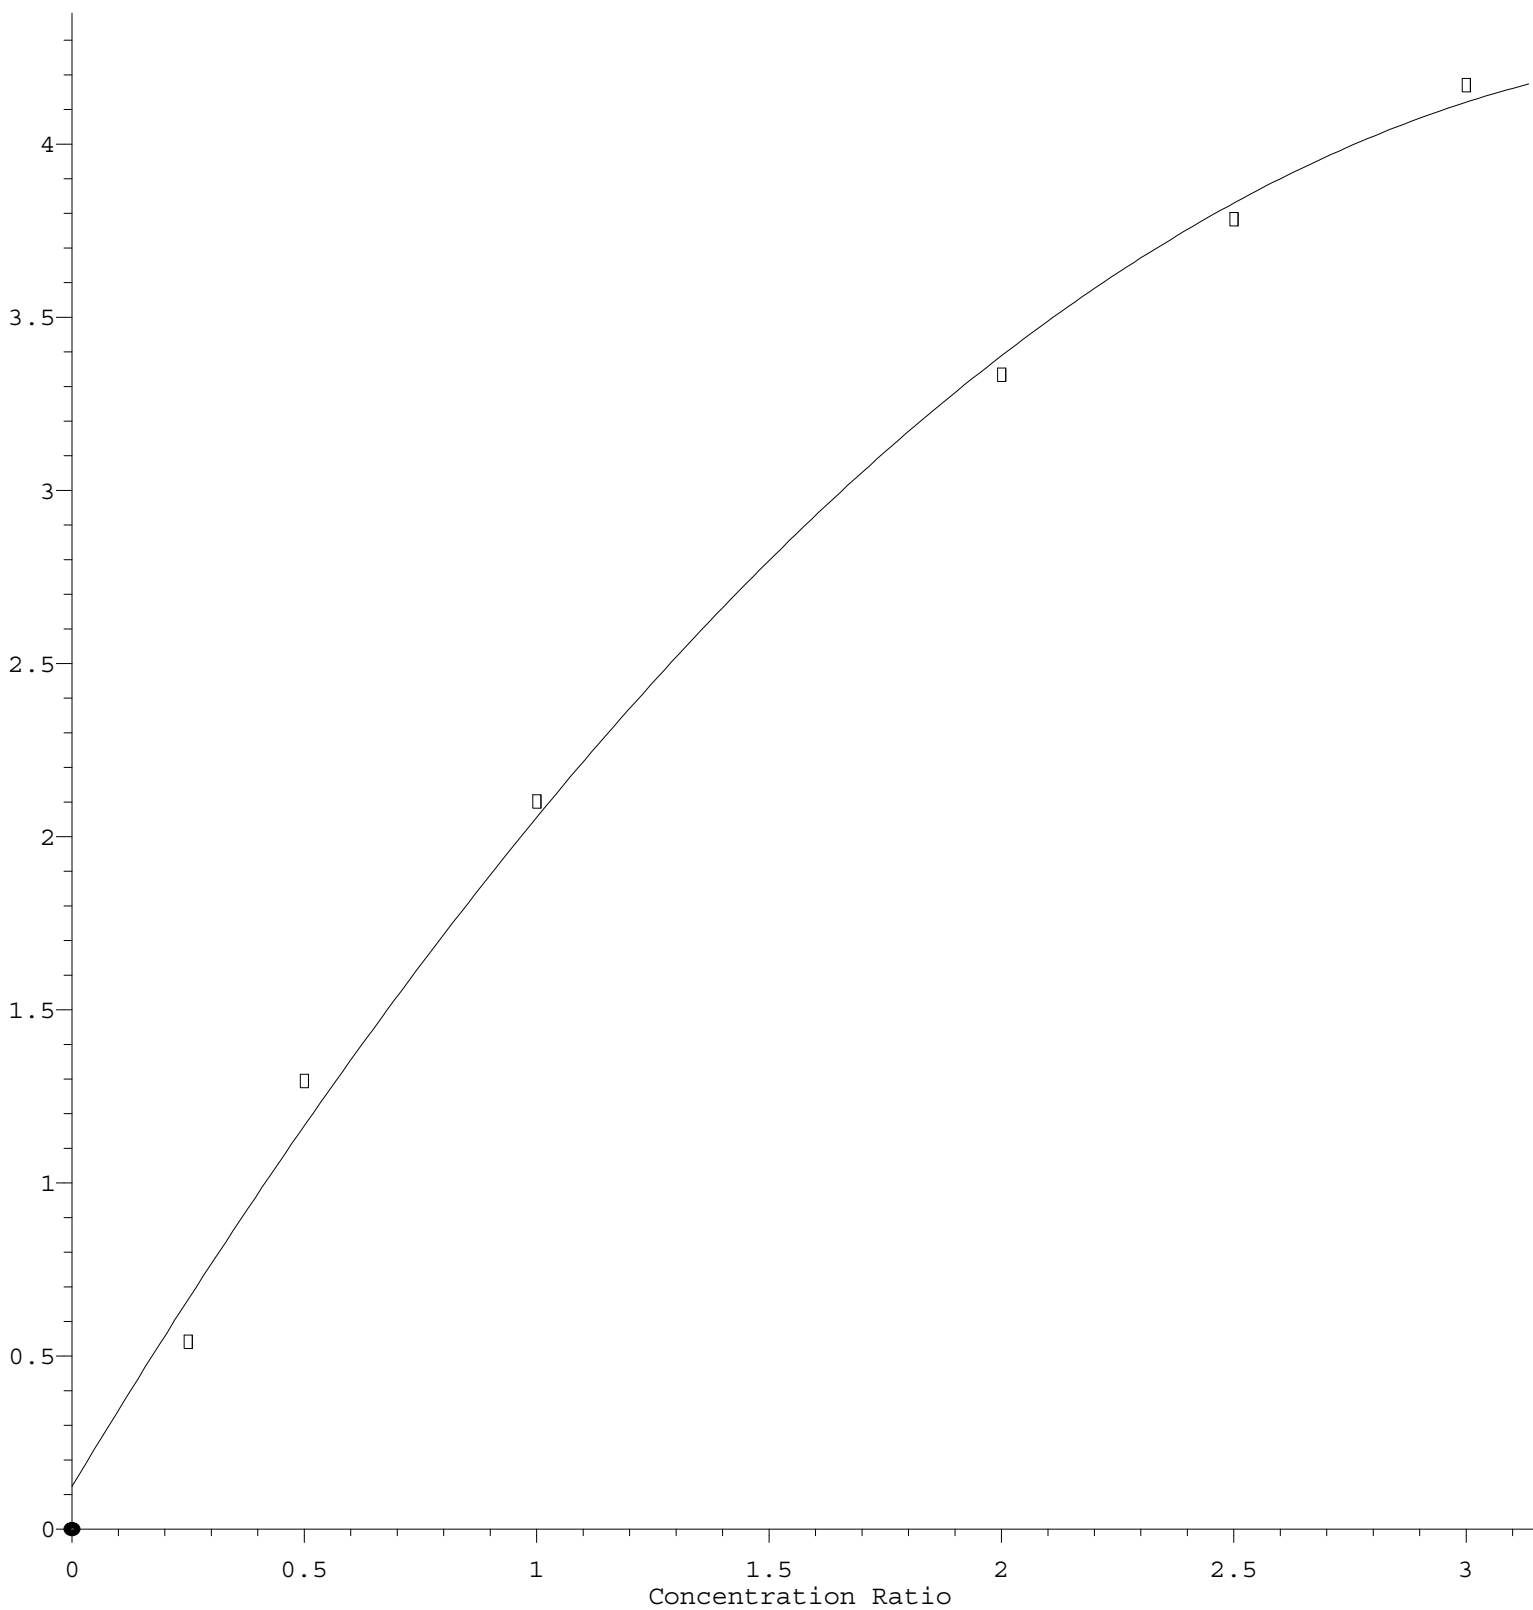

$R = -2.999e-001 A^2 + 2.232e+000 A + 1.239e-001$
 Coef of Det (r^2) = 0.996097 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031721.M
 Calibration Table Last Updated: Thu Mar 18 02:38:45 2021

3+4-Methylphenols


Response Ratio

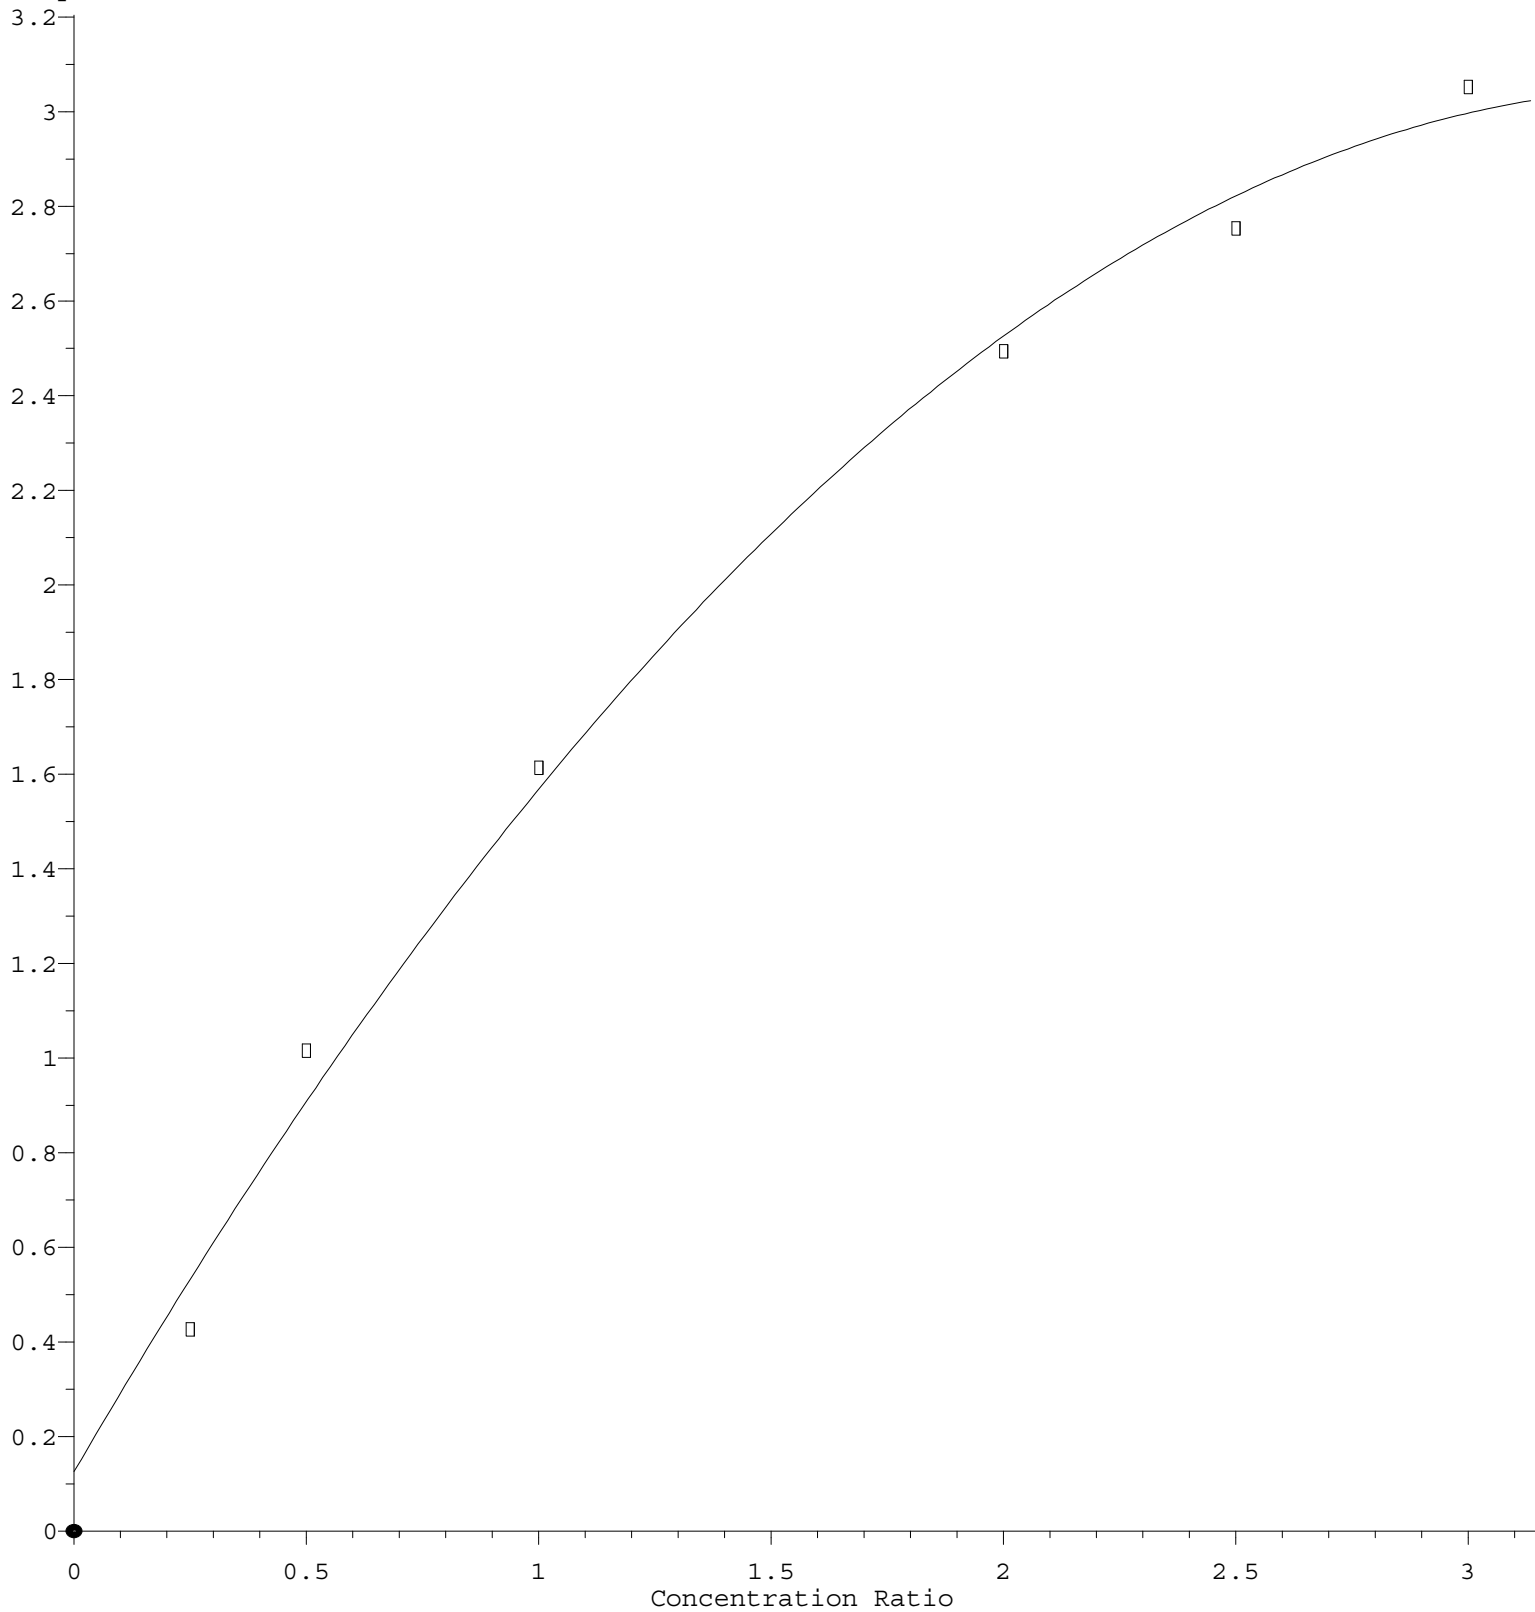

$R = -2.429e-001 A^2 + 1.686e+000 A + 1.259e-001$
 Coef of Det (r^2) = 0.993841 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031721.M
 Calibration Table Last Updated: Thu Mar 18 02:38:45 2021

2-Fluorobiphenyl

Response Ratio

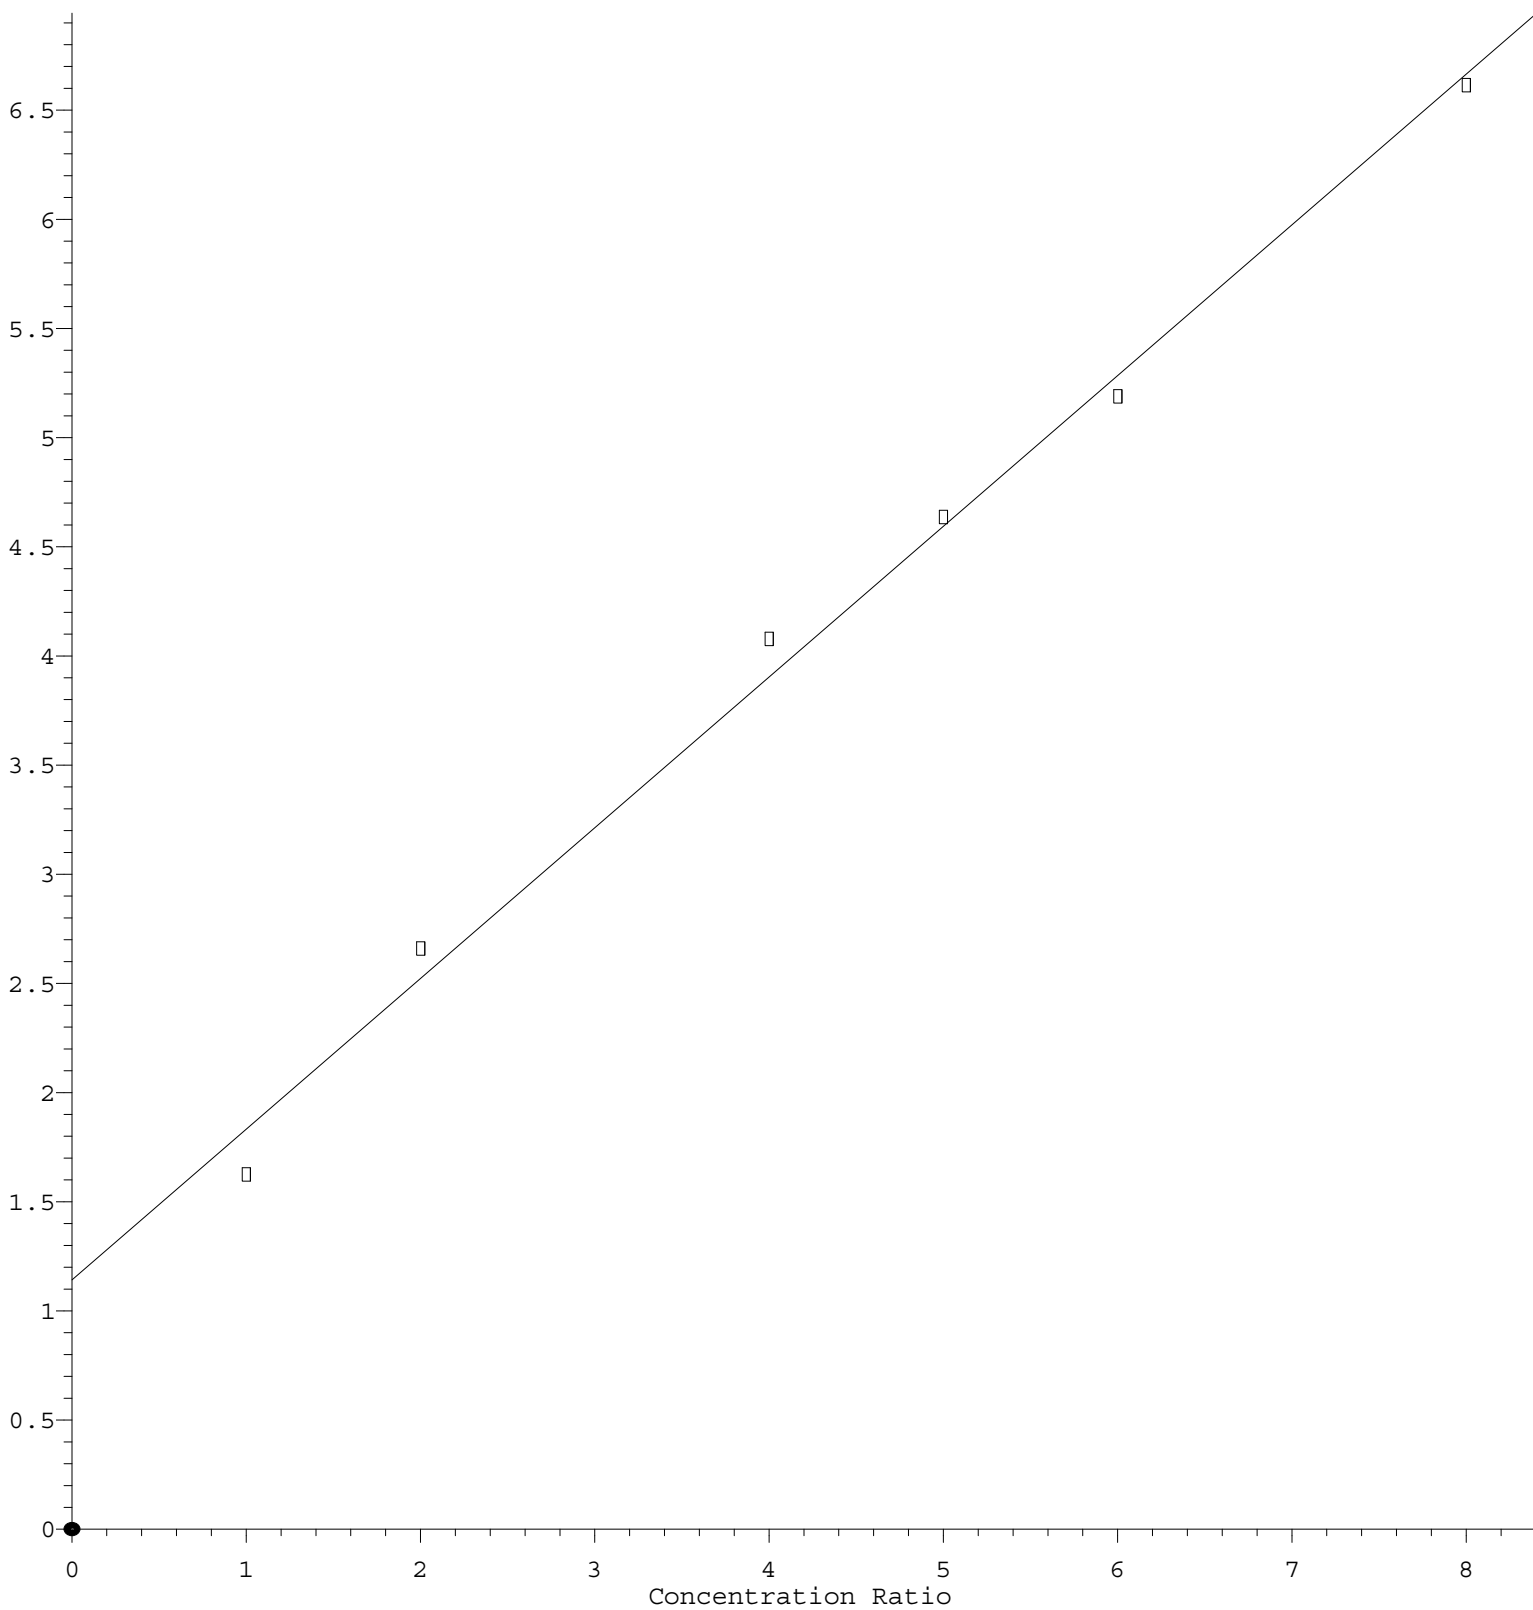

$$\text{Response} = 6.903\text{e-}001 * \text{Amt} + 1.142\text{e+}000$$


Coef of Det (r^2) = 0.993390 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031721.M

Calibration Table Last Updated: Thu Mar 18 02:38:45 2021

Dibenzofuran


Response Ratio

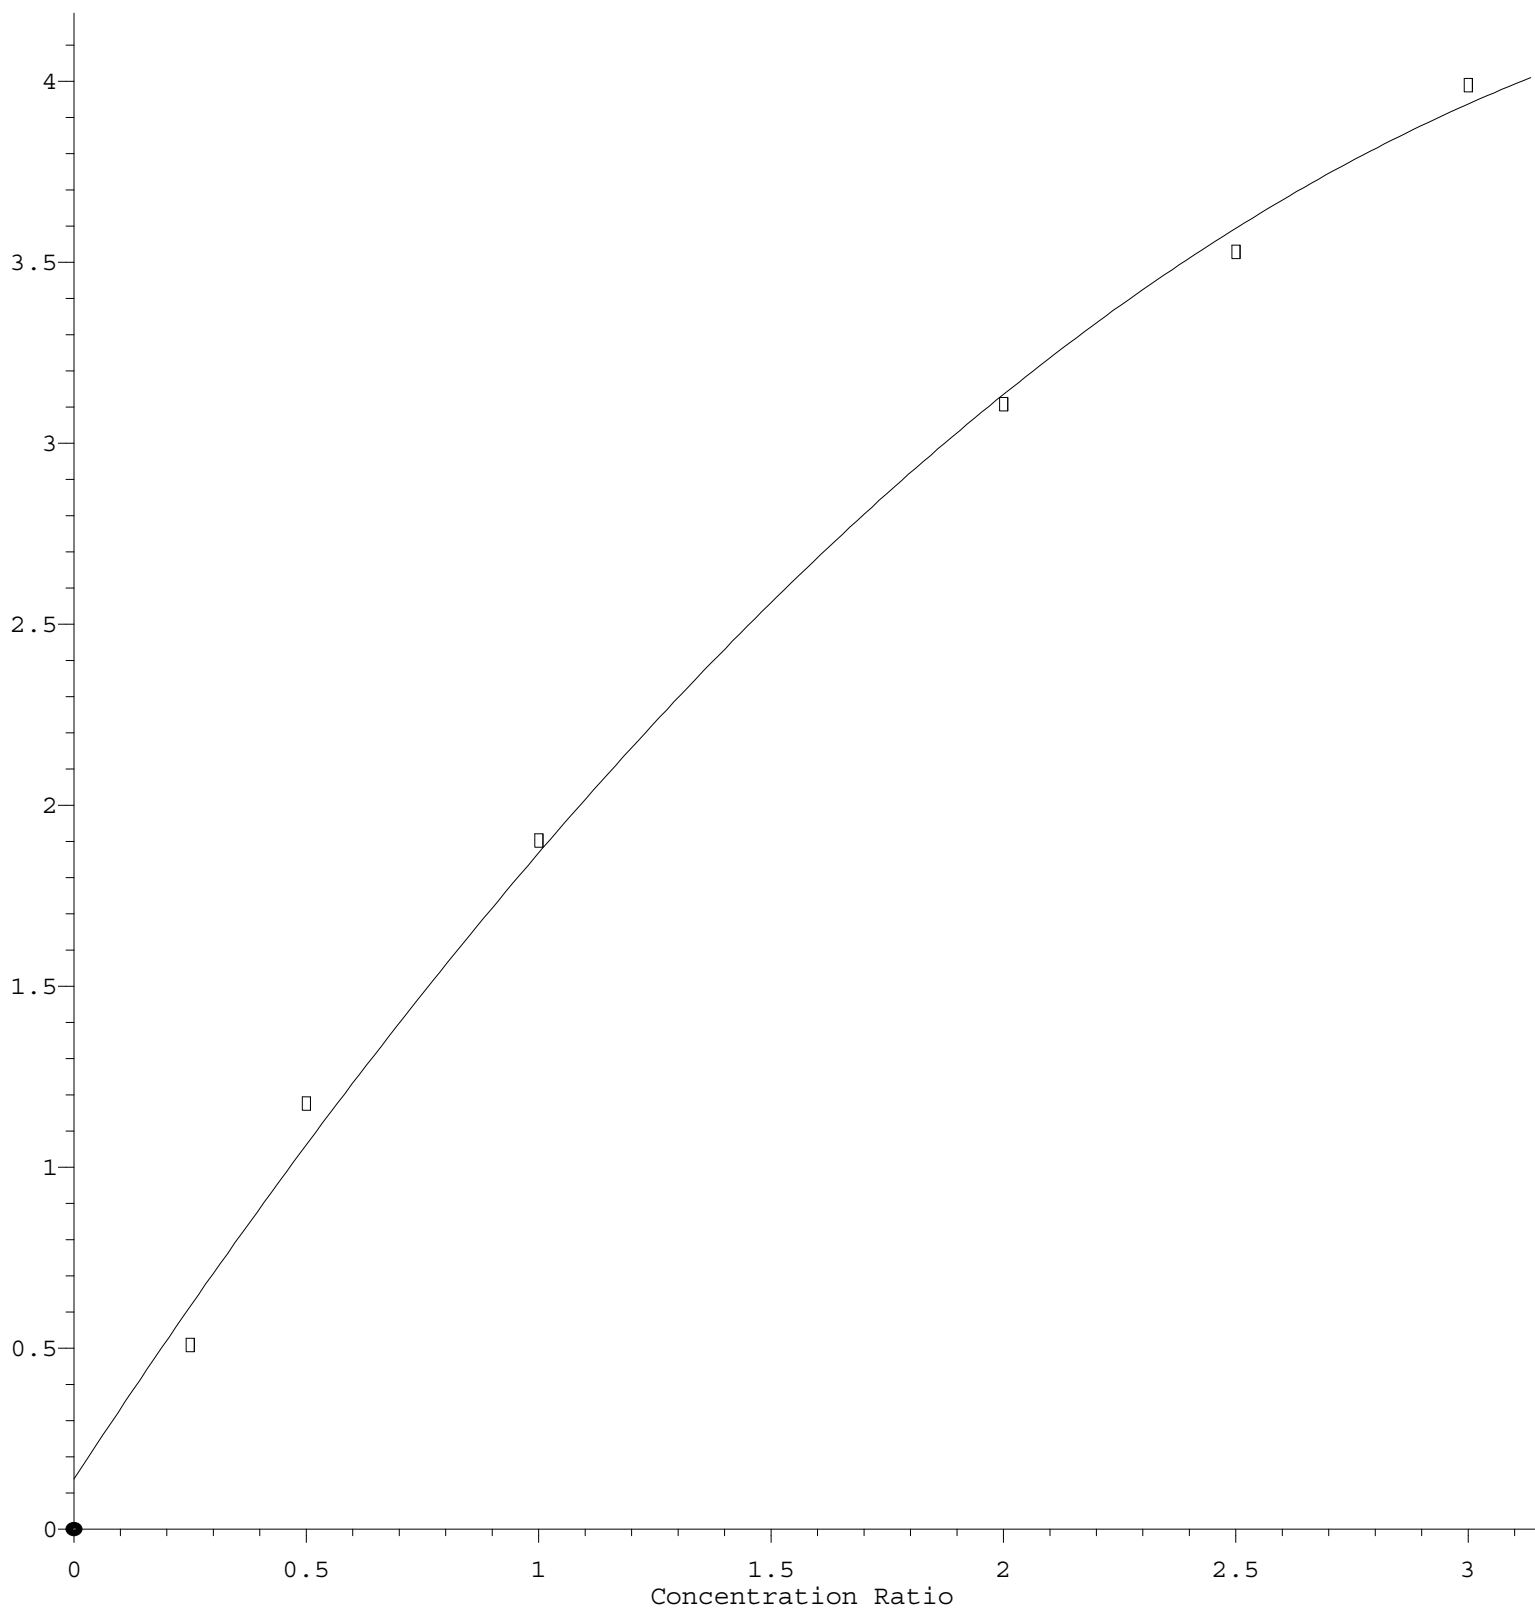

$R = -2.318e-001 A^2 + 1.961e+000 A + 1.391e-001$
 Coef of Det (r^2) = 0.996552 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031721.M
 Calibration Table Last Updated: Thu Mar 18 02:38:45 2021

Fluorene


Response Ratio

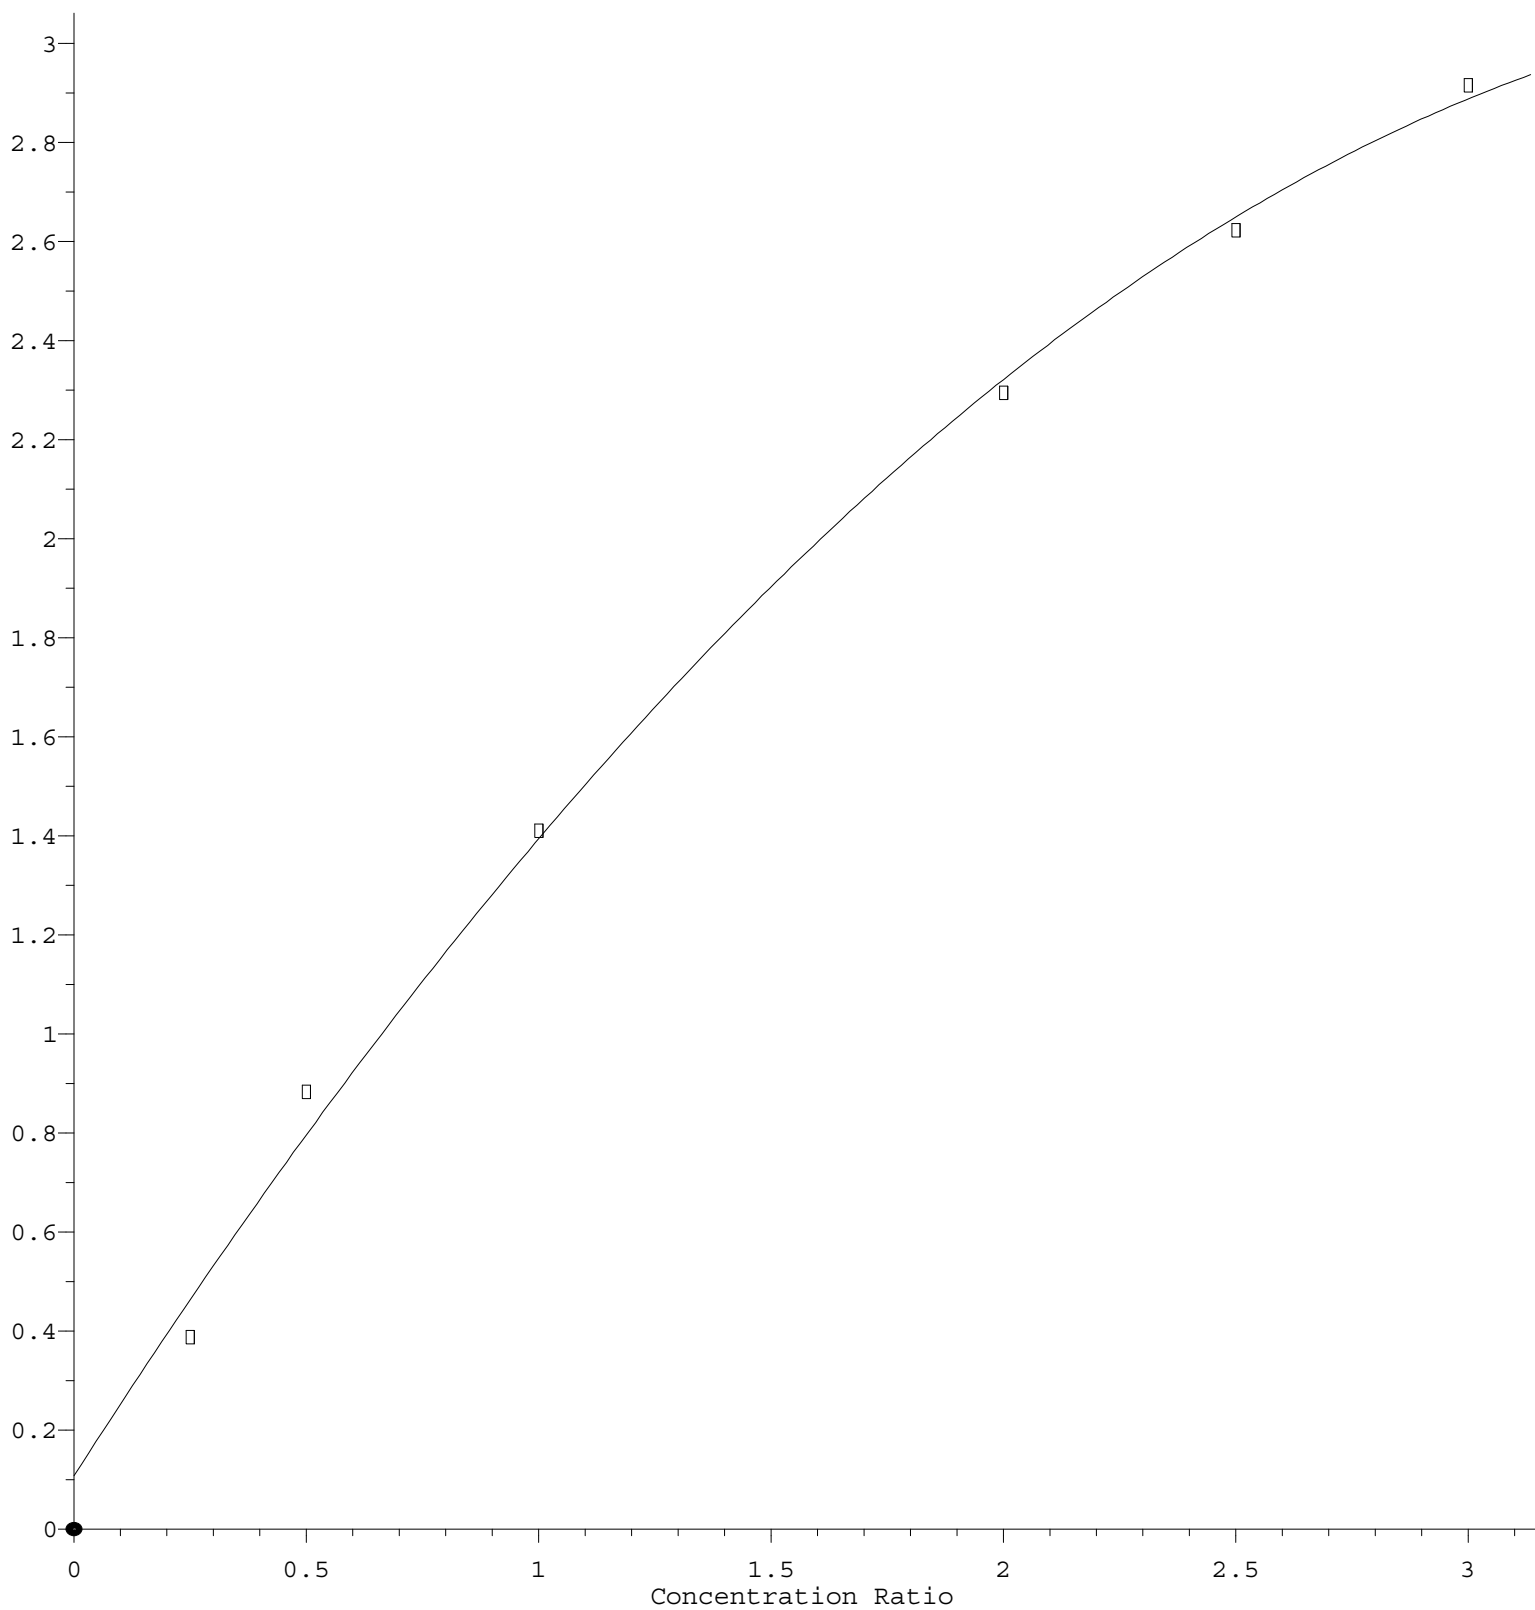

$R = -1.799e-001 A^2 + 1.467e+000 A + 1.078e-001$
 Coef of Det (r^2) = 0.996947 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031721.M
 Calibration Table Last Updated: Thu Mar 18 02:38:45 2021

4-Chlorophenyl-phenylether


Response Ratio

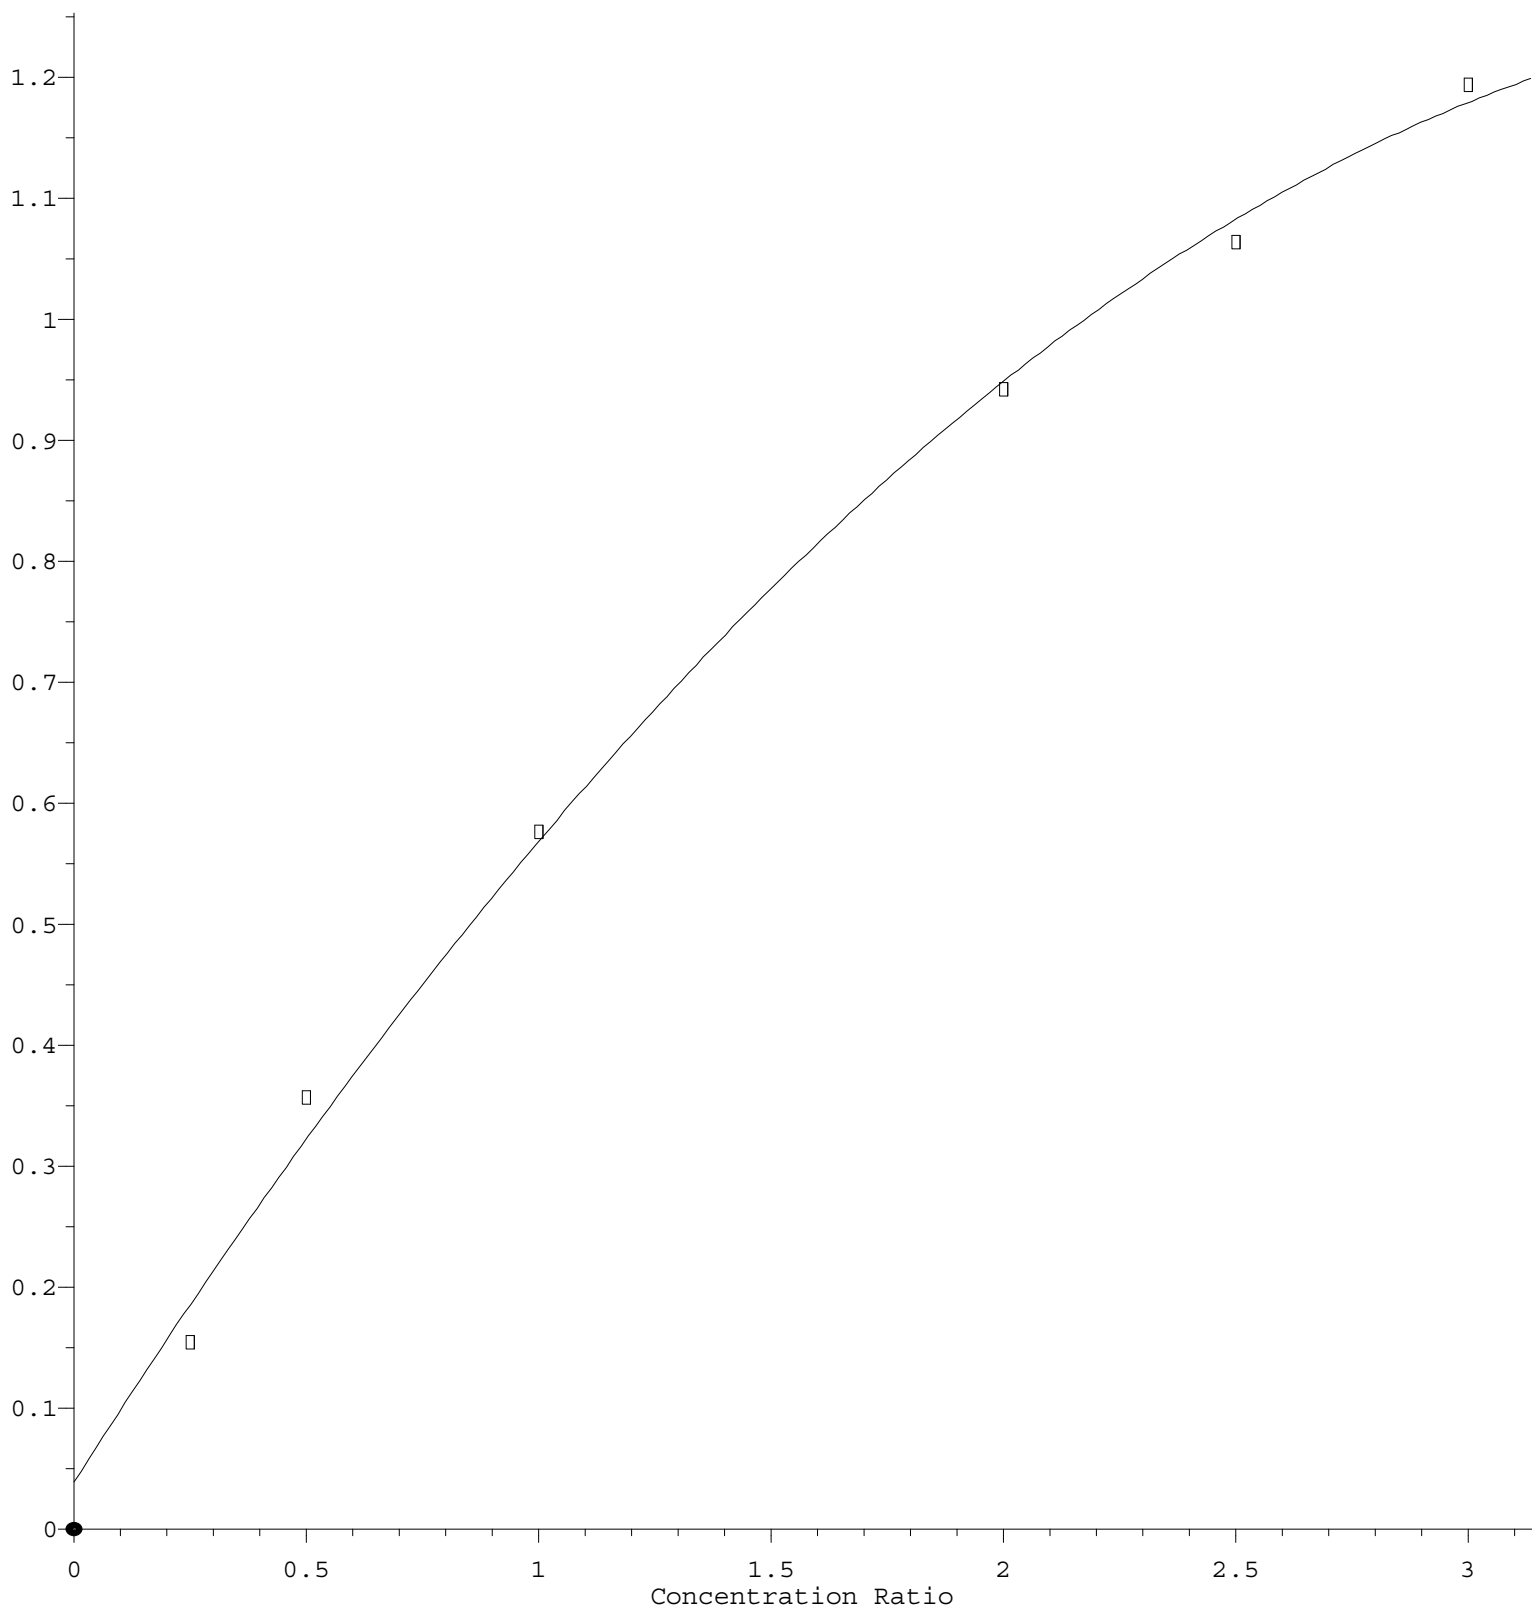

$R = -7.484e-002 A^2 + 6.046e-001 A + 3.884e-002$
Coef of Det (r^2) = 0.996759 Curve Fit: Quadratic
Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031721.M
Calibration Table Last Updated: Thu Mar 18 02:38:45 2021

Fluoranthene

Response Ratio

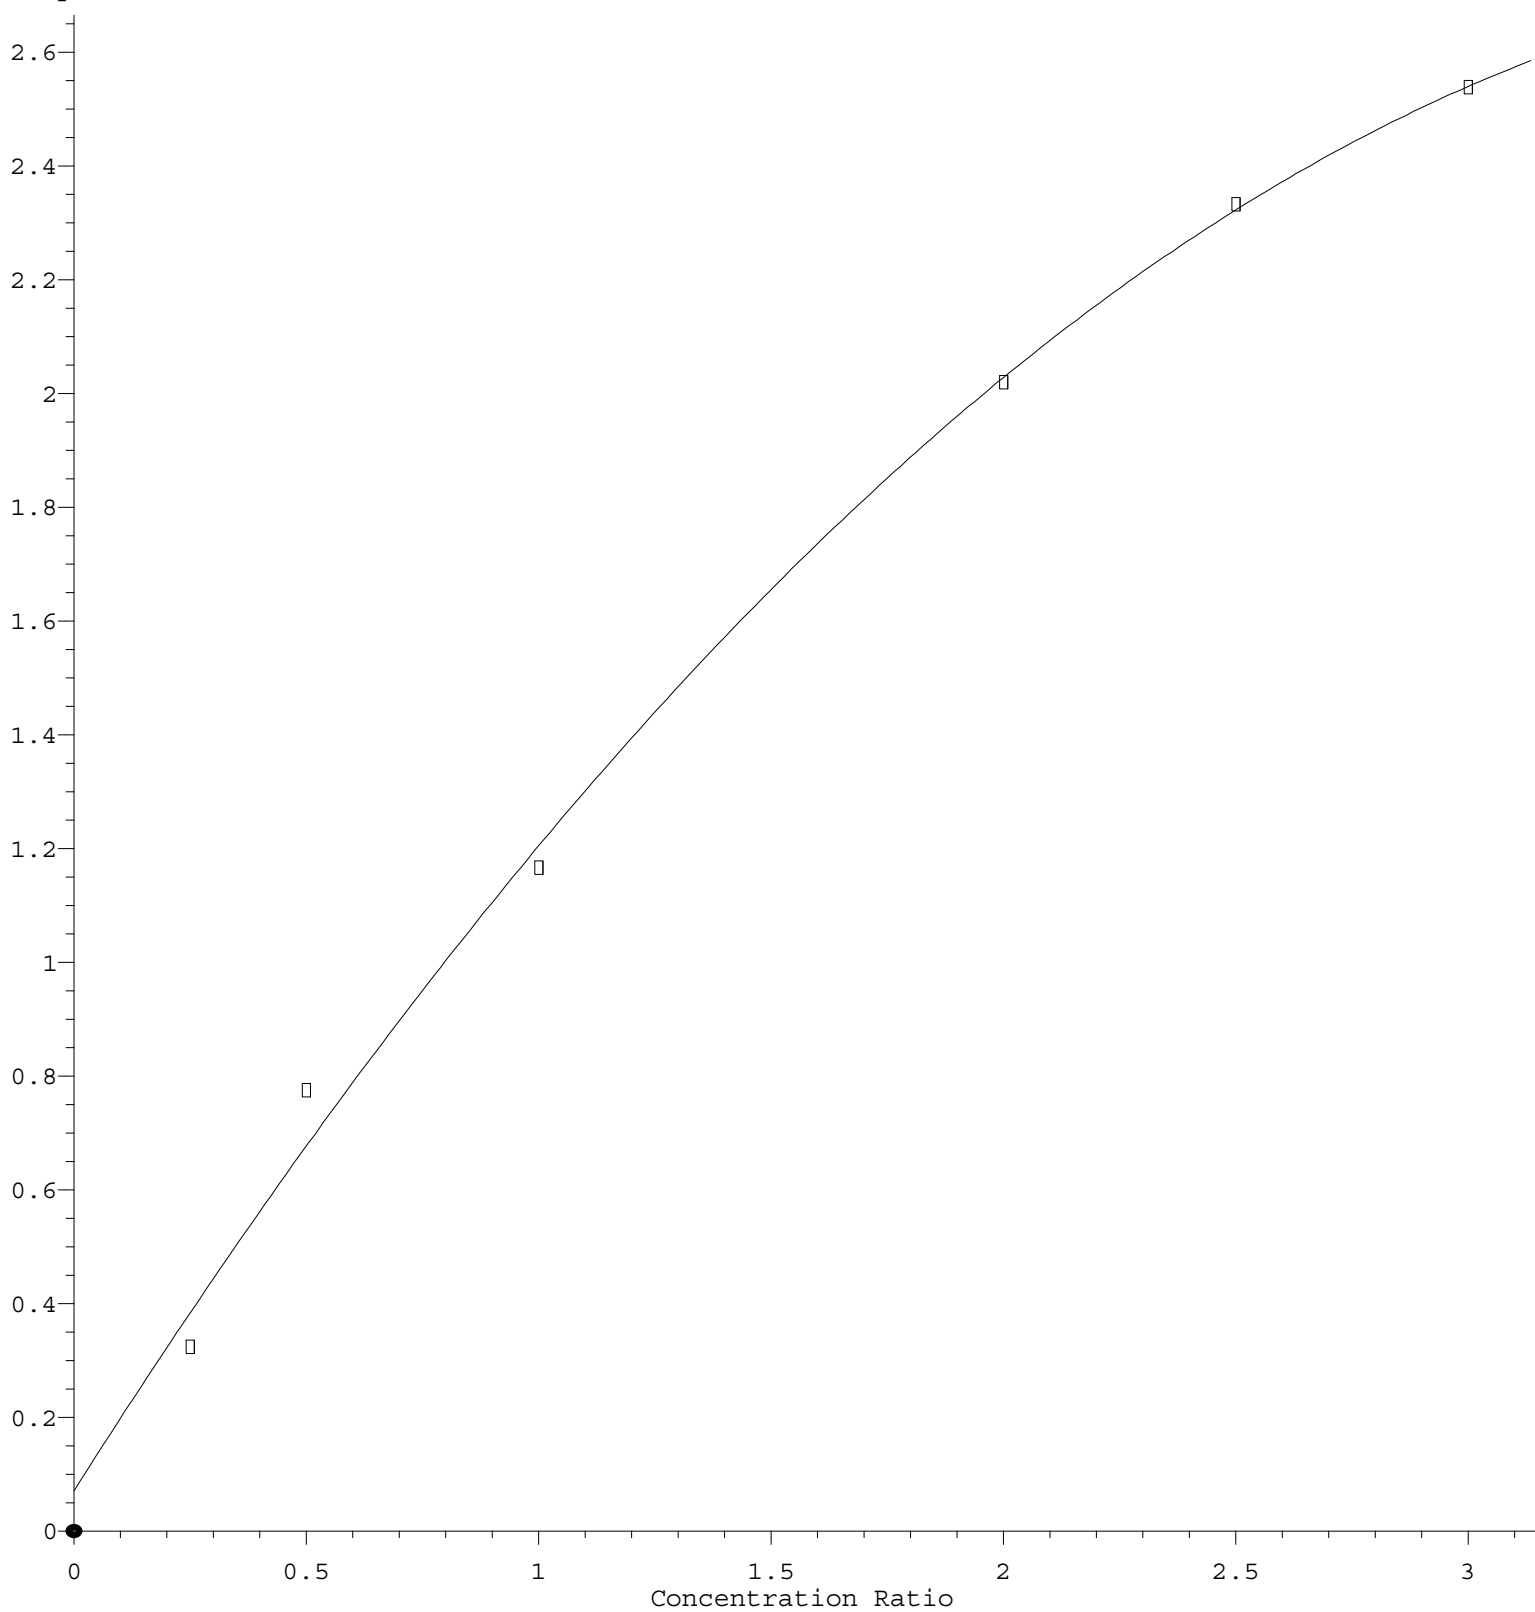

$R = -1.555e-001 A^2 + 1.289e+000 A + 7.123e-002$
 Coef of Det (r^2) = 0.996326 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031721.M
 Calibration Table Last Updated: Thu Mar 18 02:38:45 2021