
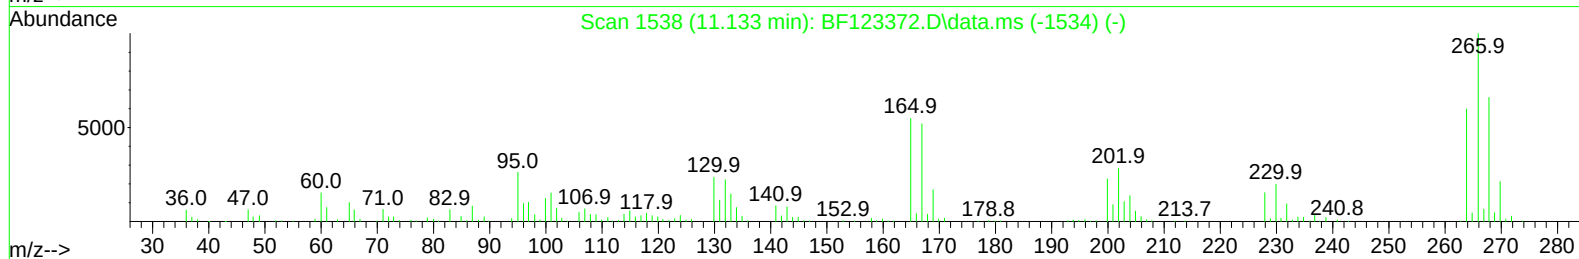
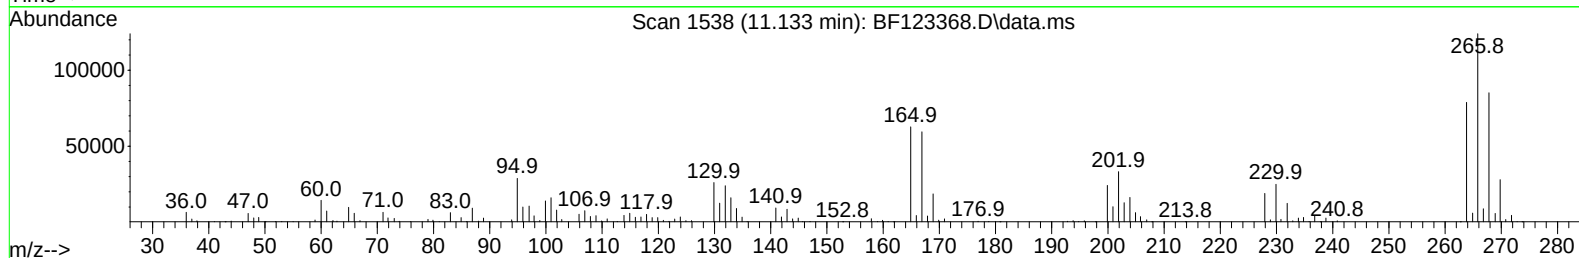


Quant Time: Mar 17 18:51:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 17 18:26:53 2021
Response via : Initial Calibration

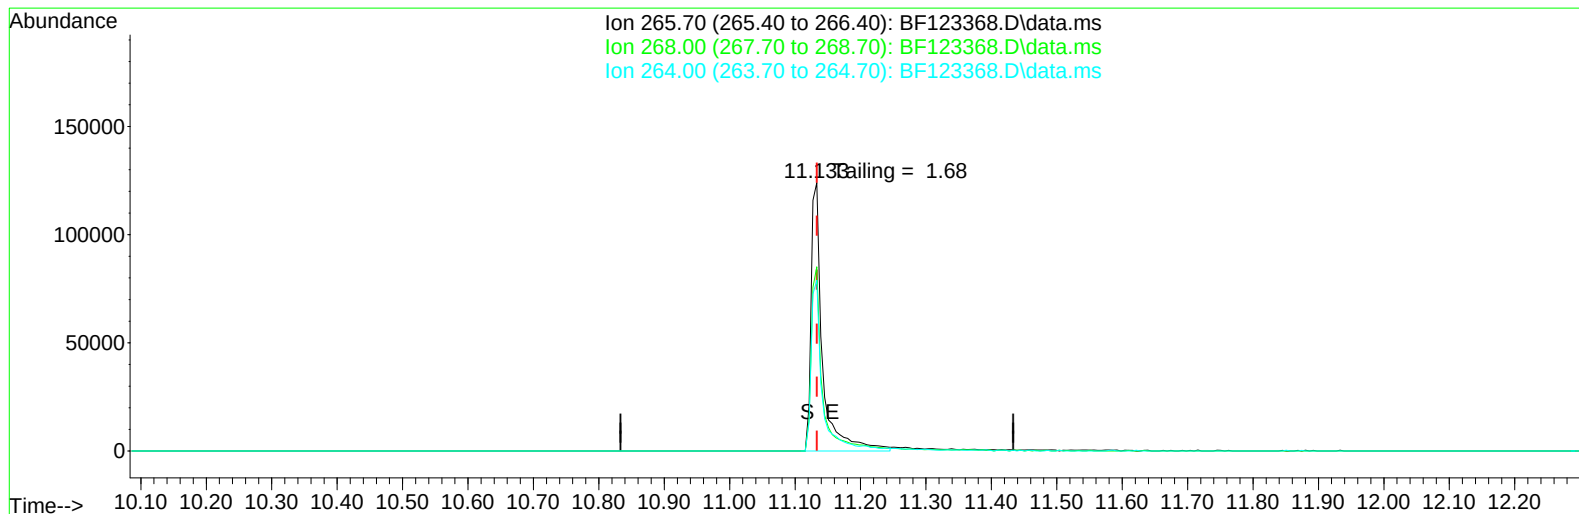

TIC: BF123368.D\data.ms




11.133min (-0.000) 33333.79 ng

response	155183
----------	--------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	68.64
264.00	62.30	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031721\
Data File : BF123368.D
Acq On : 17 Mar 2021 15:53
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 18:51:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 17 18:26:53 2021
Response via : Initial Calibration

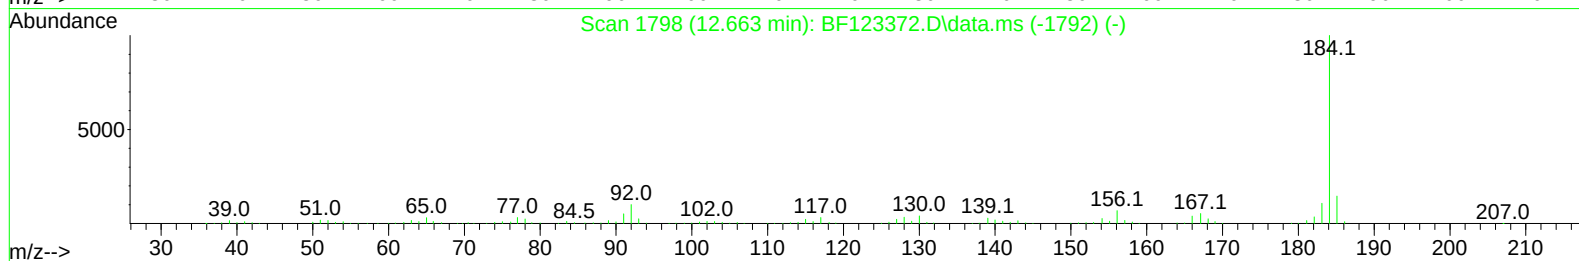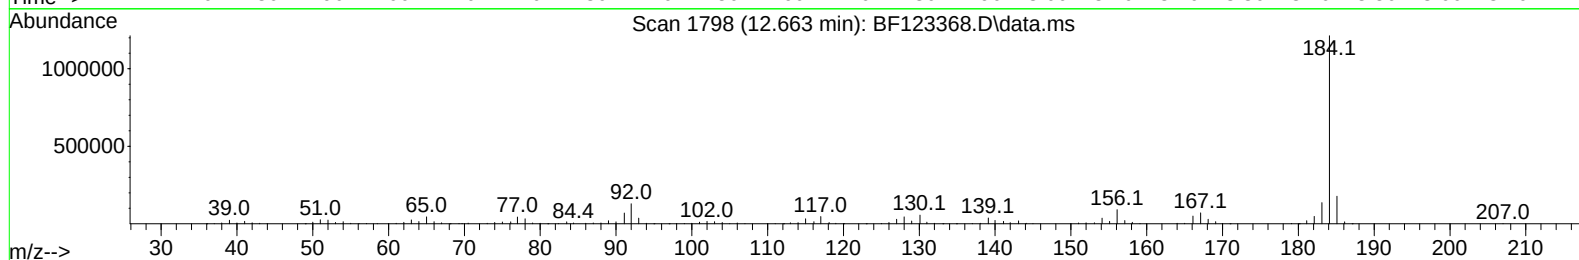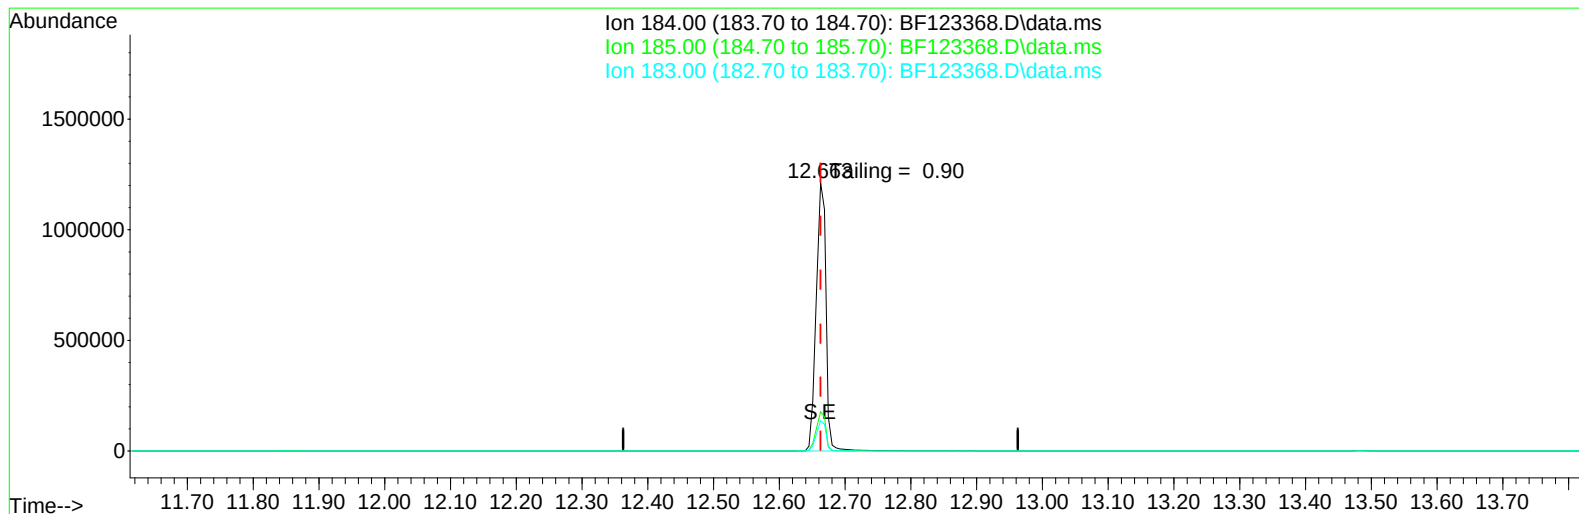

TIC: BF123368.D\data.ms

(77) Benzidine

12.663min (-0.000) 0.00 ng

response 1252767

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.70
183.00	12.10	11.30
0.00	0.00	0.00