

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031721\
 Data File : BF123377.D
 Acq On : 17 Mar 2021 21:09
 Operator : JU/CG
 Sample : PB135194BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB135194BL

Quant Time: Mar 18 03:41:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 18 02:38:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.792	152	212667	20.00	ng	0.00
21) Naphthalene-d8	8.075	136	879607	20.00	ng	# 0.00
39) Acenaphthene-d10	9.827	164	431323	20.00	ng	0.00
64) Phenanthrene-d10	11.316	188	686464	20.00	ng	# 0.00
76) Chrysene-d12	13.962	240	477441	20.00	ng	#-0.01
86) Perylene-d12	15.409	264	370716	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	1584148	105.78	ng	0.01
7) Phenol-d6	6.439	99	1866081	95.93	ng	0.00
23) Nitrobenzene-d5	7.357	82	1209595	80.77	ng	0.00
42) 2,4,6-Tribromophenol	10.627	330	322921	107.12	ng	0.00
45) 2-Fluorobiphenyl	9.151	172	1861412	91.94	ng	0.00
79) Terphenyl-d14	12.910	244	1568736	63.98	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031721\
Data File : BF123377.D
Acq On : 17 Mar 2021 21:09
Operator : JU/CG
Sample : PB135194BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135194BL

Quant Time: Mar 18 03:41:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 02:38:45 2021
Response via : Initial Calibration




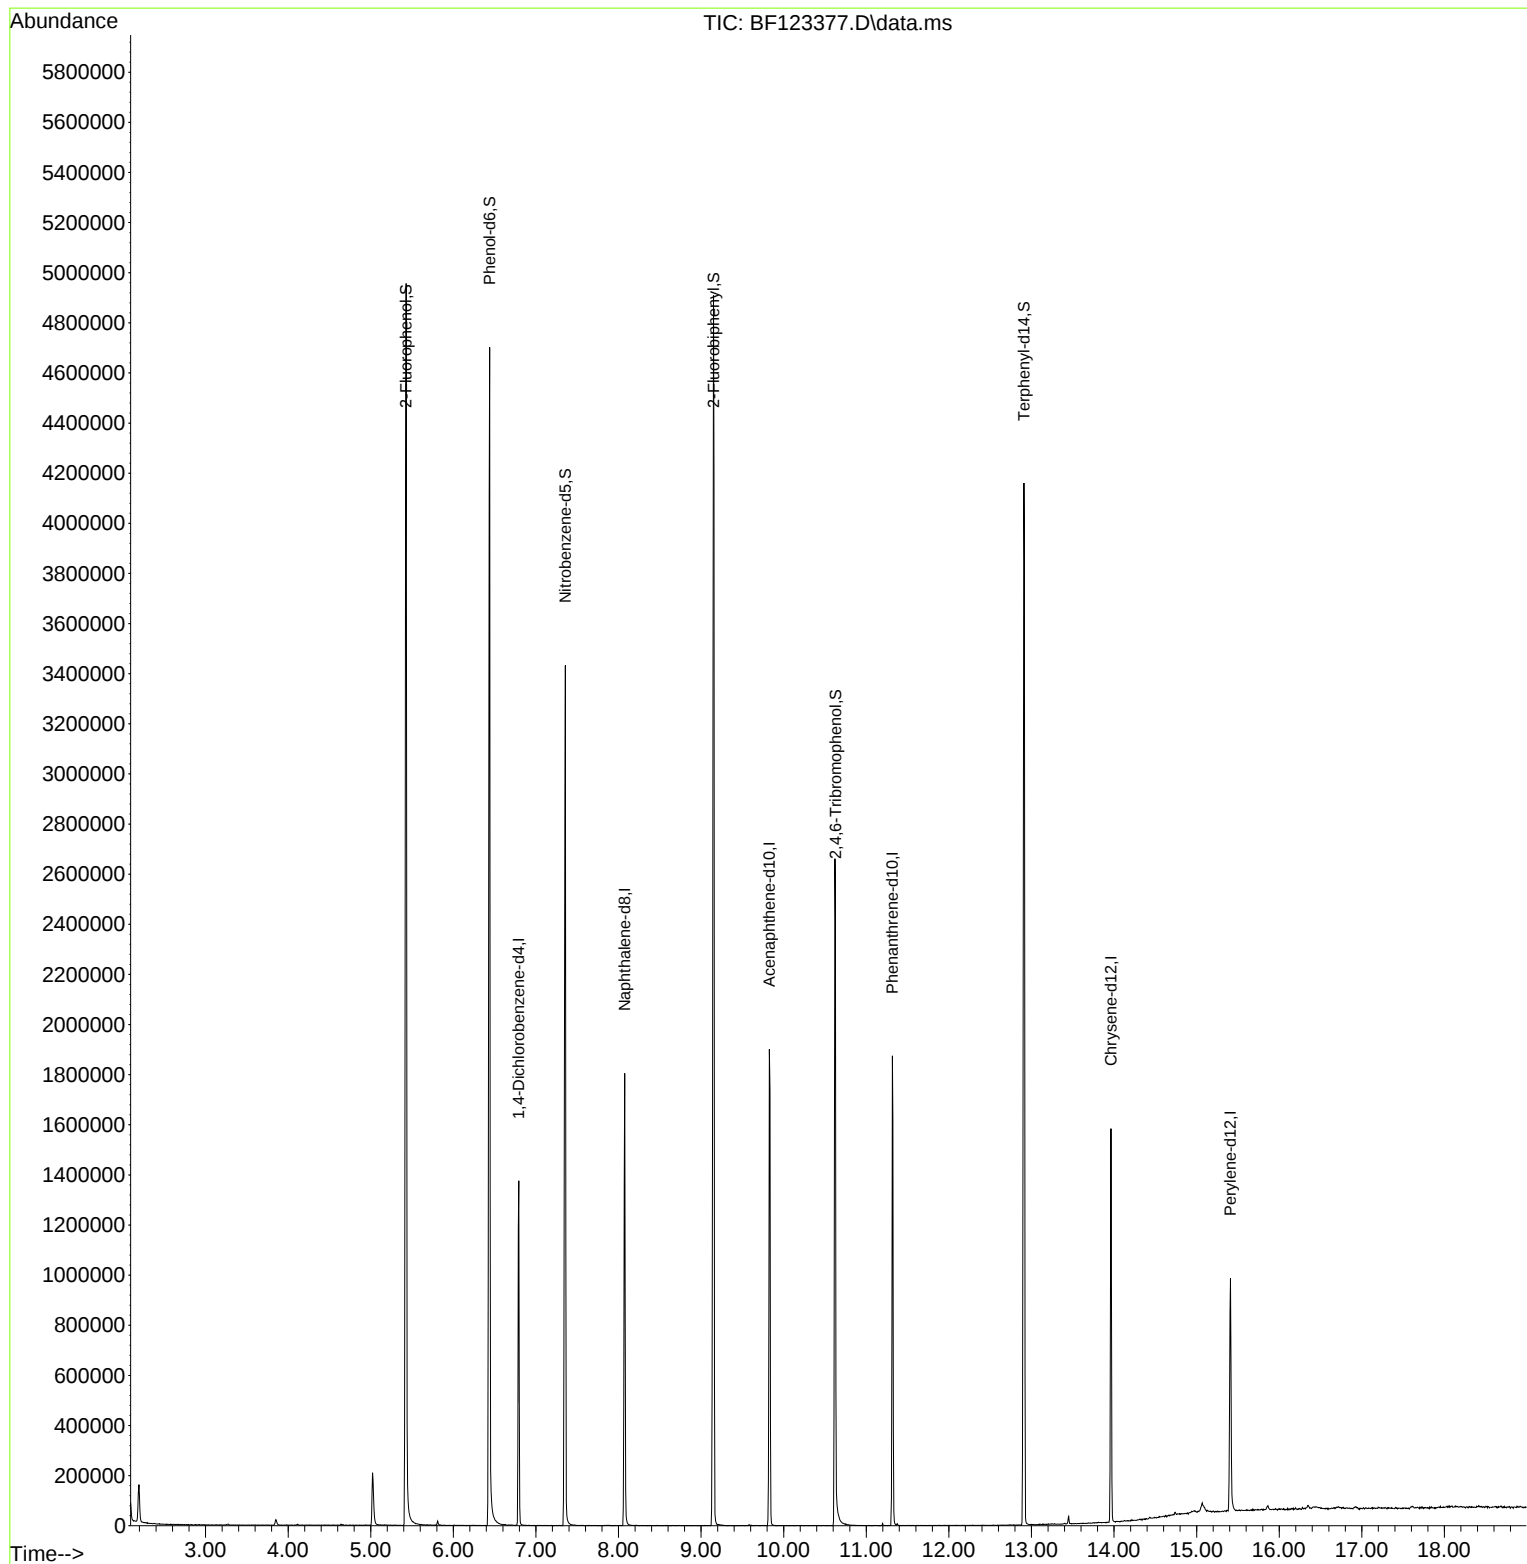


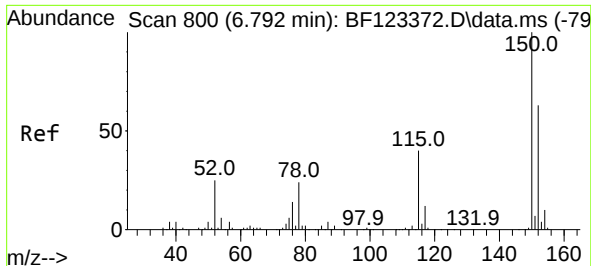

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.792 min Scan# 800
Delta R.T. 0.000 min
Lab File: BF123377.D
Acq: 17 Mar 2021 21:09




Instrument :
BNA_F
ClientSampleId :
PB135194BL


Tgt Ion:152 Resp: 212667
Ion Ratio Lower Upper
152 100
150 157.2 125.8 188.6
115 59.0 49.3 73.9

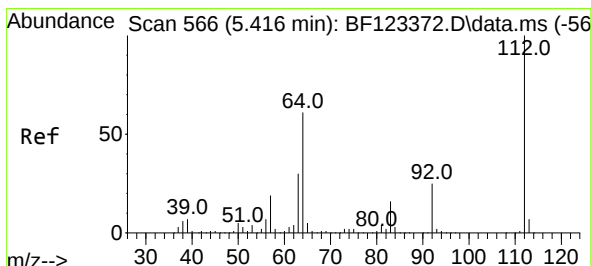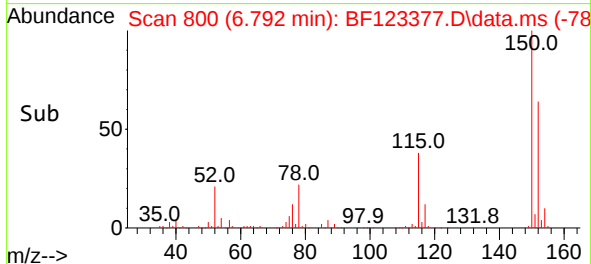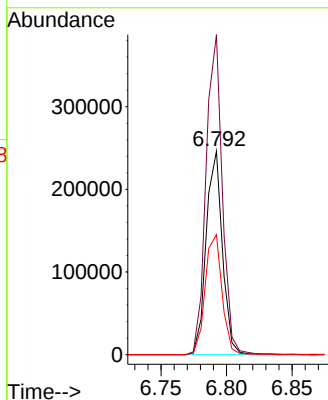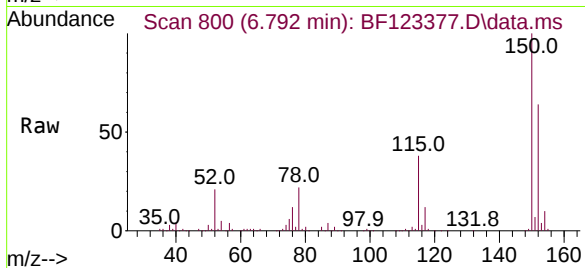

#5
2-Fluorophenol
Concen: 105.78 ng
RT: 5.428 min Scan# 568
Delta R.T. 0.012 min
Lab File: BF123377.D
Acq: 17 Mar 2021 21:09

Tgt Ion:112 Resp: 1584148
Ion Ratio Lower Upper
112 100
64 60.1 46.9 70.3
63 30.9 24.5 36.7


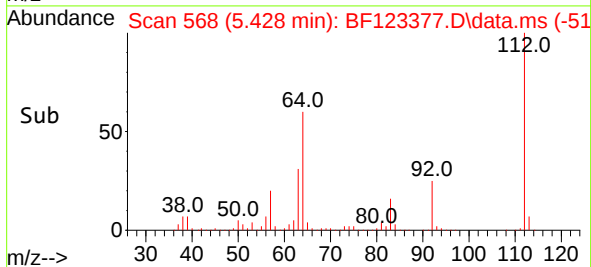
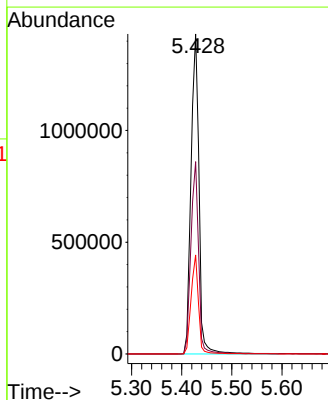
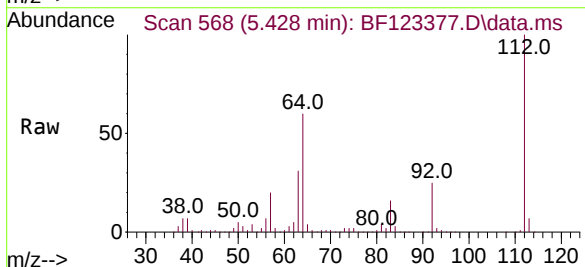


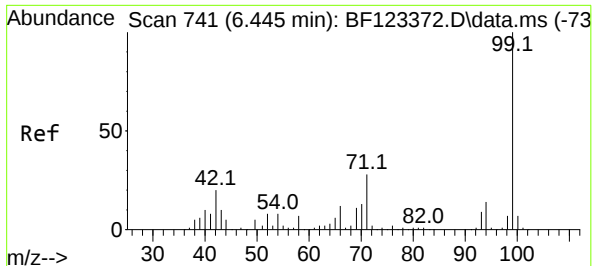

#7
Phenol-d6
Concen: 95.93 ng
RT: 6.439 min Scan# 740
Delta R.T. -0.006 min
Lab File: BF123377.D
Acq: 17 Mar 2021 21:09




Instrument :
BNA_F
ClientSampleId :
PB135194BL


Tgt Ion: 99 Resp: 1866081
Ion Ratio Lower Upper
99 100
42 21.4 13.8 20.6#
71 29.9 26.9 40.3

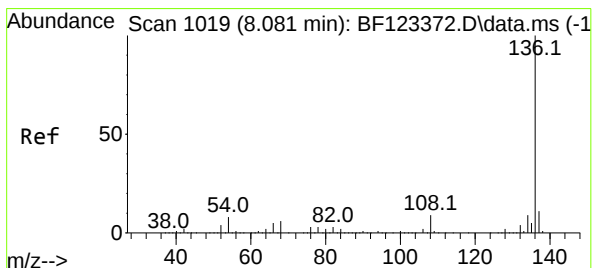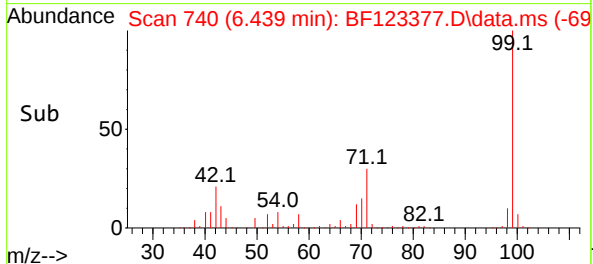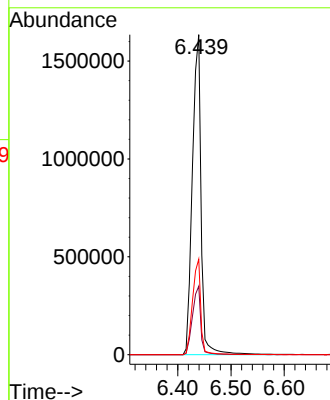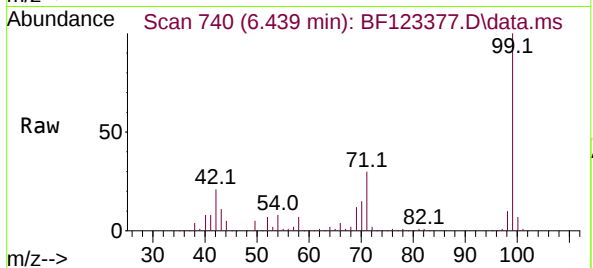

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.075 min Scan# 1018
Delta R.T. -0.006 min
Lab File: BF123377.D
Acq: 17 Mar 2021 21:09

Tgt Ion: 136 Resp: 879607
Ion Ratio Lower Upper
136 100
137 11.2 8.8 13.2
54 8.7 5.5 8.3#
68 6.3 4.6 6.8

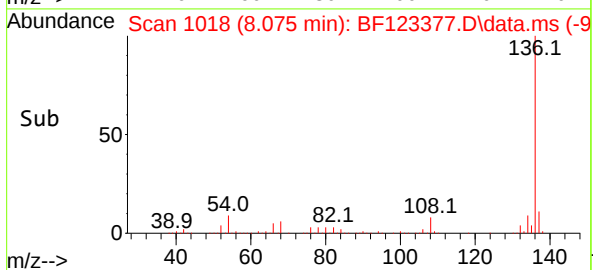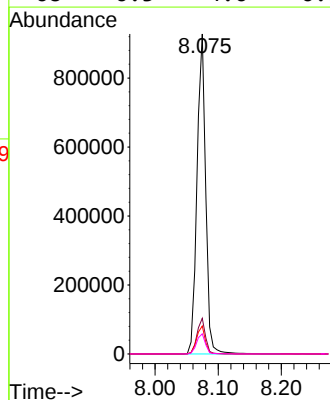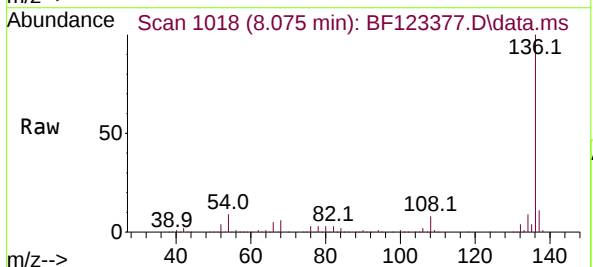

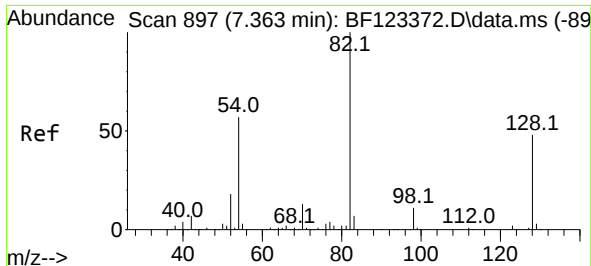

#23

Nitrobenzene-d5

Concen: 80.77 ng

RT: 7.357 min Scan# 896

Delta R.T. -0.006 min

Lab File: BF123377.D

Acq: 17 Mar 2021 21:09

Tgt Ion: 82 Resp: 1209595





Ion	Ratio	Lower	Upper
82	100		
128	48.5	37.0	55.4
54	57.1	38.4	57.6

Instrument :

BNA_F

ClientSampleId :

PB135194BL

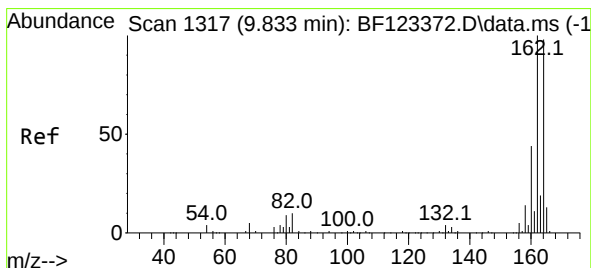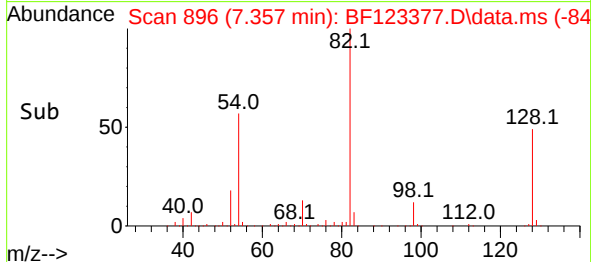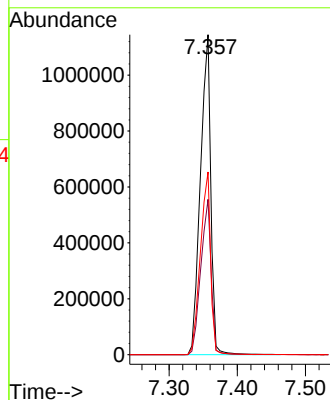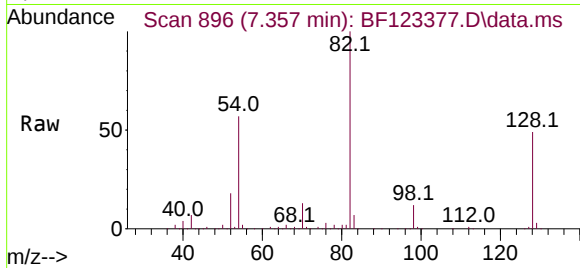

#39

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.827 min Scan# 1316




Delta R.T. -0.006 min


Lab File: BF123377.D

Acq: 17 Mar 2021 21:09

Tgt Ion:164 Resp: 431323

Ion	Ratio	Lower	Upper
164	100		
162	98.5	80.8	121.2
160	43.3	35.4	53.0


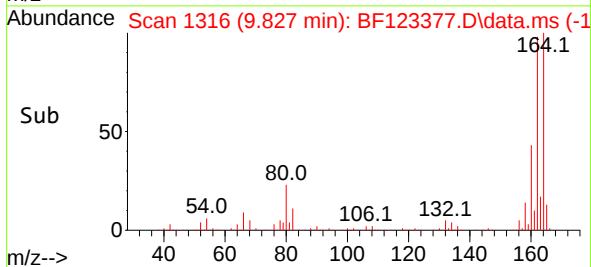
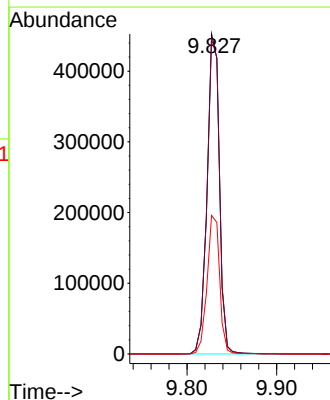
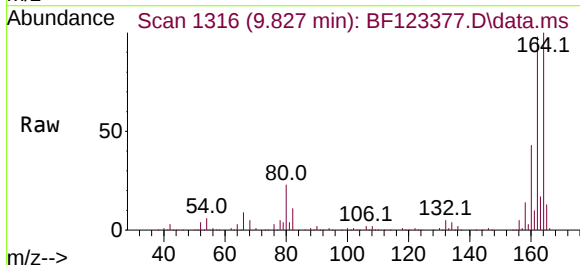


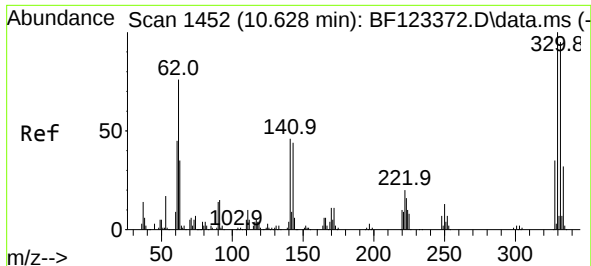

#42
2,4,6-Tribromophenol
Concen: 107.12 ng
RT: 10.627 min Scan# 1452
Delta R.T. -0.001 min
Lab File: BF123377.D
Acq: 17 Mar 2021 21:09




Instrument :
BNA_F
ClientSampleId :
PB135194BL


Tgt Ion:330 Resp: 322921
Ion Ratio Lower Upper
330 100
332 94.5 77.5 116.3
141 44.7 23.8 35.8#

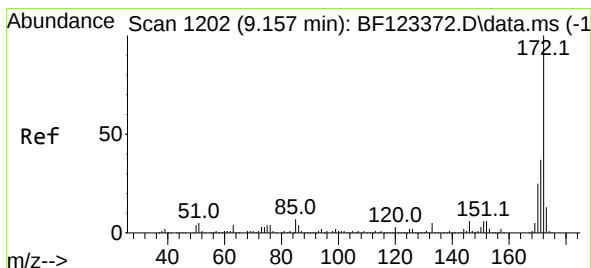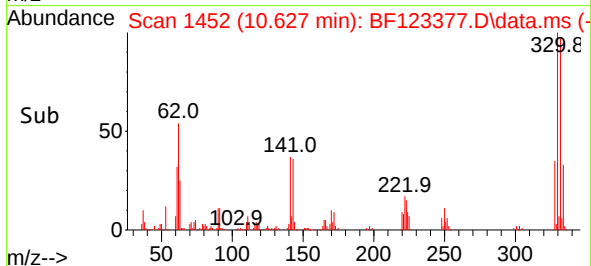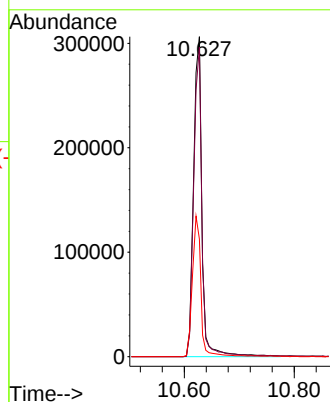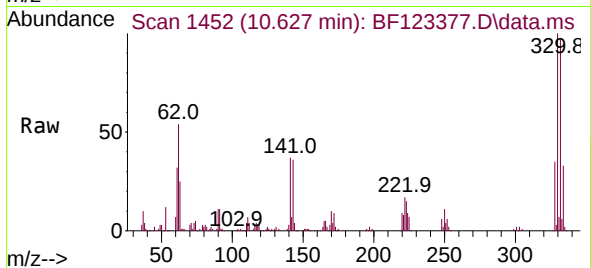

#45
2-Fluorobiphenyl
Concen: 91.94 ng
RT: 9.151 min Scan# 1201
Delta R.T. -0.006 min
Lab File: BF123377.D
Acq: 17 Mar 2021 21:09

Tgt Ion:172 Resp: 1861412
Ion Ratio Lower Upper
172 100
171 35.5 29.6 44.4
170 24.3 19.5 29.3


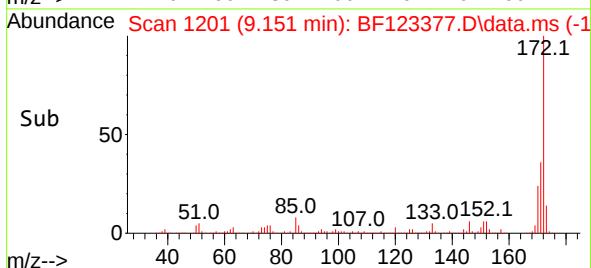
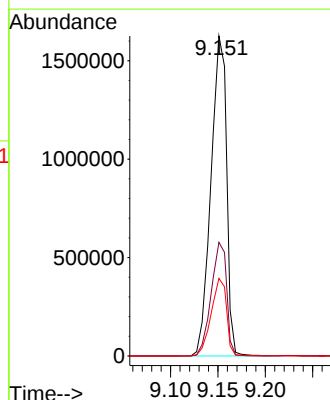
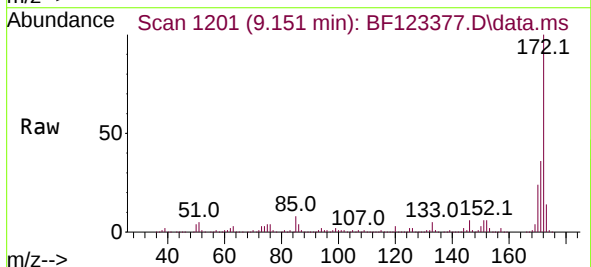


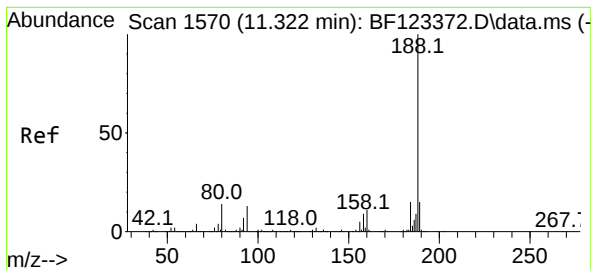

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.316 min Scan# 1569
Delta R.T. -0.006 min
Lab File: BF123377.D
Acq: 17 Mar 2021 21:09




Instrument :
BNA_F
ClientSampleId :
PB135194BL


Tgt Ion:188 Resp: 686464
Ion Ratio Lower Upper
188 100
94 13.2 7.4 11.2#
80 13.8 8.2 12.4#

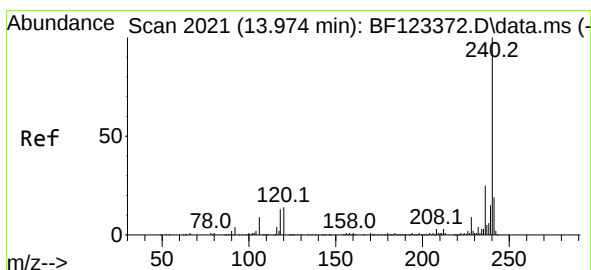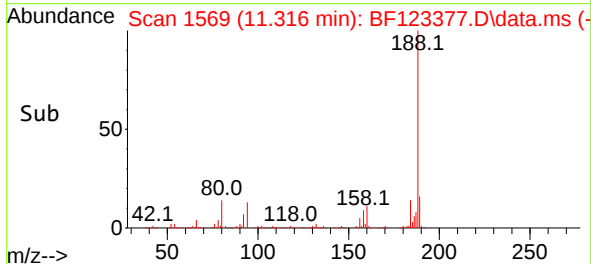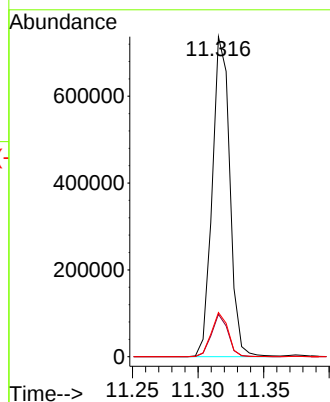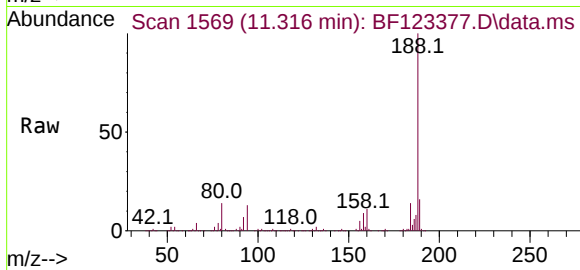

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.962 min Scan# 2019
Delta R.T. -0.012 min
Lab File: BF123377.D
Acq: 17 Mar 2021 21:09

Tgt Ion:240 Resp: 477441
Ion Ratio Lower Upper
240 100
120 17.1 8.6 12.8#
236 26.3 20.3 30.5


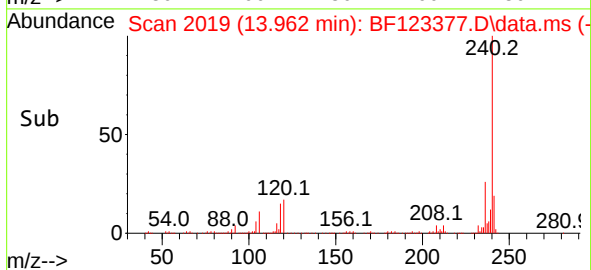
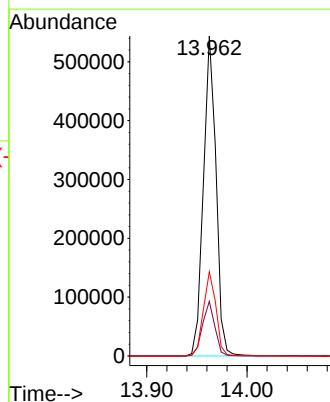
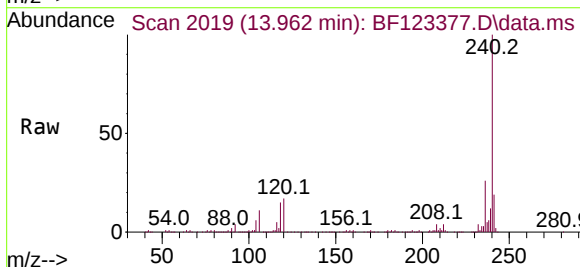


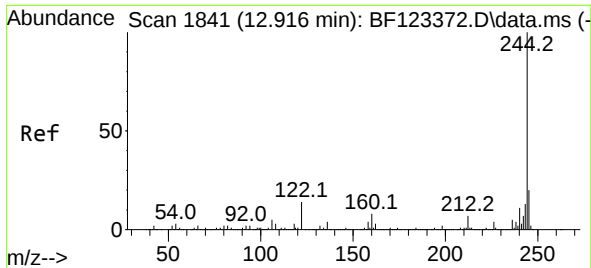

#79
 Terphenyl-d14
 Concen: 63.98 ng
 RT: 12.910 min Scan# 1840
 Delta R.T. -0.006 min
 Lab File: BF123377.D
 Acq: 17 Mar 2021 21:09

Instrument :
 BNA_F
 ClientSampleId :
 PB135194BL

Tgt Ion:244 Resp: 1568736
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.7 8.5
 122 16.1 8.3 12.5#

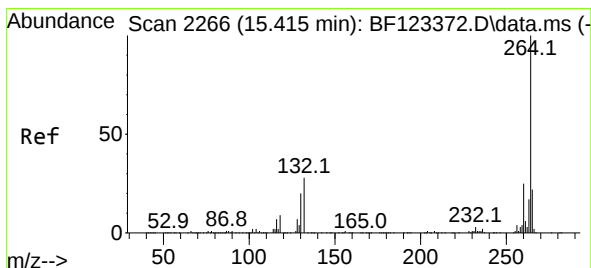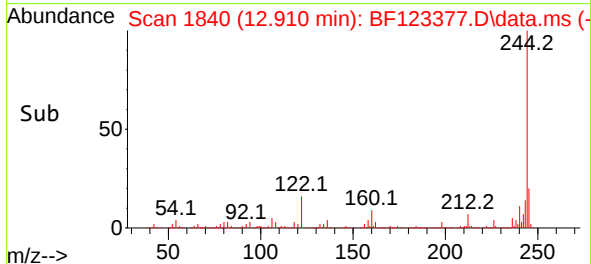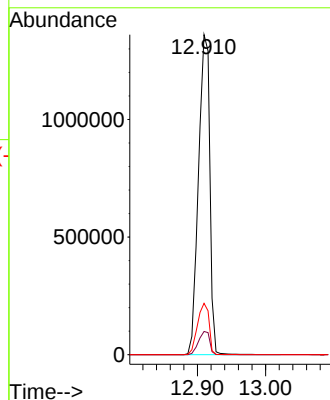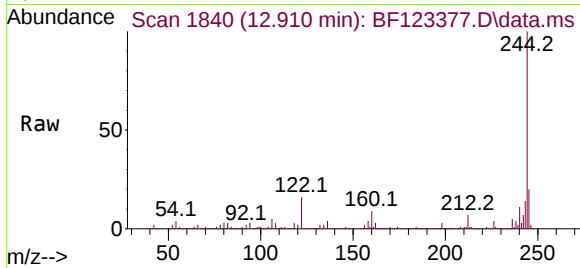

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.409 min Scan# 2265
 Delta R.T. -0.006 min
 Lab File: BF123377.D
 Acq: 17 Mar 2021 21:09

Tgt Ion:264 Resp: 370716
 Ion Ratio Lower Upper
 264 100
 260 24.1 18.6 28.0
 265 21.9 17.0 25.6

