


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031721\
 Data File : BF123368.D
 Acq On : 17 Mar 2021 15:53
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 18 02:38:45 2021

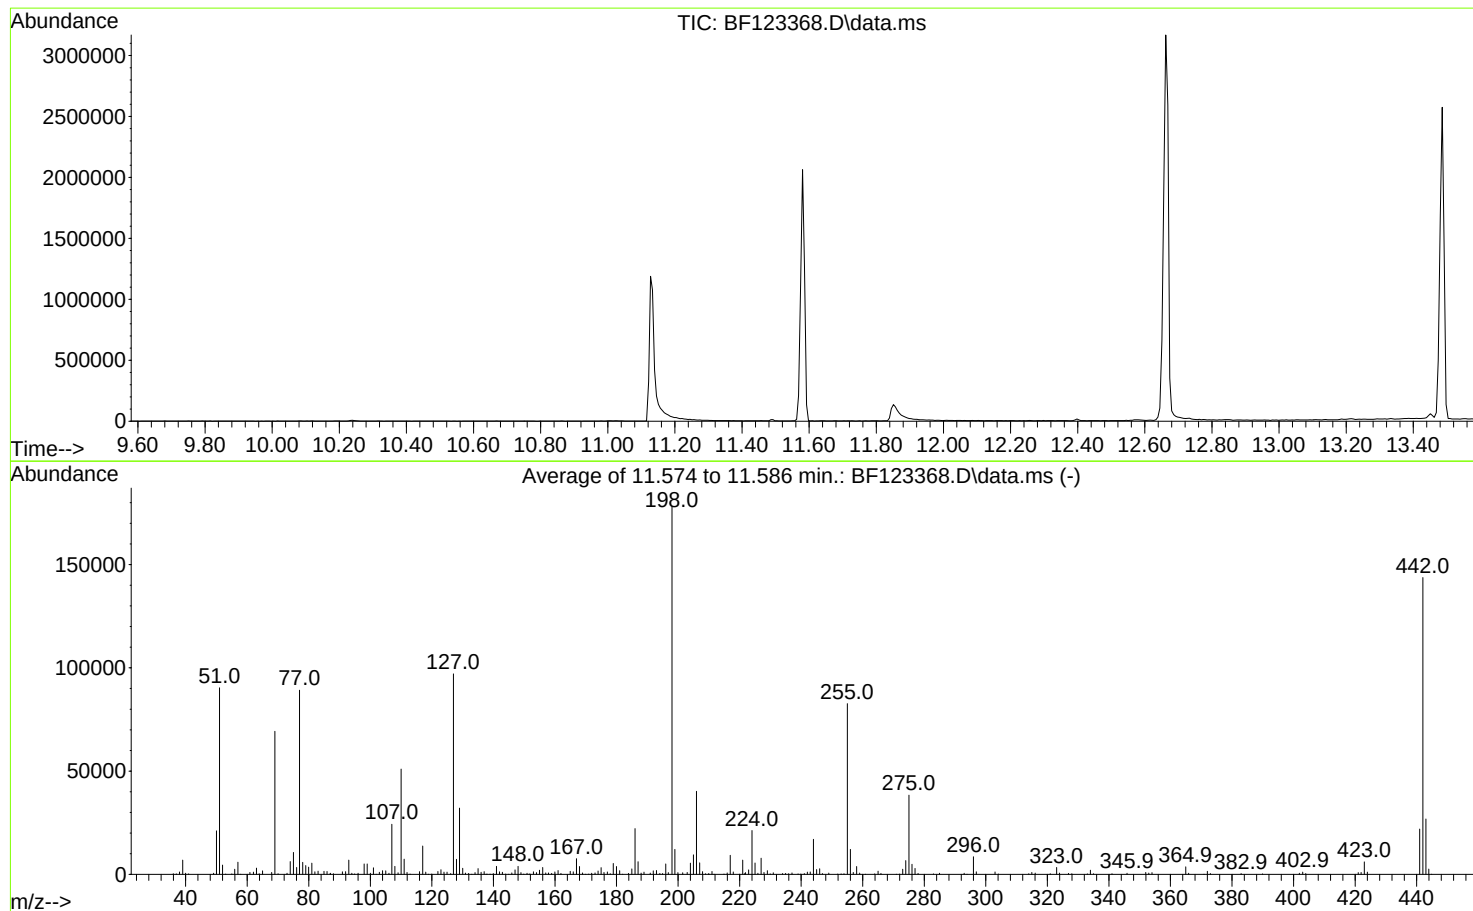

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	90333	PASS
68	69	0.00	2	1.4	952	PASS
69	198	0.00	100	38.9	69259	PASS
70	69	0.00	2	0.4	293	PASS
127	198	10	80	54.5	97091	PASS
197	198	0.00	2	0.5	875	PASS
198	198	100	100	100.0	178133	PASS
199	198	5	9	6.8	12072	PASS
275	198	10	60	21.5	38331	PASS
365	198	1	100	2.1	3662	PASS
441	198	0.01	100	12.3	21936	PASS
442	442	50	100	100.0	143720	PASS
443	442	15	24	18.7	26836	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/17/2021	BNA_F	<u>BF123368.D</u>
Compound Name	Response	Retention Time
DDT	427692	13.48
DDD	1756	13.18
DDE	774	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2530	430222	0.59

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031721\  
Data File : BF123368.D  
Acq On    : 17 Mar 2021  15:53  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 17 18:51:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 17 18:26:53 2021
Response via : Initial Calibration

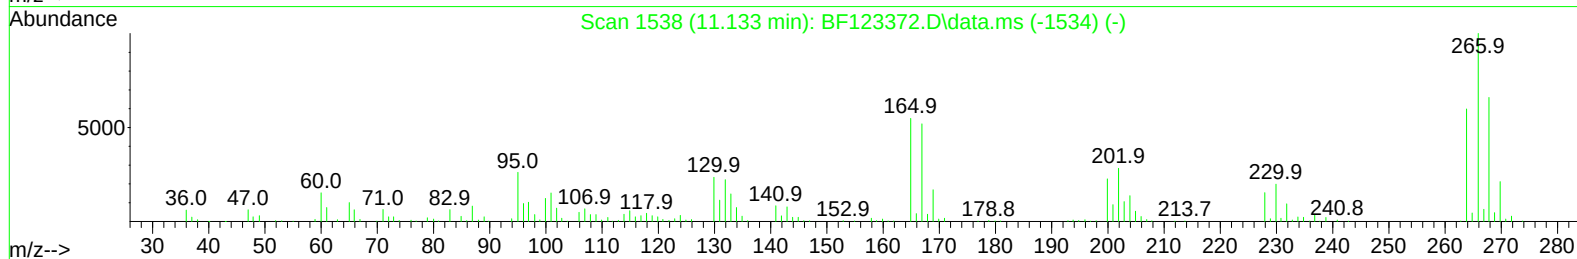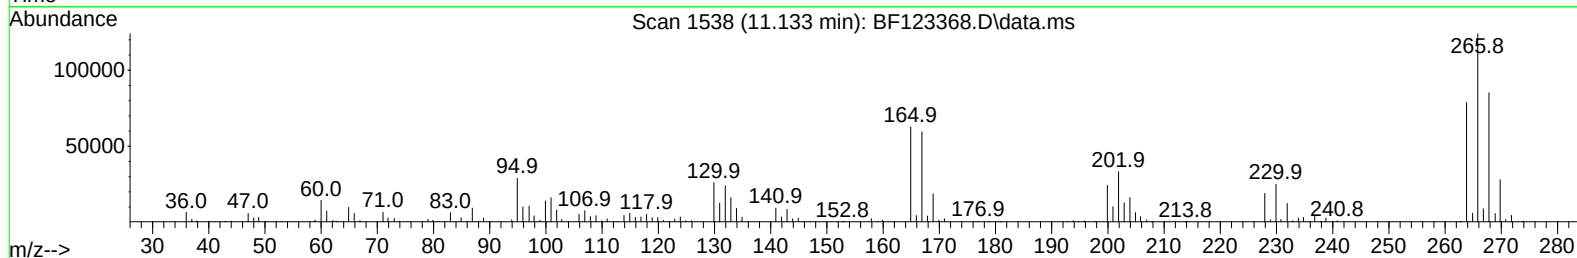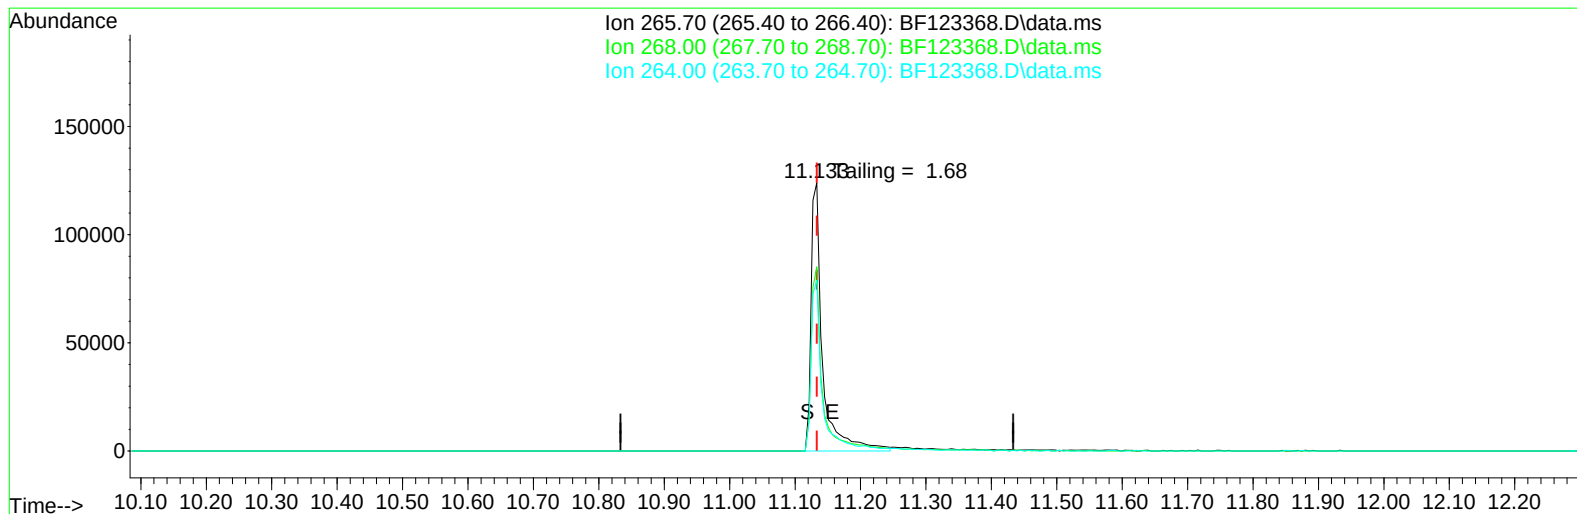

TIC: BF123368.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.000) 33333.79 ng




response **155183**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	68.64
264.00	62.30	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031721\
 Data File : BF123368.D
 Acq On : 17 Mar 2021 15:53
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 17 18:51:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 17 18:26:53 2021
 Response via : Initial Calibration

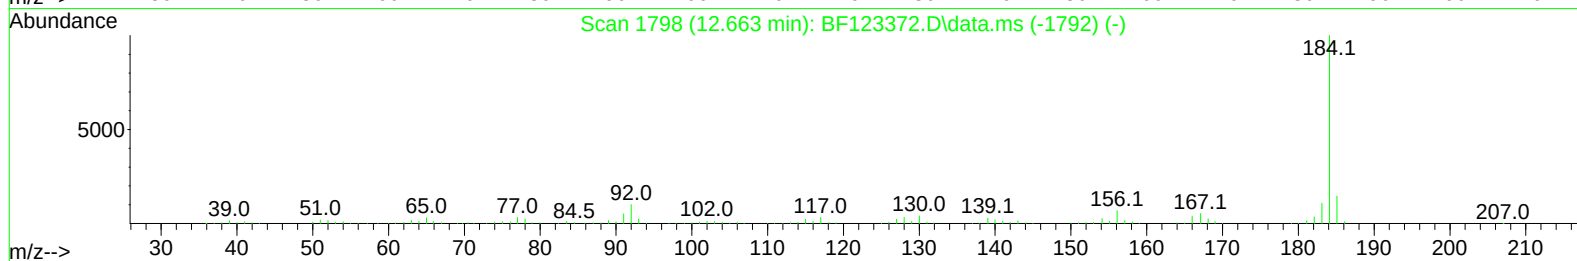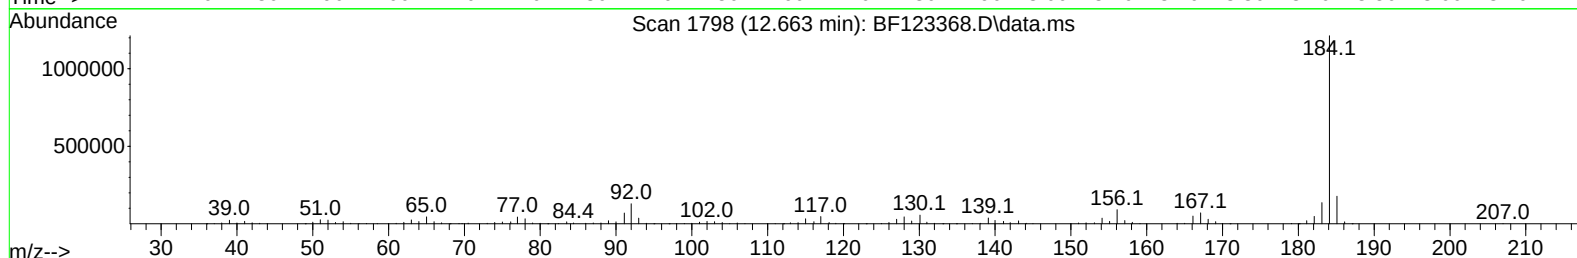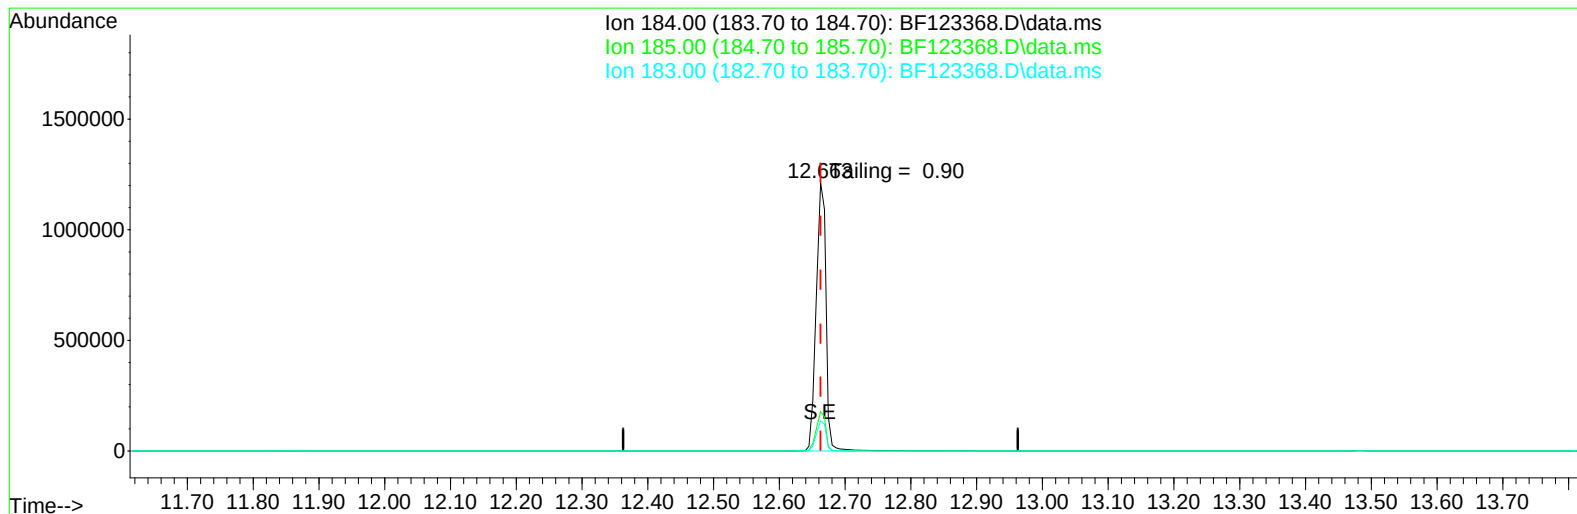

TIC: BF123368.D\data.ms

(77) Benzidine

12.663min (-0.000) 0.00 ng

response 1252767

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.70
183.00	12.10	11.30
0.00	0.00	0.00