

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031821\
 Data File : BF123383.D
 Acq On : 18 Mar 2021 15:00
 Operator : JU/CG
 Sample : PB135224BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB135224BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	562	566	589	rBV	4142215	4261304	76.19%	10.755%
2	6.434	735	739	742	rBV	3927555	4128485	73.81%	10.419%
3	6.792	796	800	803	rBV	1623093	1393450	24.91%	3.517%
4	6.951	822	827	830	rBV	4392047	4434622	79.28%	11.192%
5	7.357	891	896	899	rBV	3657766	3935337	70.36%	9.932%
6	8.075	1014	1018	1021	rBV	2204047	1834277	32.79%	4.629%
7	9.157	1196	1202	1205	rBV	5152309	5593333	100.00%	14.116%
8	9.827	1312	1316	1320	rBV	2230957	1944535	34.77%	4.908%
9	10.621	1447	1451	1468	rBV	2453992	2405264	43.00%	6.070%
10	11.316	1565	1569	1573	rBV	2090701	1816994	32.48%	4.586%
11	12.910	1835	1840	1843	rBV	4437744	5084988	90.91%	12.834%
12	13.962	2015	2019	2028	rVB	1596776	1471147	26.30%	3.713%
13	15.409	2259	2265	2273	rBV	1024558	1318992	23.58%	3.329%




Sum of corrected areas: 39622728

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031821\
Data File : BF123383.D
Acq On : 18 Mar 2021 15:00
Operator : JU/CG
Sample : PB135224BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135224BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

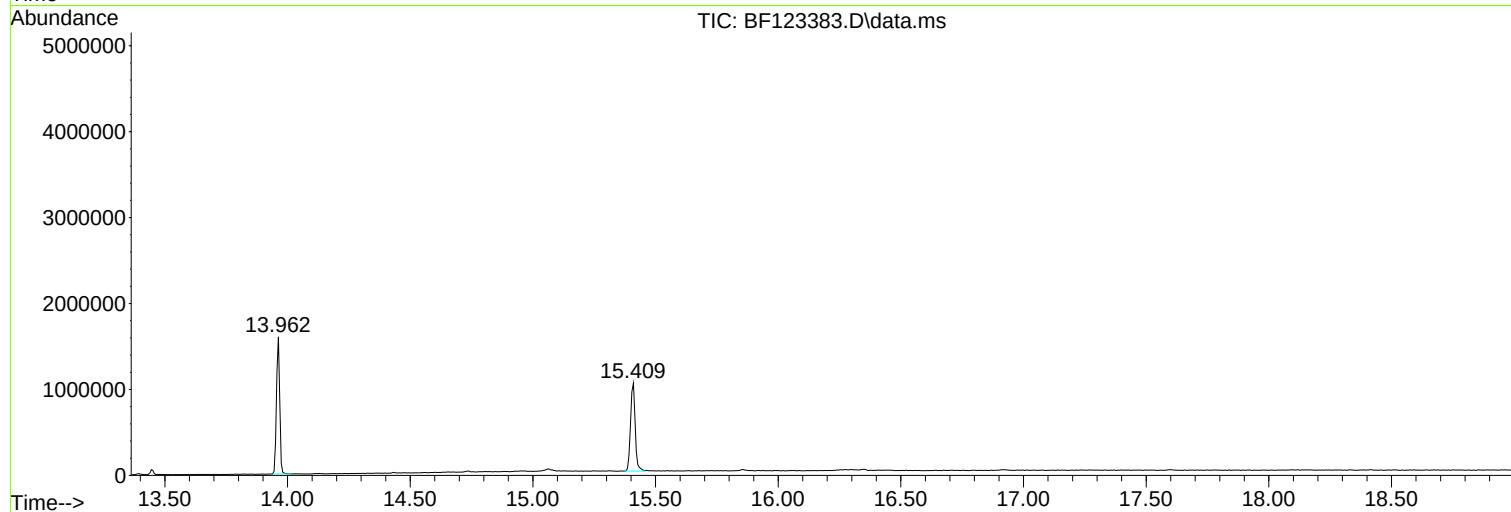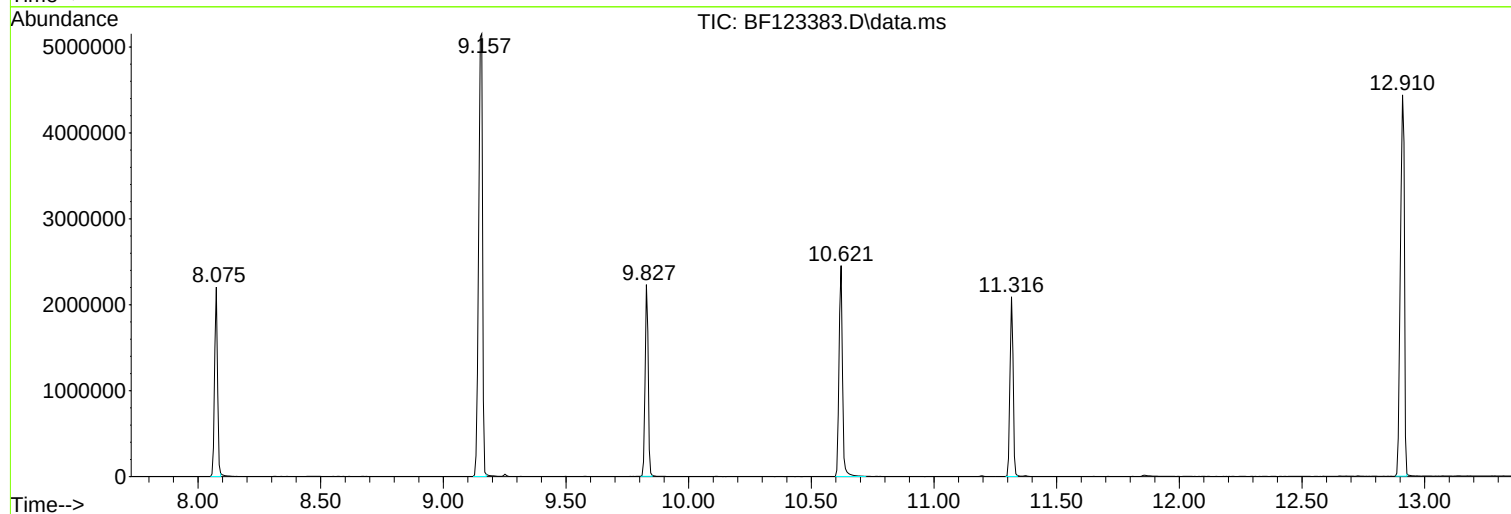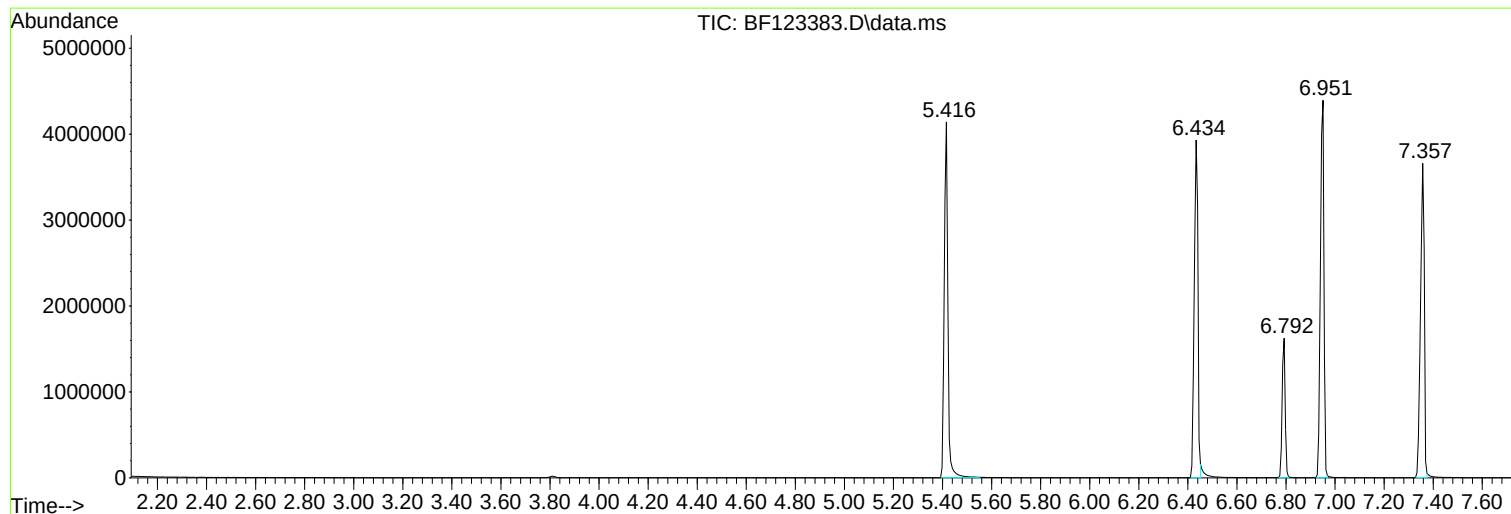

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031821\
Data File : BF123383.D
Acq On : 18 Mar 2021 15:00
Operator : JU/CG
Sample : PB135224BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135224BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031821\
Data File : BF123383.D
Acq On : 18 Mar 2021 15:00
Operator : JU/CG
Sample : PB135224BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135224BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------