
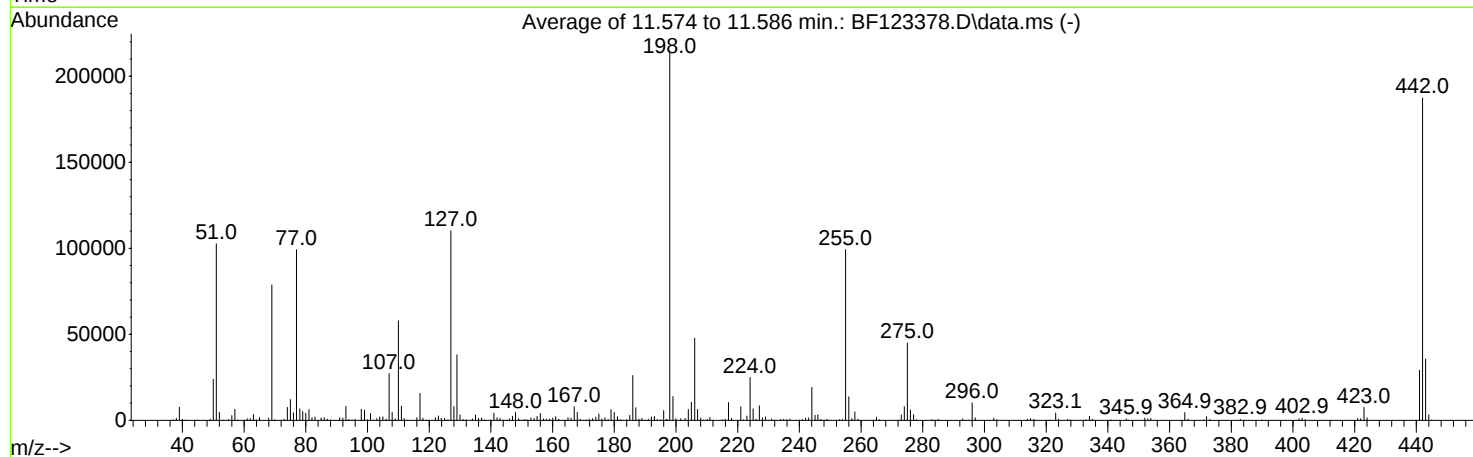


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031821\
 Data File : BF123378.D
 Acq On : 18 Mar 2021 10:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 18 02:38:45 2021

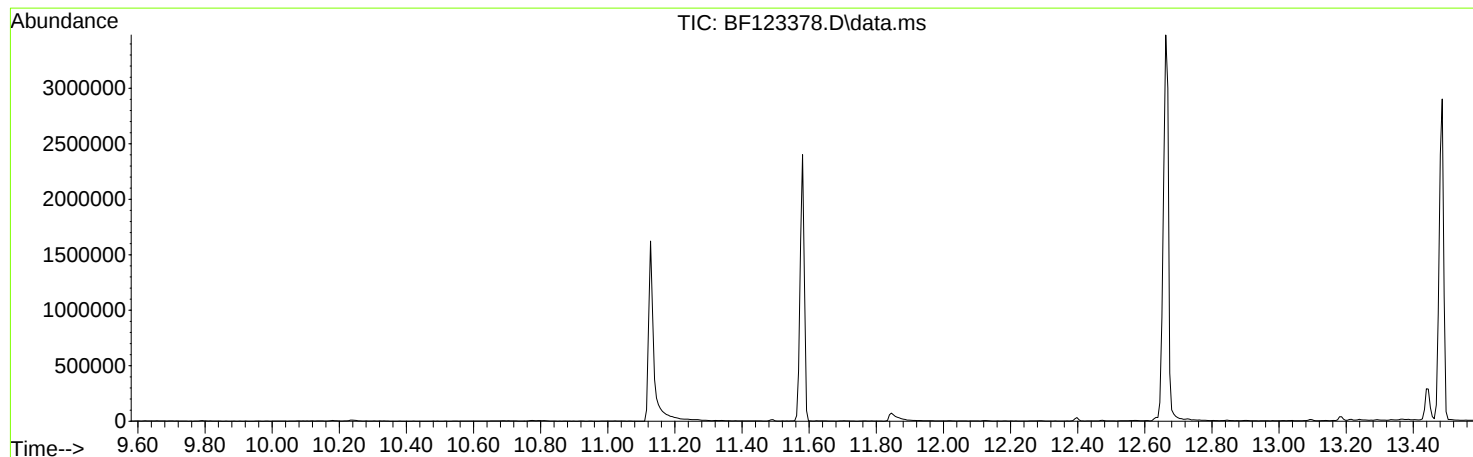

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.0	102581	PASS
68	69	0.00	2	1.7	1315	PASS
69	198	0.00	100	36.9	78808	PASS
70	69	0.00	2	0.4	354	PASS
127	198	10	80	51.5	110187	PASS
197	198	0.00	2	0.3	585	PASS
198	198	100	100	100.0	213803	PASS
199	198	5	9	6.5	13829	PASS
275	198	10	60	21.0	44957	PASS
365	198	1	100	2.1	4550	PASS
441	198	0.01	100	13.6	29138	PASS
442	442	50	100	100.0	187400	PASS
443	442	15	24	19.0	35603	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/18/2021	BNA_F	<u>BF123378.D</u>
Compound Name	Response	Retention Time
DDT	511315	13.48
DDD	7693	13.18
DDE	932	12.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8625	519940	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031821\
Data File : BF123378.D
Acq On : 18 Mar 2021 10:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 18 12:14:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 02:38:45 2021
Response via : Initial Calibration

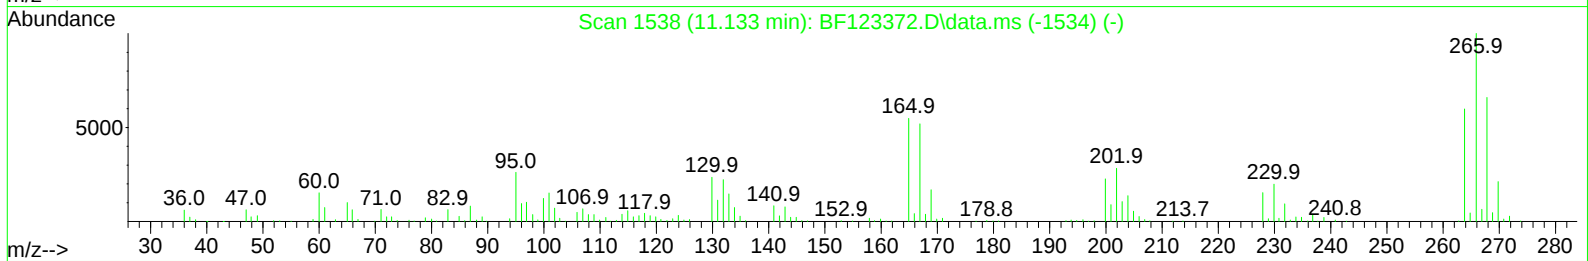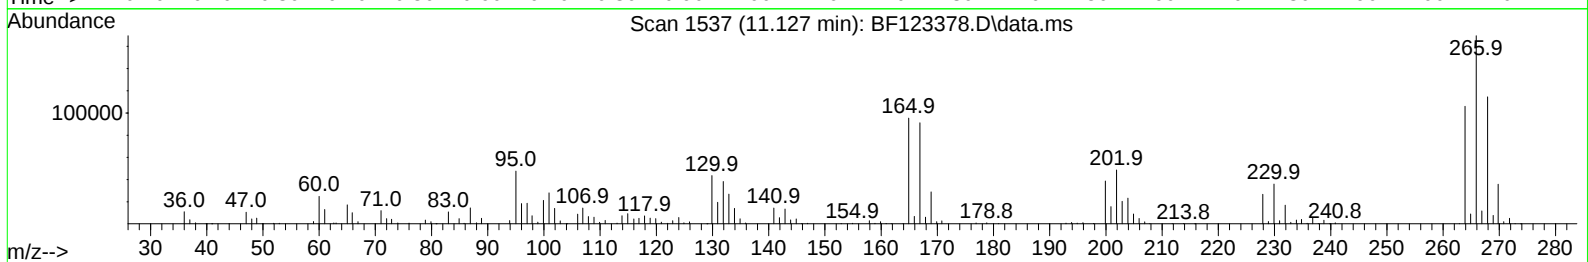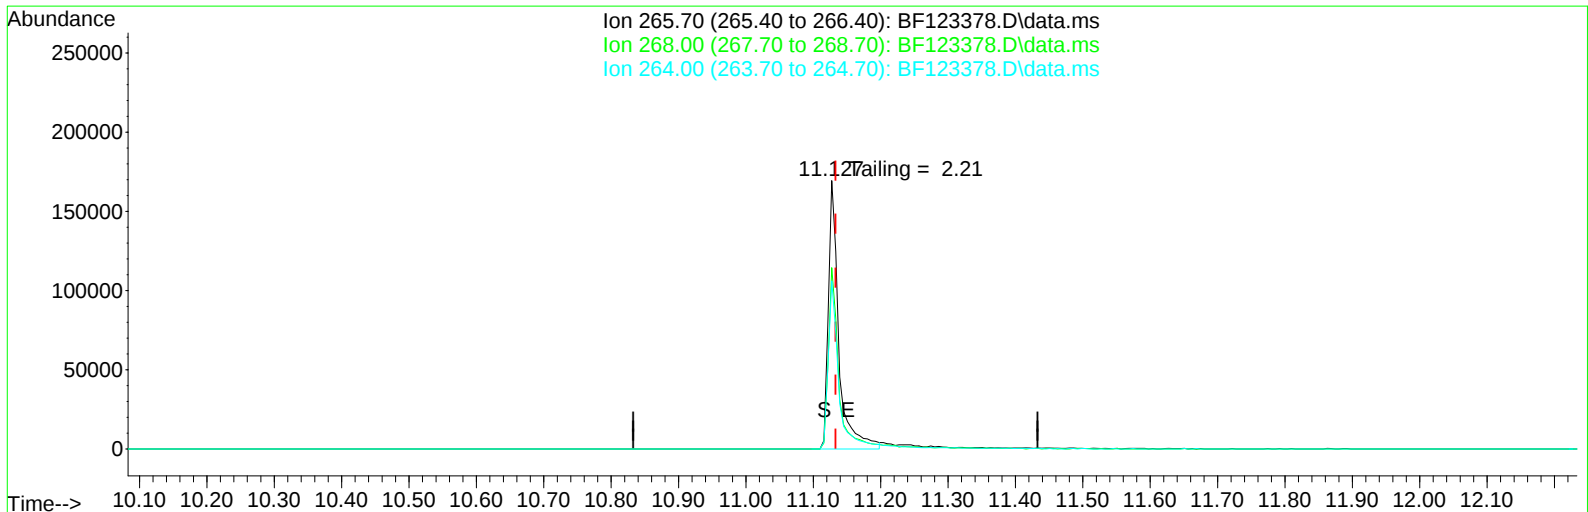

TIC: BF123378.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.006) 323436.44 ng




response 190686

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	67.56
264.00	62.30	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031821\
Data File : BF123378.D
Acq On : 18 Mar 2021 10:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 18 12:14:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 02:38:45 2021
Response via : Initial Calibration

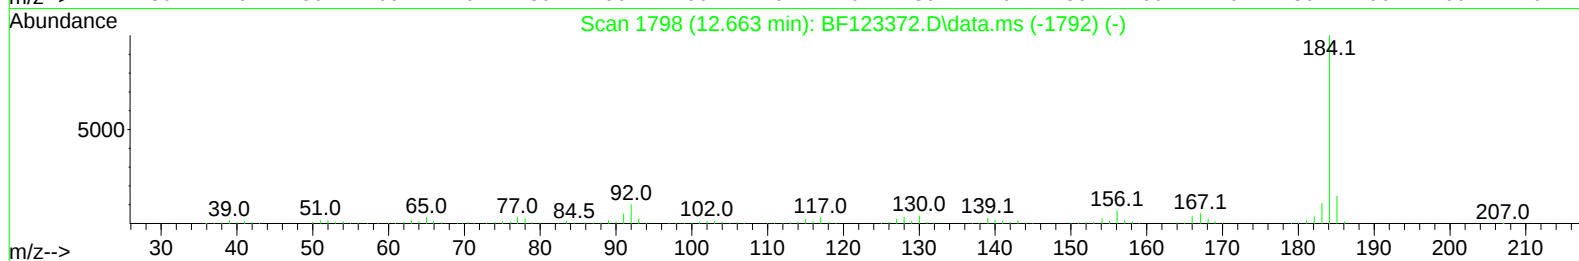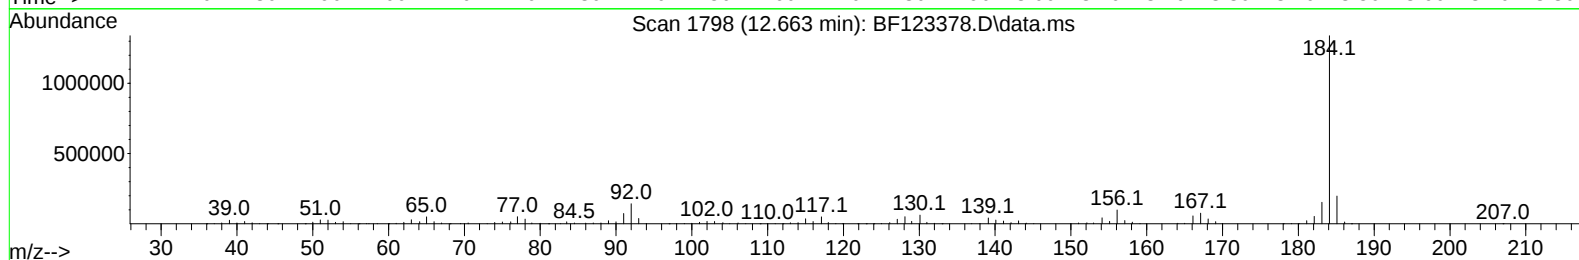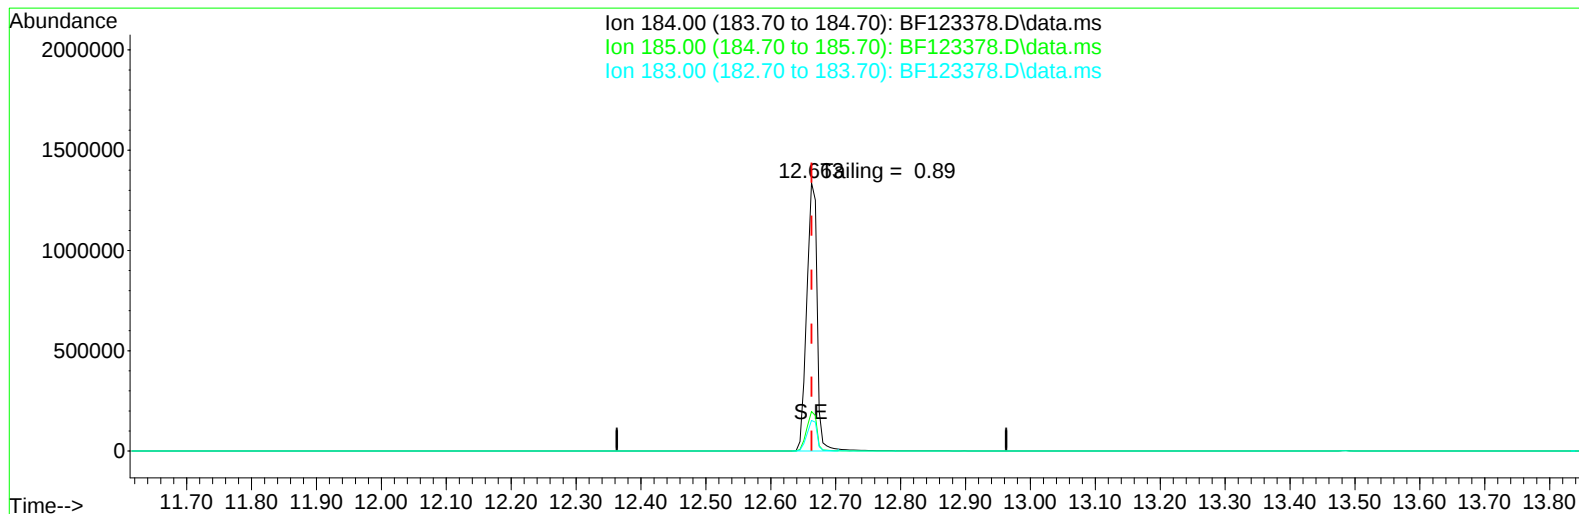

TIC: BF123378.D\data.ms

(77) Benzidine

12.663min (-0.000) 0.00 ng

response 1490262

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.76
183.00	12.10	11.41
0.00	0.00	0.00