
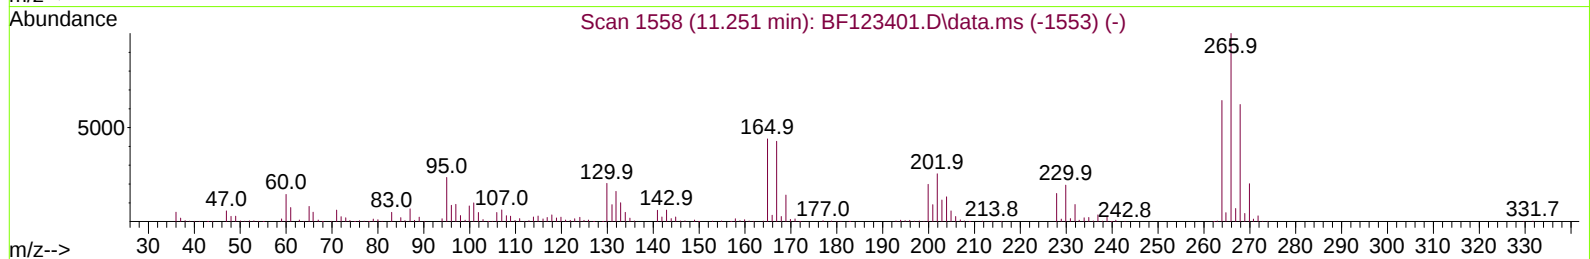
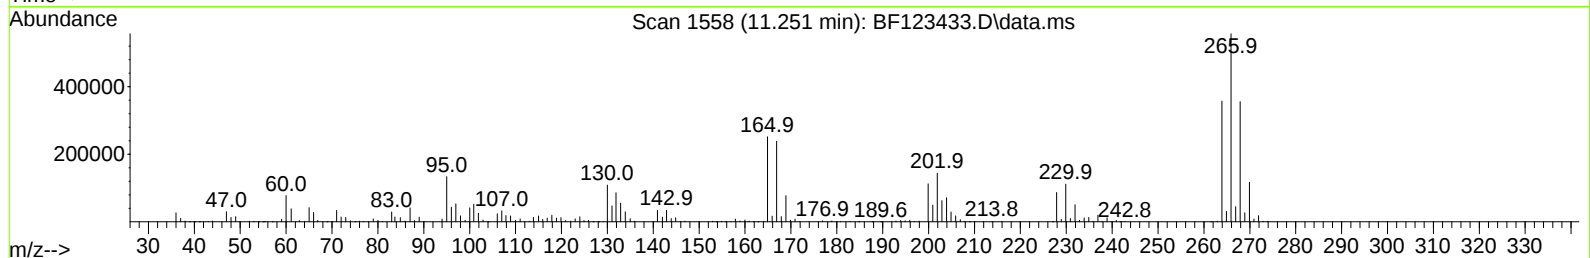


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032421\
Data File : BF123433.D
Acq On : 24 Mar 2021 11:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 12:41:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 23 15:58:35 2021
Response via : Initial Calibration

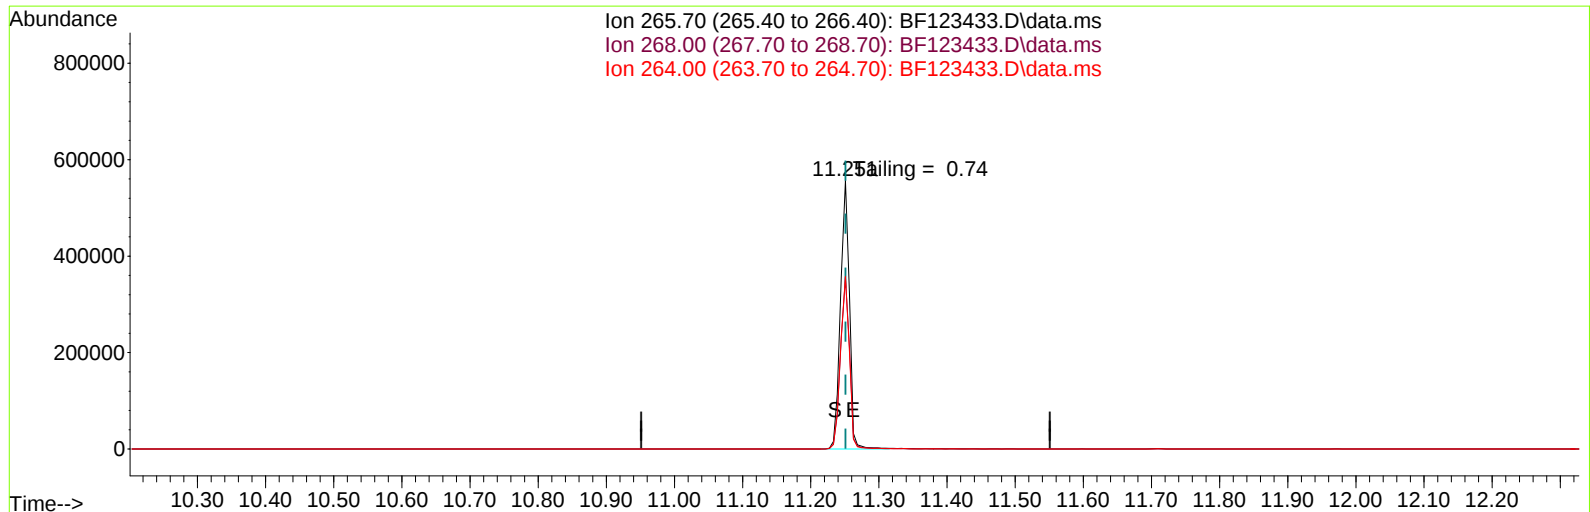

TIC: BF123433.D\data.ms

(70) Pentachlorophenol (C)




11.251min (-0.000) 488653.75 ng

response 506163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.93
264.00	62.30	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032421\
Data File : BF123433.D
Acq On : 24 Mar 2021 11:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 12:41:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 23 15:58:35 2021
Response via : Initial Calibration

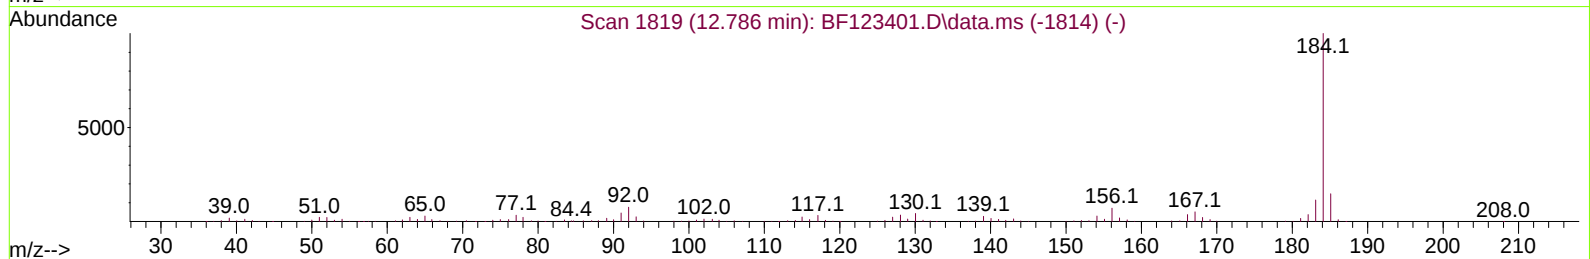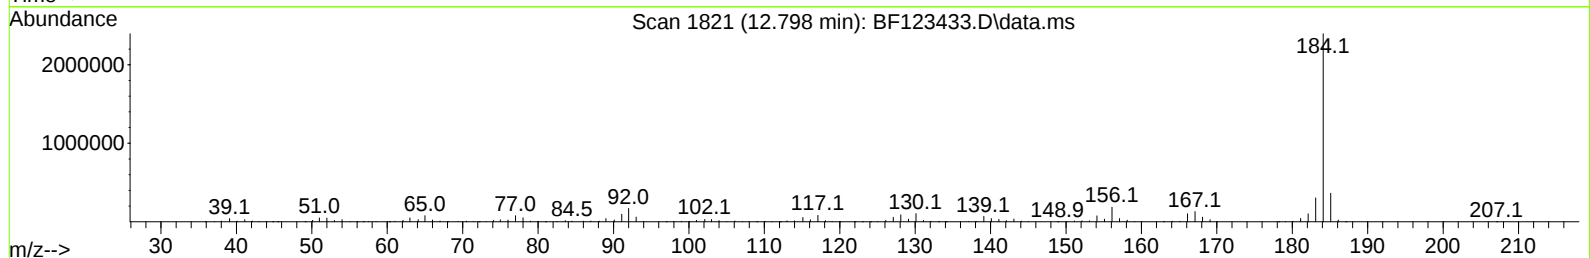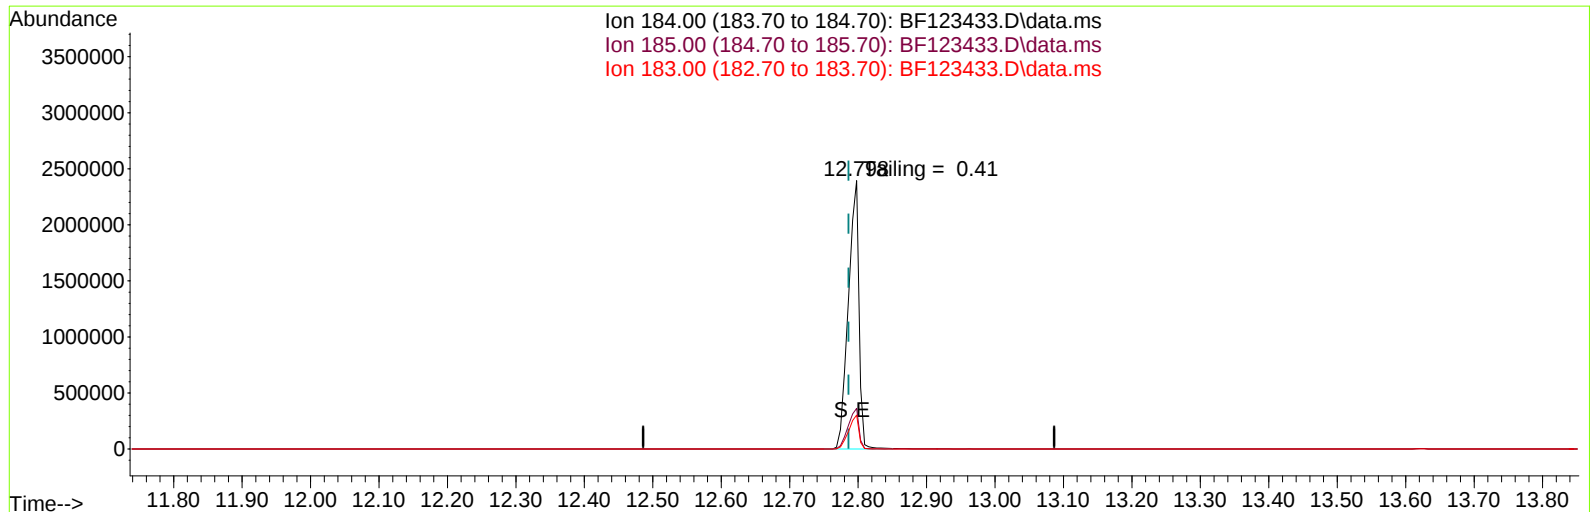

TIC: BF123433.D\data.ms

(77) Benzidine

12.798min (+ 0.011) 4839.63 ng m

response 2587153

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.16
183.00	12.10	12.66
0.00	0.00	0.00