


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032421\
 Data File : BF123433.D
 Acq On : 24 Mar 2021 11:20
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 25 12:42:42 2021

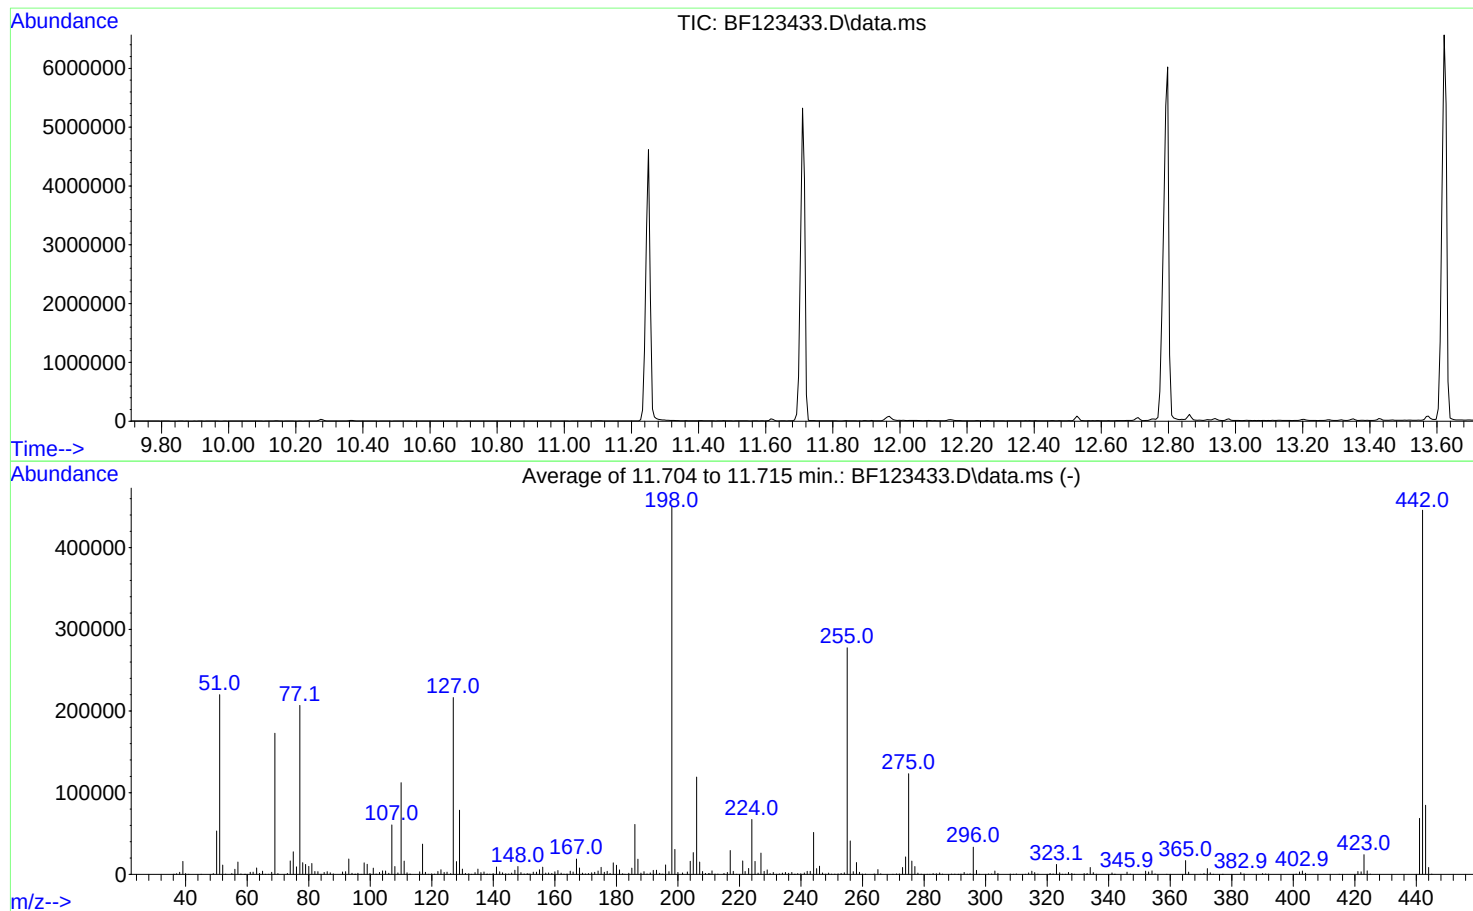




AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	220117	PASS
68	69	0.00	2	1.5	2545	PASS
69	198	0.00	100	38.4	172891	PASS
70	69	0.00	2	0.5	928	PASS
127	198	10	80	48.1	216512	PASS
197	198	0.00	2	0.7	3326	PASS
198	198	100	100	100.0	450432	PASS
199	198	5	9	6.8	30533	PASS
275	198	10	60	27.3	123155	PASS
365	198	1	100	3.7	16851	PASS
441	198	0.01	100	15.2	68493	PASS
442	442	50	100	100.0	445973	PASS
443	442	15	24	19.0	84701	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032421\
 Data File : BF123433.D
 Acq On : 24 Mar 2021 11:20
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 24 12:41:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 23 15:58:35 2021
 Response via : Initial Calibration

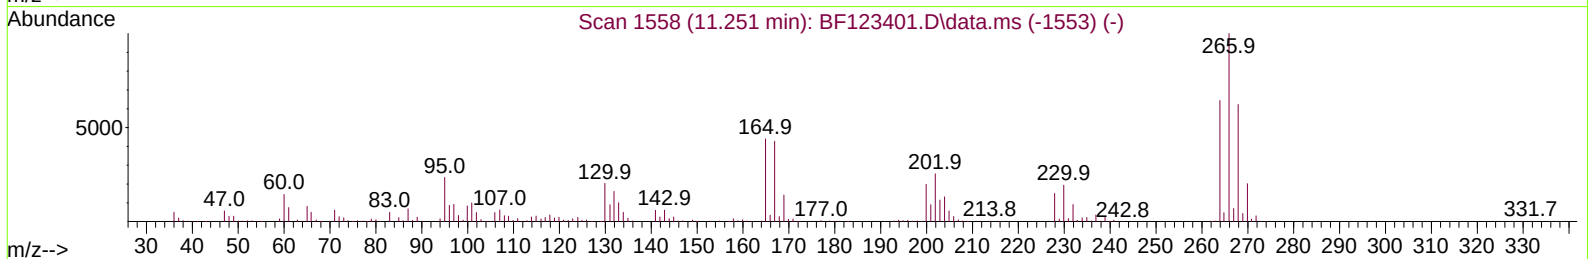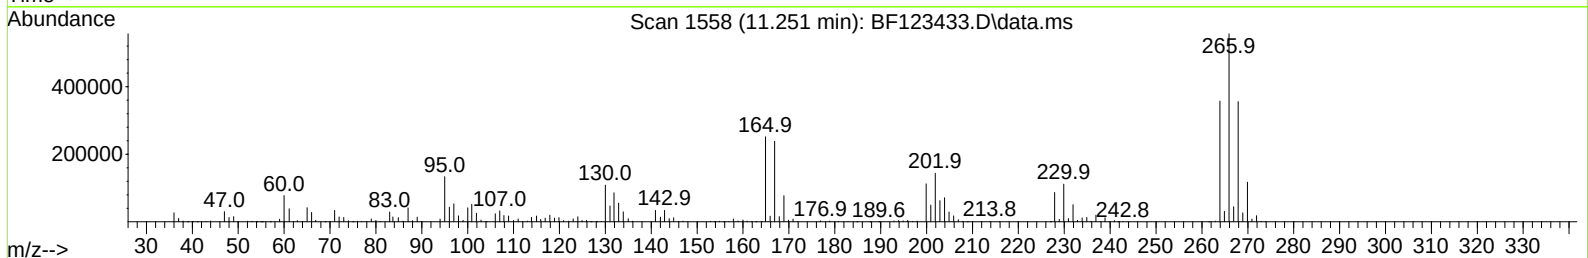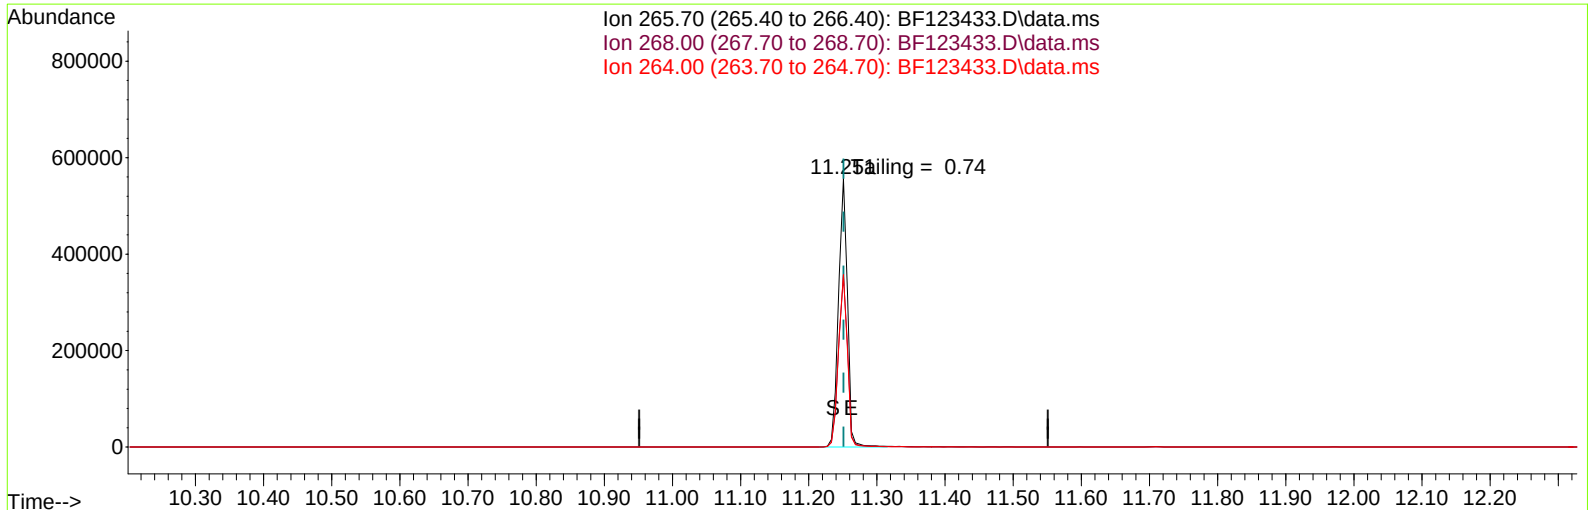

TIC: BF123433.D\data.ms

(70) Pentachlorophenol (C)

11.251min (-0.000) 488653.75 ng




response 506163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.93
264.00	62.30	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032421\
Data File : BF123433.D
Acq On : 24 Mar 2021 11:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 24 12:41:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 23 15:58:35 2021
Response via : Initial Calibration

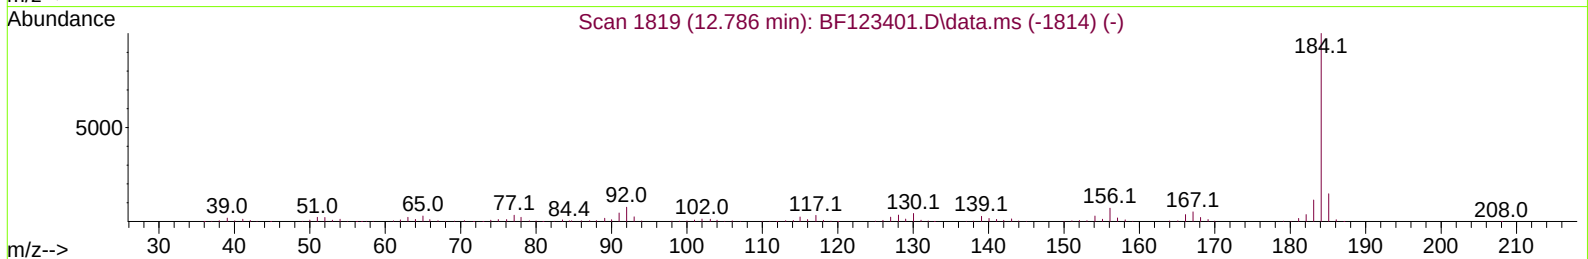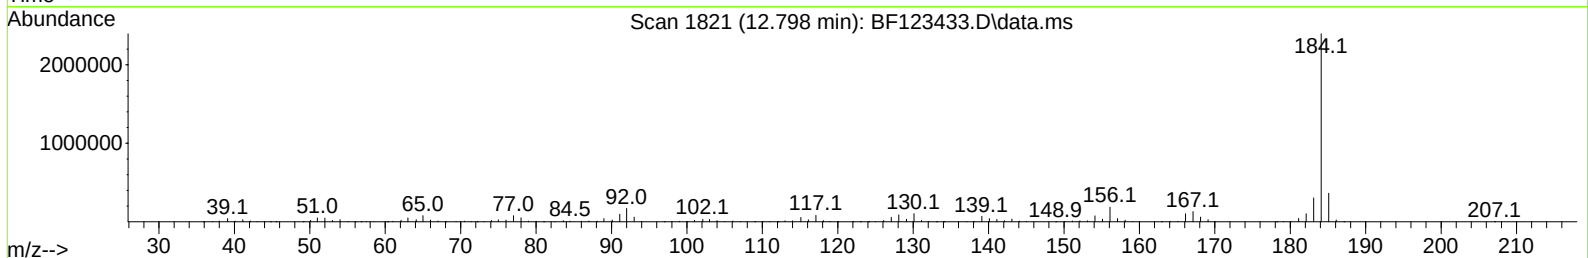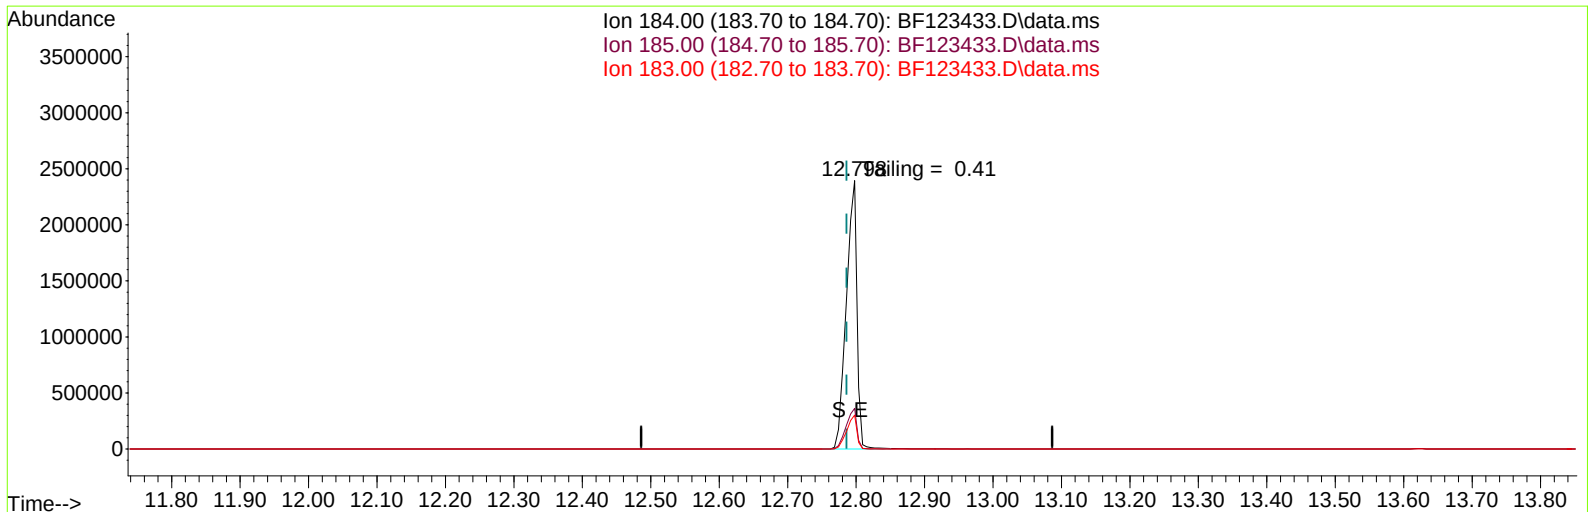

TIC: BF123433.D\data.ms

(77) Benzidine

12.798min (+ 0.011) 4839.63 ng m

response 2587153

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.16
183.00	12.10	12.66
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/24/2021	BNA_F	<u>BF123433.D</u>
Compound Name	Response	Retention Time
DDT	1247764	13.621
DDD	7455	13.351
DDE	3571	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11026	1258790	0.88