
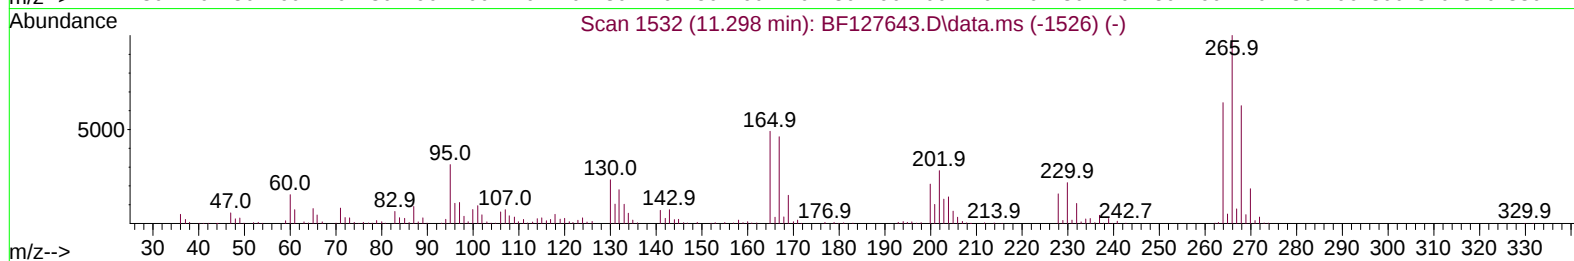
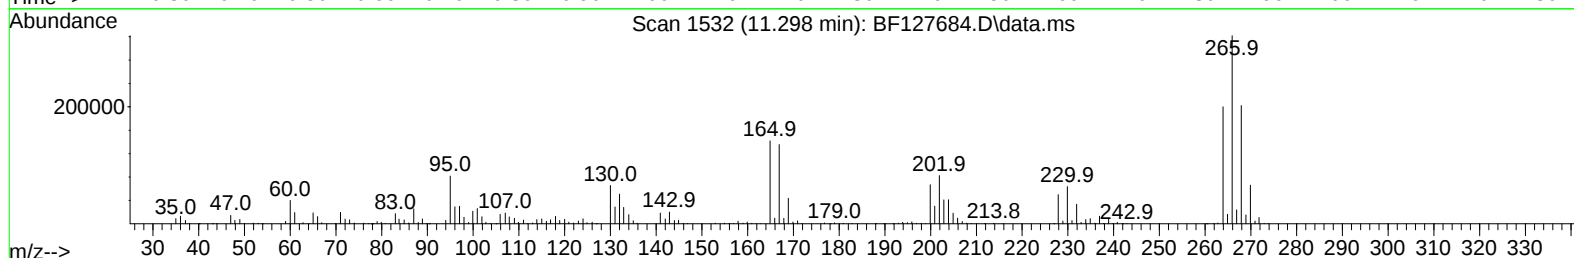


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040722\  
Data File : BF127684.D  
Acq On : 07 Apr 2022 15:22  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 17:02:05 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 06 13:55:27 2022  
Response via : Initial Calibration

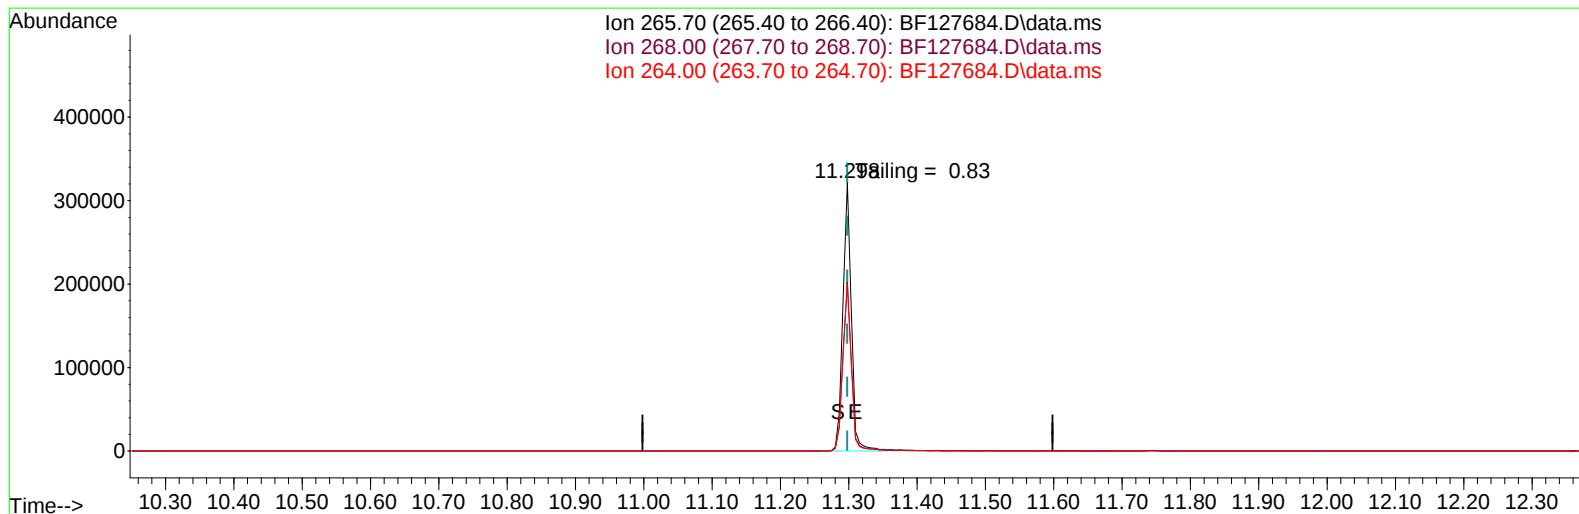

TIC: BF127684.D\data.ms

**(70) Pentachlorophenol (C)**




11.298min (-0.000) 369666.59 ng

response 278267

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 62.92  |
| 264.00 | 60.60  | 62.20  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040722\  
 Data File : BF127684.D  
 Acq On : 07 Apr 2022 15:22  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 17:02:05 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Apr 06 13:55:27 2022  
 Response via : Initial Calibration

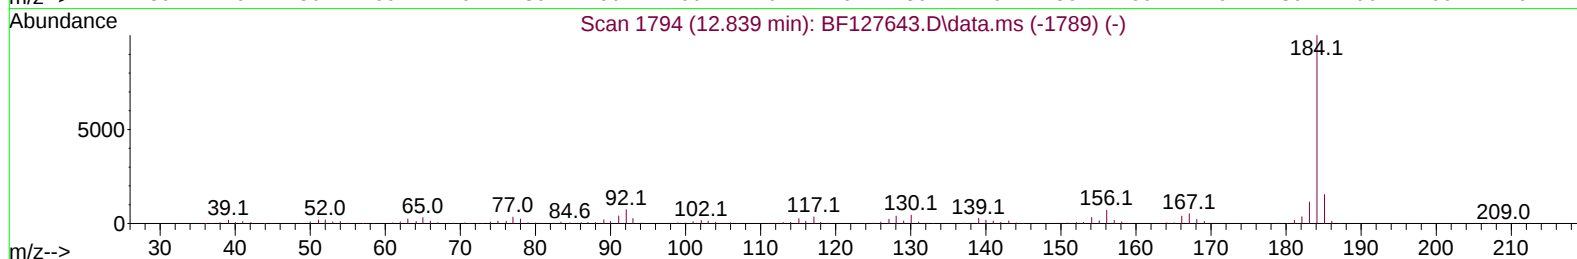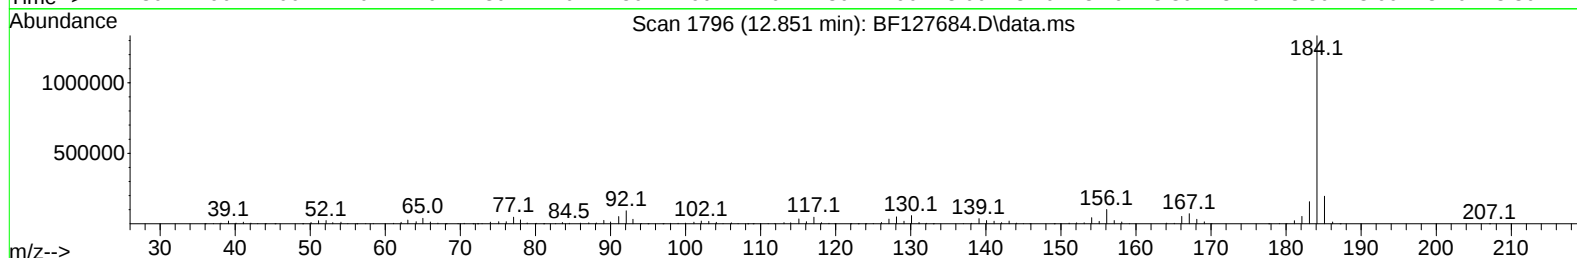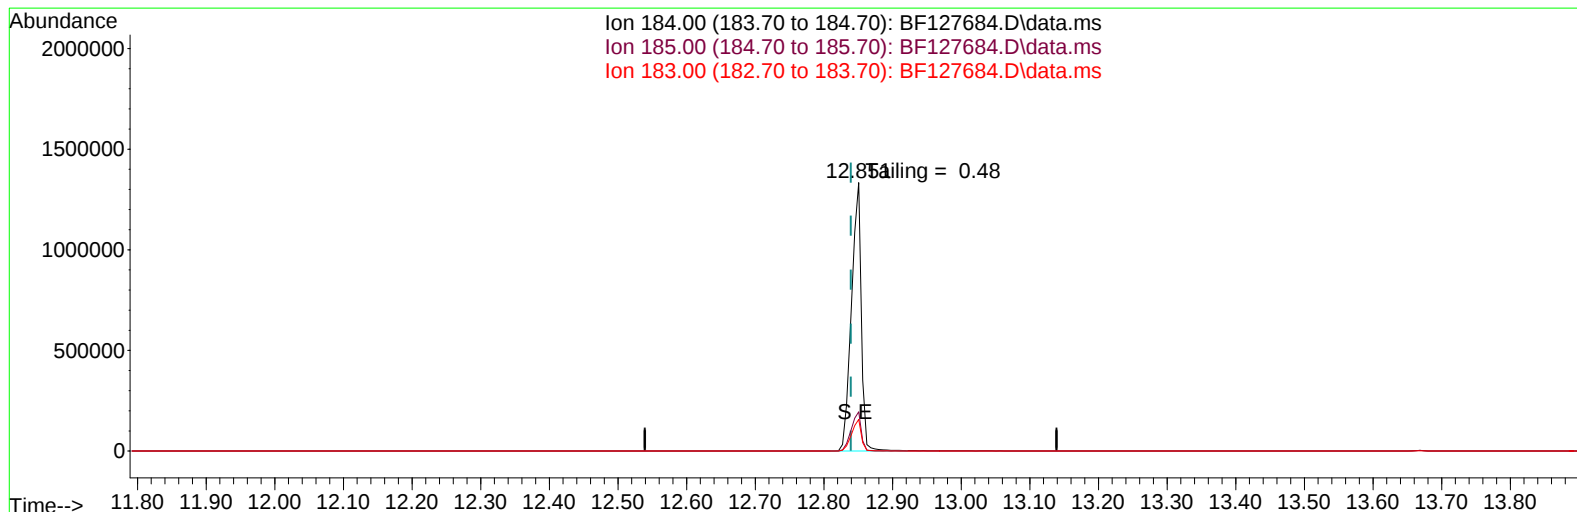

TIC: BF127684.D\data.ms

**(77) Benzidine**

12.851min (+ 0.012) 5528.51 ng m

response 1328119

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.20  | 14.61  |
| 183.00 | 11.70  | 11.77  |
| 0.00   | 0.00   | 0.00   |