

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040722\
 Data File : BF127675.D
 Acq On : 07 Apr 2022 10:44
 Operator : CG\JU
 Sample : PB143932BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143932BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.228	496	500	507	rBV	72748	94981	1.79%	0.309%
2	5.592	556	562	565	rBV	3583764	3776140	71.35%	12.302%
3	6.581	723	730	733	rBV	3259522	3909441	73.87%	12.736%
4	6.963	791	795	798	rBV	1058379	825265	15.59%	2.689%
5	7.528	885	891	894	rBV	2458906	2627612	49.65%	8.560%
6	8.245	1008	1013	1017	rBV	1196706	1066153	20.14%	3.473%
7	9.328	1190	1197	1200	rBV	4966252	4732312	89.42%	15.417%
8	10.010	1307	1313	1316	rBV	1506325	1274478	24.08%	4.152%
9	10.798	1441	1447	1451	rBV	3080734	3288876	62.14%	10.714%
10	11.504	1562	1567	1570	rBV	1442814	1345380	25.42%	4.383%
11	13.098	1832	1838	1841	rBV	5269421	5292431	100.00%	17.241%
12	14.151	2013	2017	2020	rBV	1313797	1189694	22.48%	3.876%
13	15.674	2270	2276	2287	rBV	748071	974903	18.42%	3.176%
14	16.615	2418	2436	2452	rBV3	55368	298376	5.64%	0.972%




Sum of corrected areas: 30696042

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040722\
Data File : BF127675.D
Acq On : 07 Apr 2022 10:44
Operator : CG\JU
Sample : PB143932BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143932BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

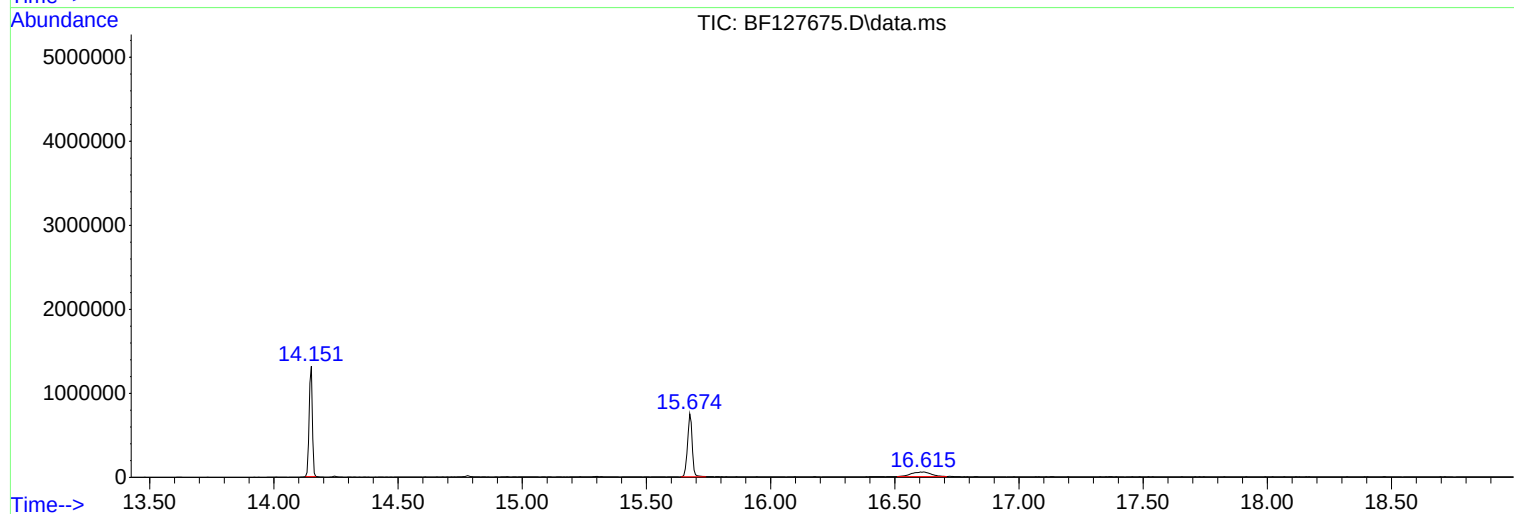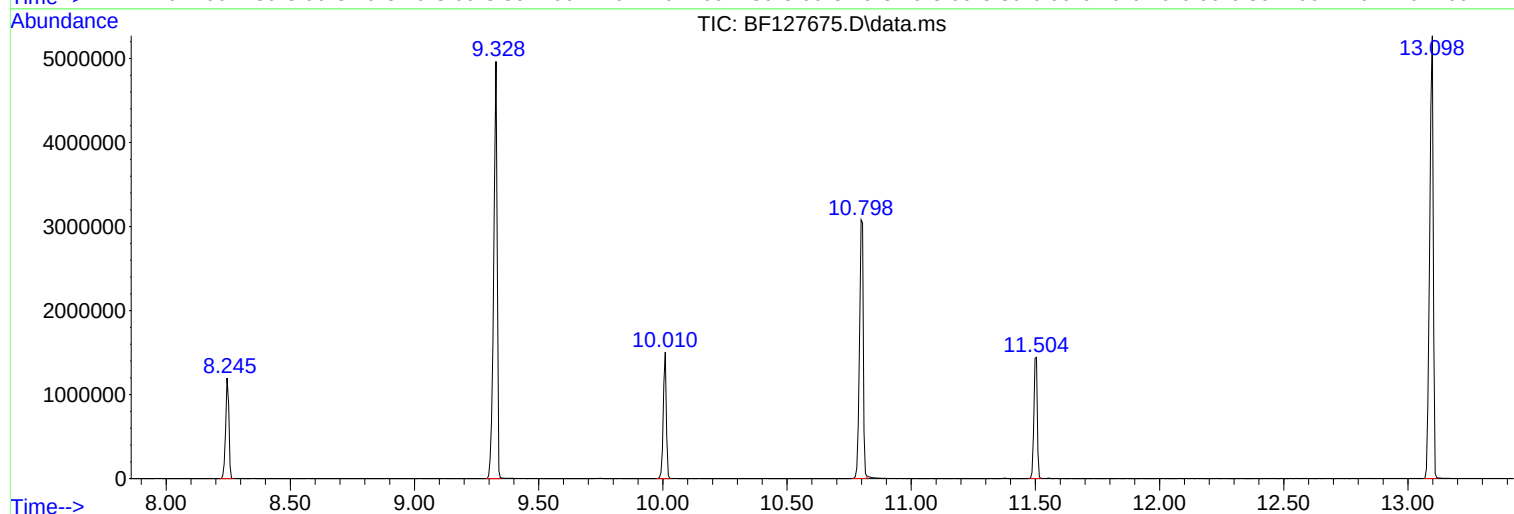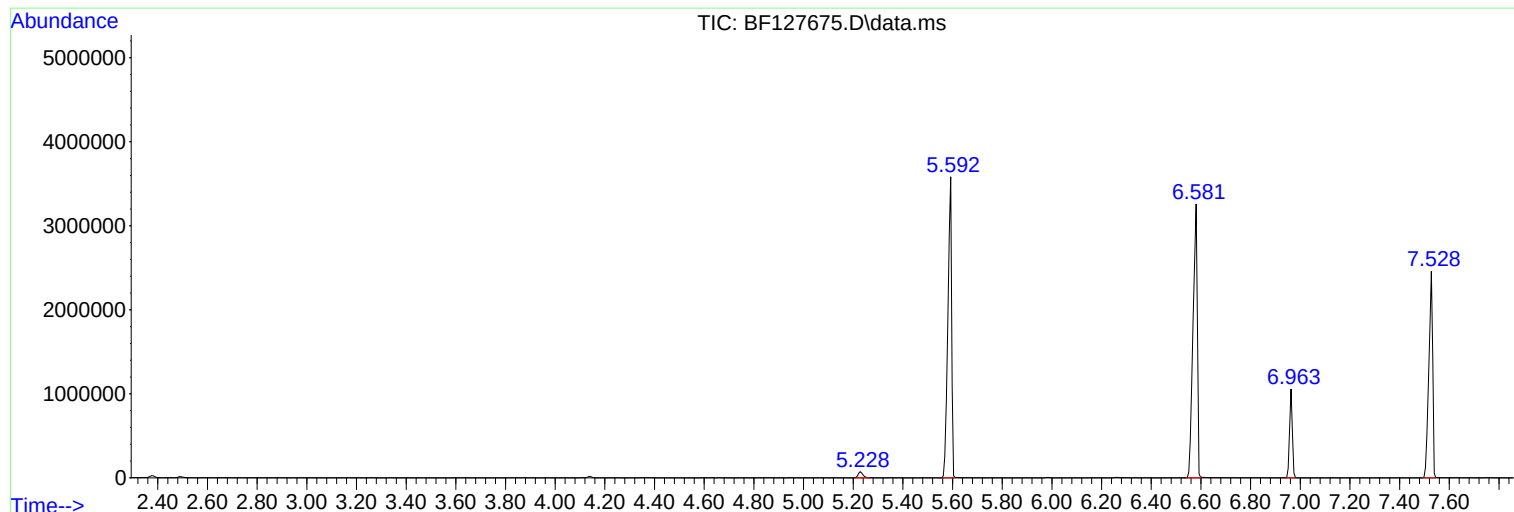

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040722\
Data File : BF127675.D
Acq On : 07 Apr 2022 10:44
Operator : CG\JU
Sample : PB143932BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143932BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040722\
Data File : BF127675.D
Acq On : 07 Apr 2022 10:44
Operator : CG\JU
Sample : PB143932BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143932BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------