

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040722\  
 Data File : BF127683.D  
 Acq On : 07 Apr 2022 14:47  
 Operator : CG\JU  
 Sample : PB143804BL  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB143804BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127683.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.228       | 496           | 500         | 507          | rVB      | 67813          | 88197         | 1.74%           | 0.297%        |
| 2         | 5.593       | 556           | 562         | 565          | rBV      | 3435752        | 3637240       | 71.61%          | 12.238%       |
| 3         | 6.581       | 723           | 730         | 733          | rBV      | 3137770        | 3705953       | 72.97%          | 12.469%       |
| 4         | 6.963       | 791           | 795         | 798          | rBV      | 1097612        | 883160        | 17.39%          | 2.972%        |
| 5         | 7.528       | 885           | 891         | 894          | rBV      | 2603478        | 2748626       | 54.12%          | 9.248%        |
| 6         | 8.245       | 1008          | 1013        | 1017         | rBV      | 1214811        | 1105778       | 21.77%          | 3.721%        |
| 7         | 9.328       | 1190          | 1197        | 1200         | rBV      | 5003025        | 4793483       | 94.38%          | 16.128%       |
| 8         | 10.010      | 1307          | 1313        | 1316         | rBV      | 1434372        | 1273353       | 25.07%          | 4.284%        |
| 9         | 10.798      | 1441          | 1447        | 1451         | rBV      | 3181115        | 3074584       | 60.54%          | 10.345%       |
| 10        | 11.504      | 1562          | 1567        | 1570         | rBV      | 1432231        | 1331089       | 26.21%          | 4.479%        |
| 11        | 13.098      | 1832          | 1838        | 1841         | rBV      | 4964698        | 5078923       | 100.00%         | 17.089%       |
| 12        | 14.151      | 2013          | 2017        | 2020         | rBV      | 1225132        | 1141465       | 22.47%          | 3.841%        |
| 13        | 15.674      | 2270          | 2276        | 2287         | rBV      | 668594         | 858928        | 16.91%          | 2.890%        |




Sum of corrected areas: 29720779

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040722\  
Data File : BF127683.D  
Acq On : 07 Apr 2022 14:47  
Operator : CG\JU  
Sample : PB143804BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB143804BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

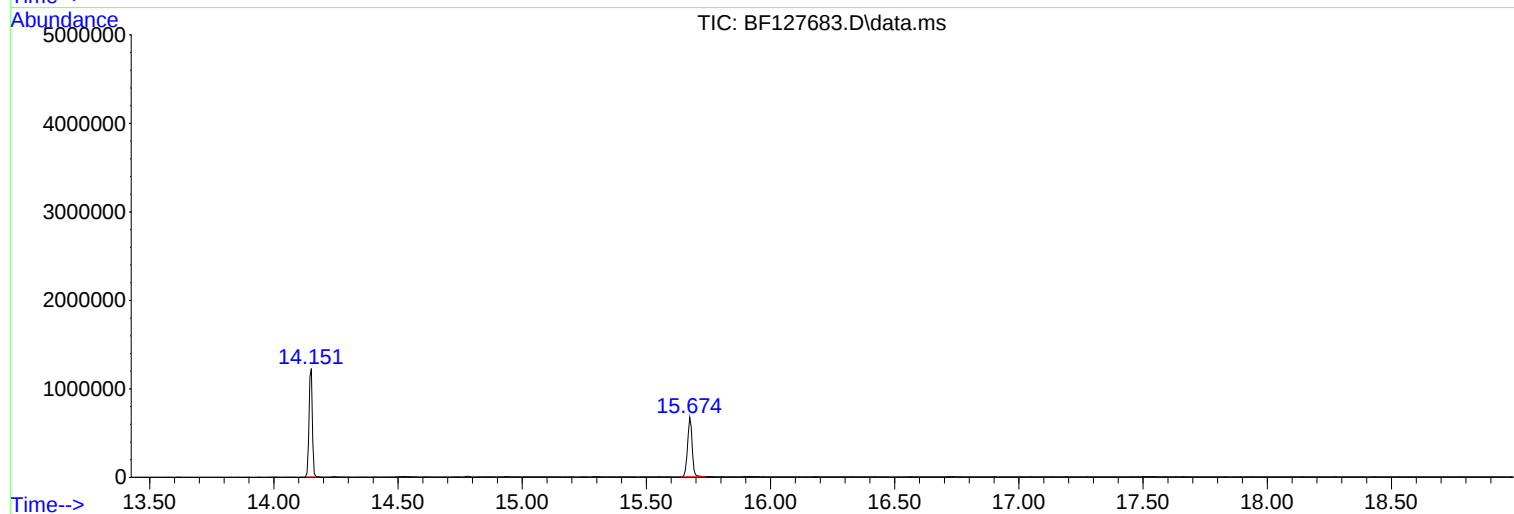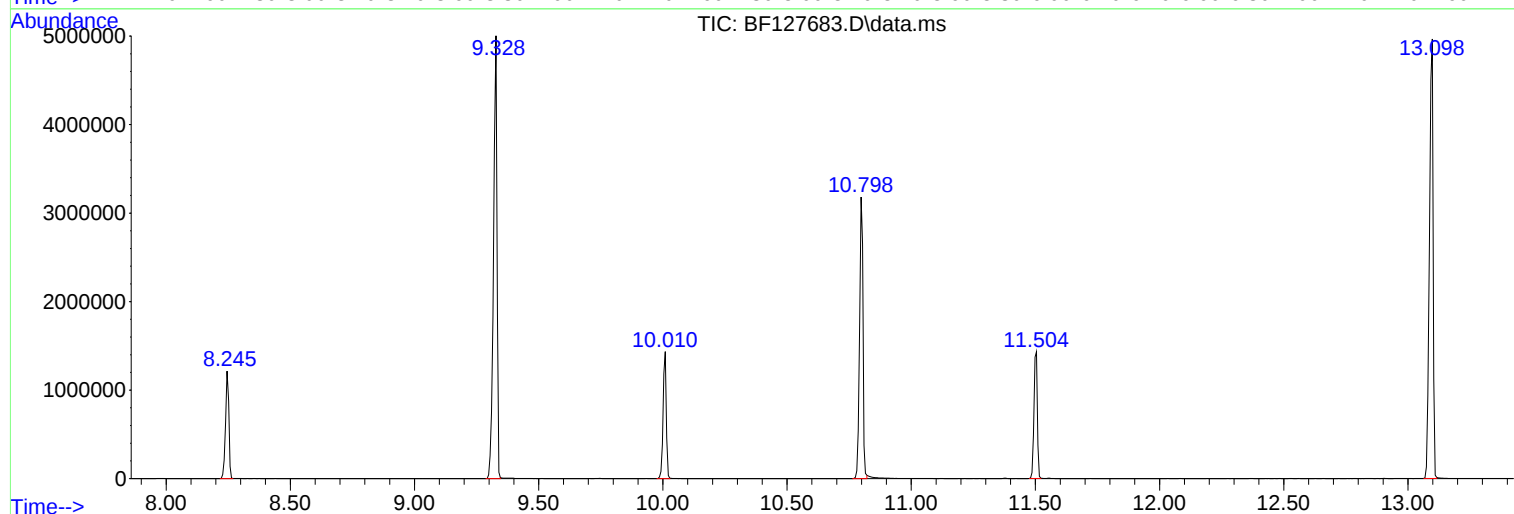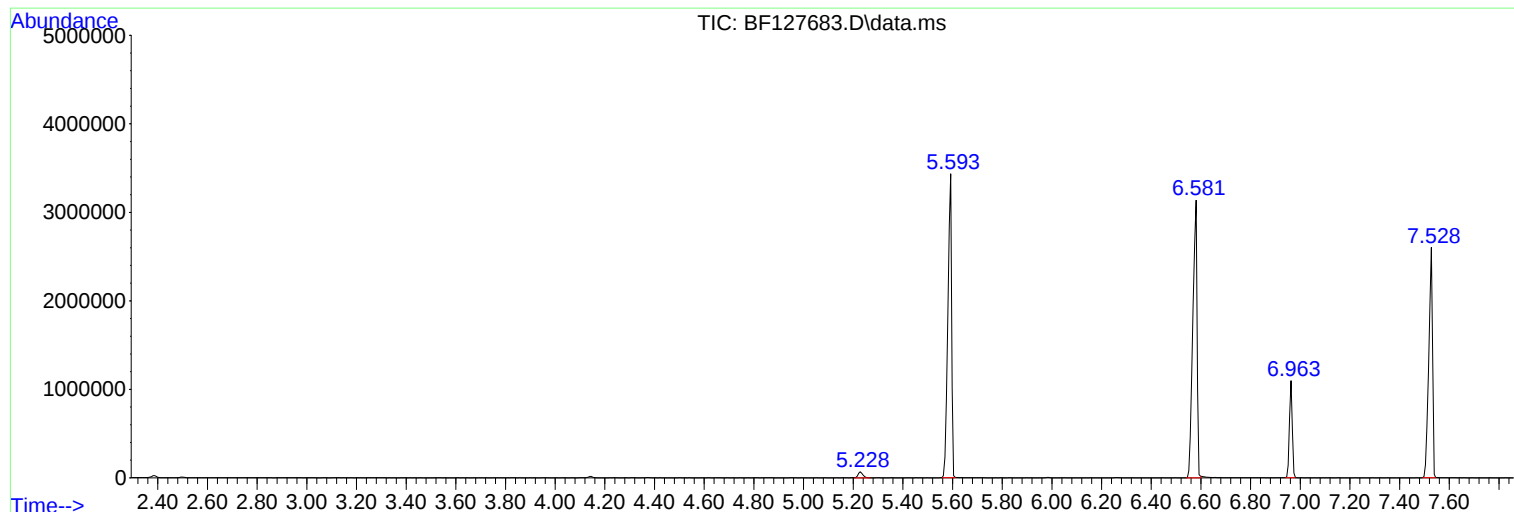

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040722\  
Data File : BF127683.D  
Acq On : 07 Apr 2022 14:47  
Operator : CG\JU  
Sample : PB143804BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB143804BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040722\  
Data File : BF127683.D  
Acq On : 07 Apr 2022 14:47  
Operator : CG\JU  
Sample : PB143804BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB143804BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|