
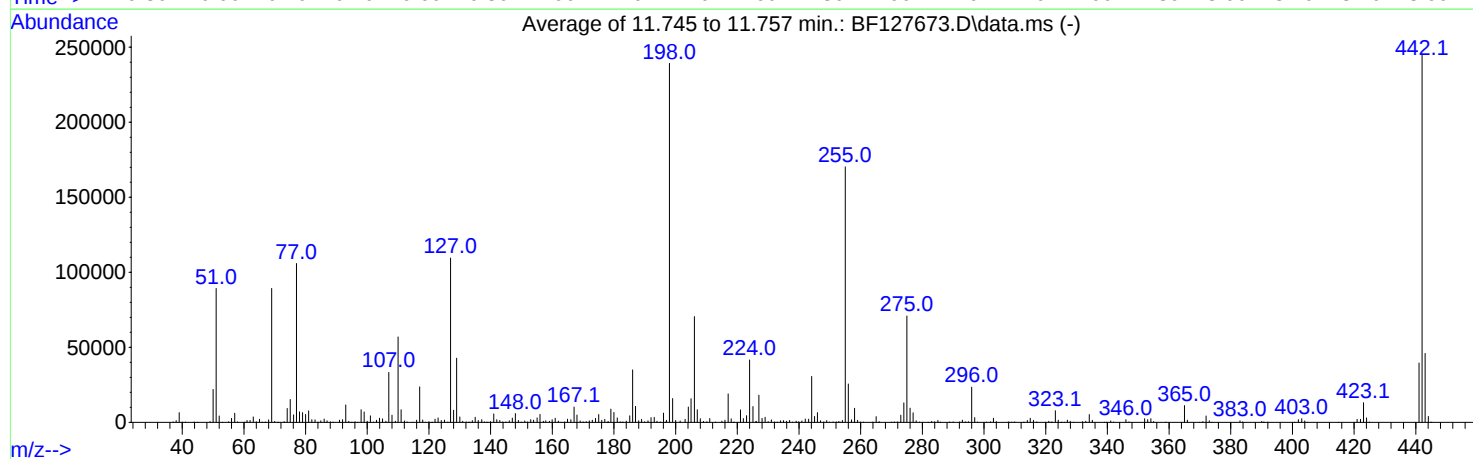


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040722\
 Data File : BF127673.D
 Acq On : 07 Apr 2022 09:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 06 13:55:27 2022

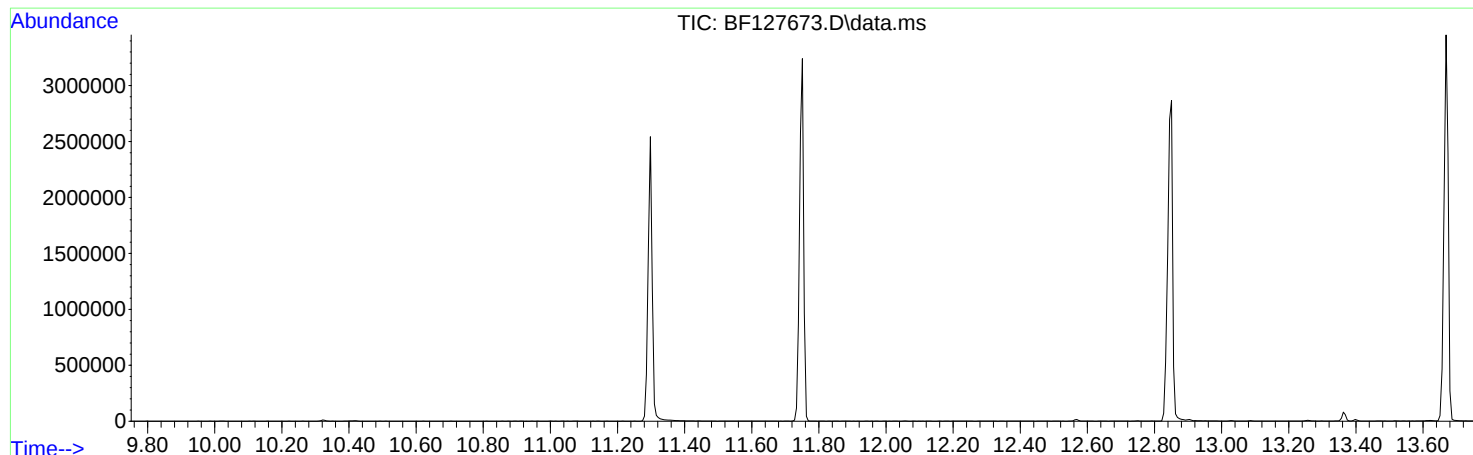


AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	89227	PASS
68	69	0.00	2	1.9	1694	PASS
69	198	0.00	100	37.3	89227	PASS
70	69	0.00	2	0.7	601	PASS
127	198	10	80	45.7	109459	PASS
197	198	0.00	2	0.6	1422	PASS
198	198	100	100	100.0	239269	PASS
199	198	5	9	6.6	15902	PASS
275	198	10	60	29.6	70939	PASS
365	198	1	100	4.7	11252	PASS
441	198	0.01	100	16.6	39611	PASS
442	442	50	100	100.0	245141	PASS
443	442	15	24	18.7	45925	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040722\
 Data File : BF127673.D
 Acq On : 07 Apr 2022 09:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 07 17:05:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 06 13:55:27 2022
 Response via : Initial Calibration

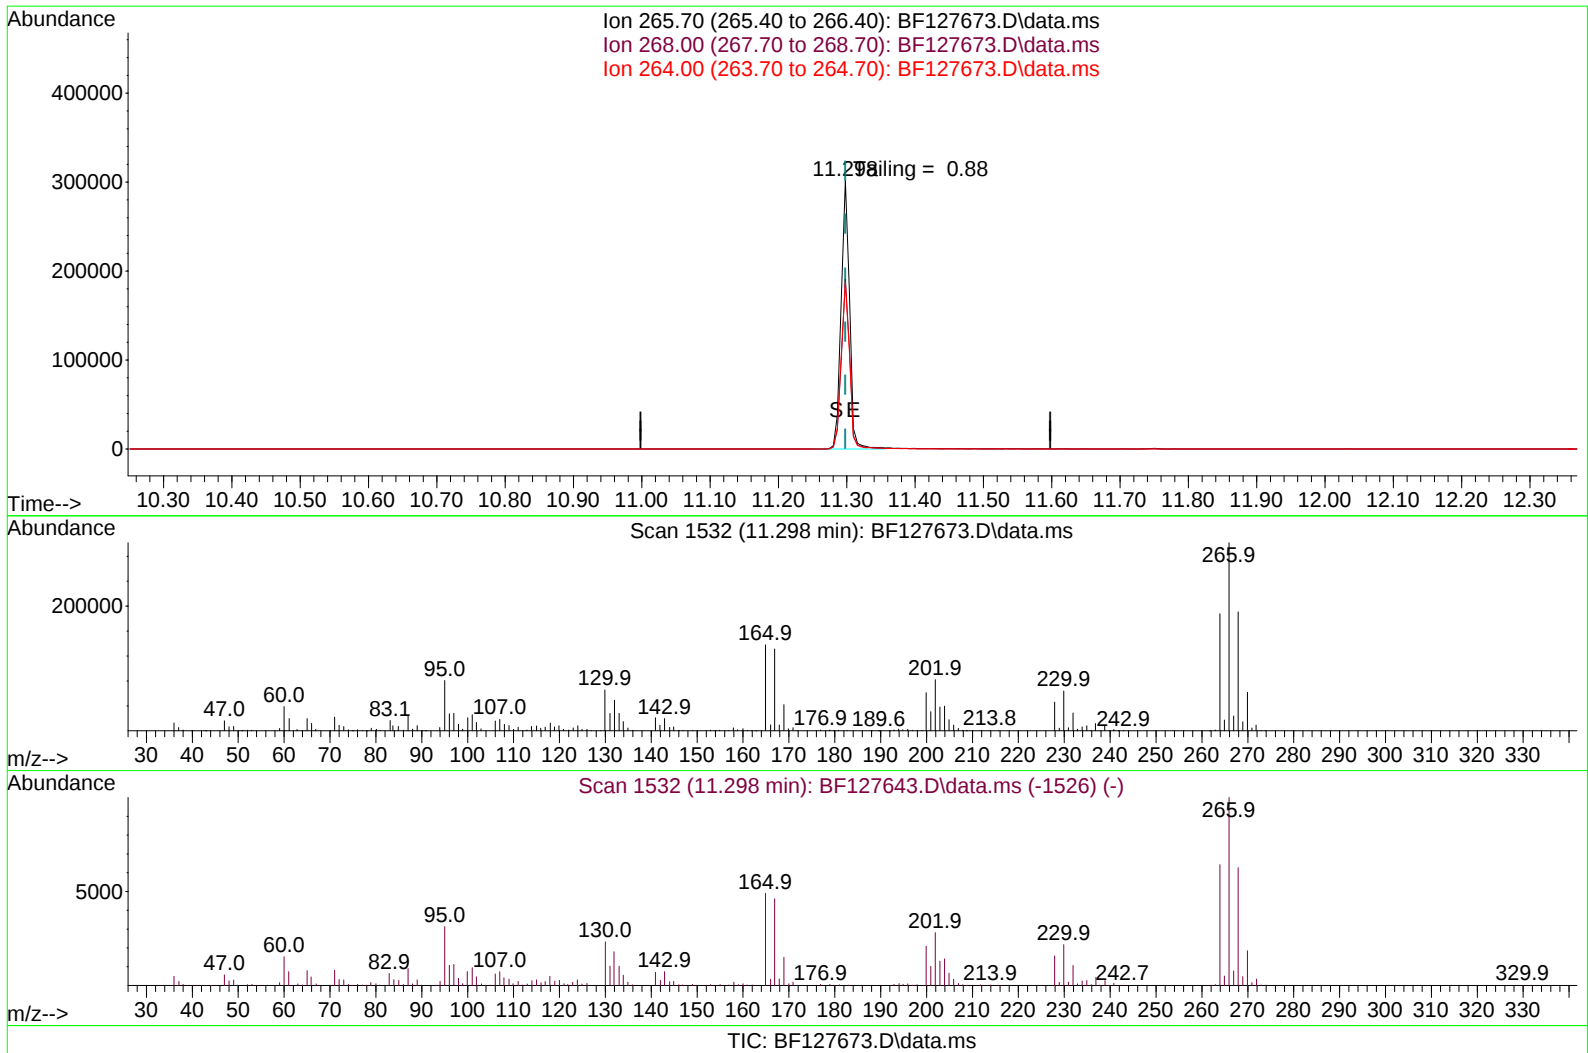

(70) Pentachlorophenol (C)

11.298min (-0.000) 392502.53 ng




response 261246

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.22
264.00	60.60	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040722\
Data File : BF127673.D
Acq On : 07 Apr 2022 09:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 07 17:05:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 13:55:27 2022
Response via : Initial Calibration

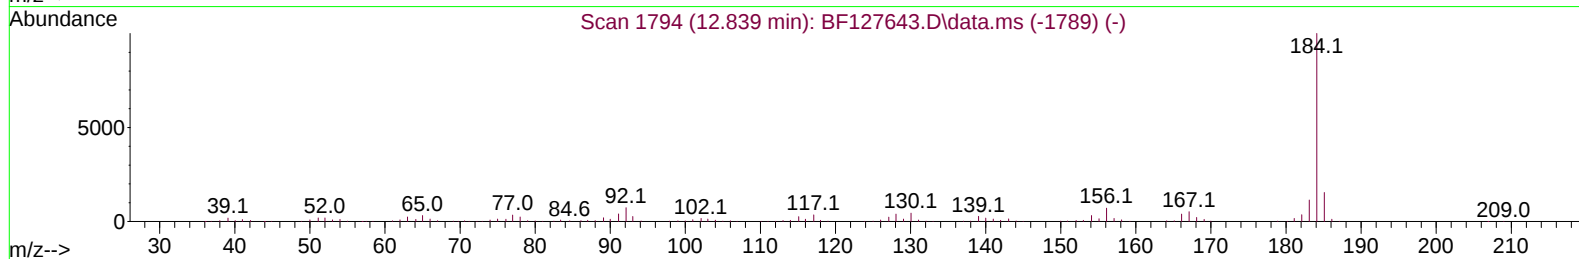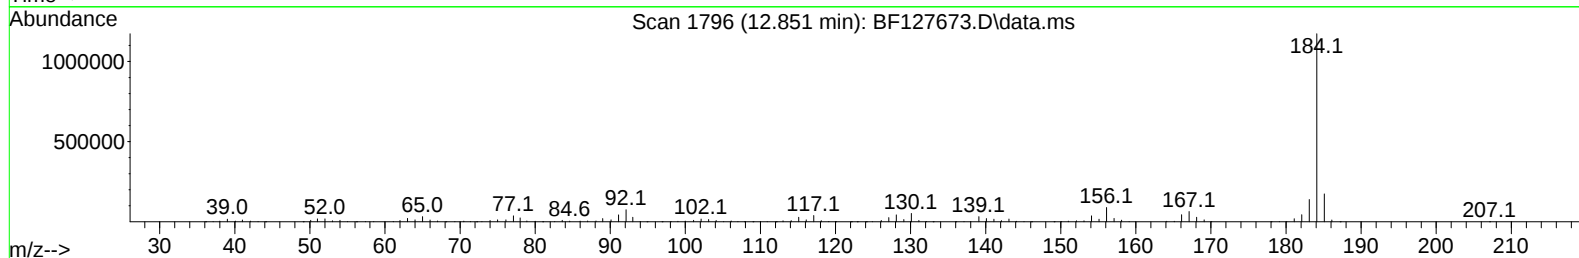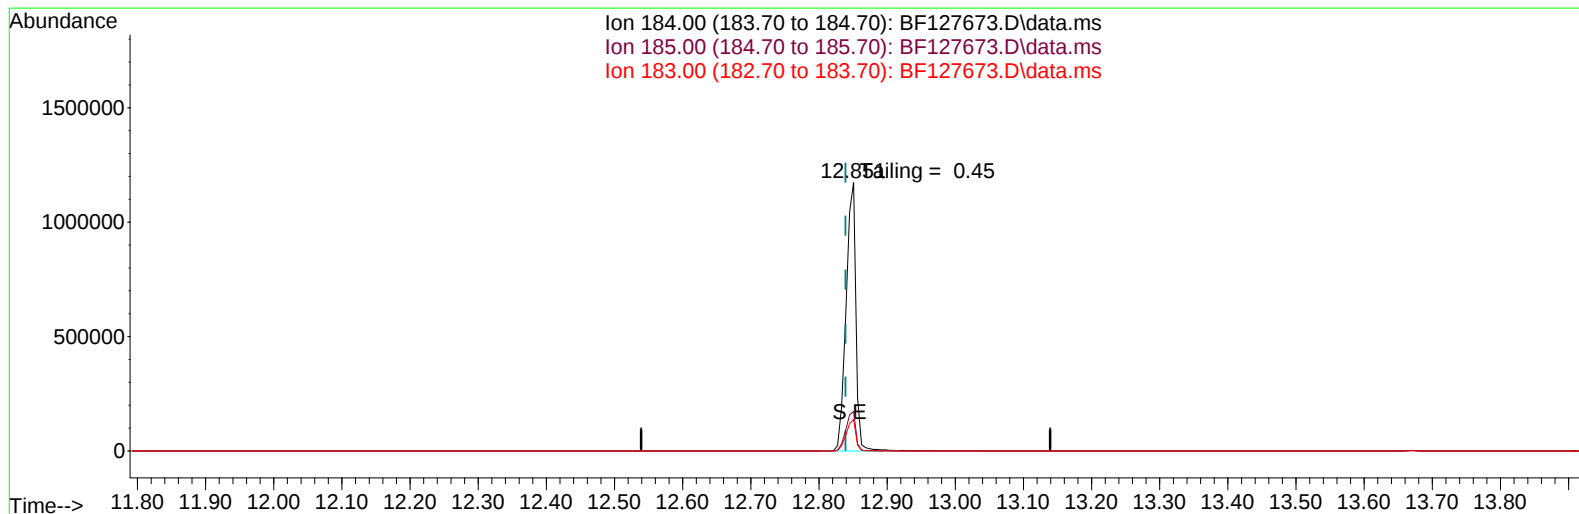

TIC: BF127673.D\data.ms

(77) Benzidine

12.851min (+ 0.012) 5065.52 ng m

response 1175114

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.80
183.00	11.70	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/7/2022	BNA_F	<u>BF127673.D</u>
Compound Name	Response	Retention Time
DDT	582118	13.66
DDD	13276	13.36
DDE	649	13.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13925	596043	2.34

Instrument :
BNA_F
ClientSampleId :
DFTPP