
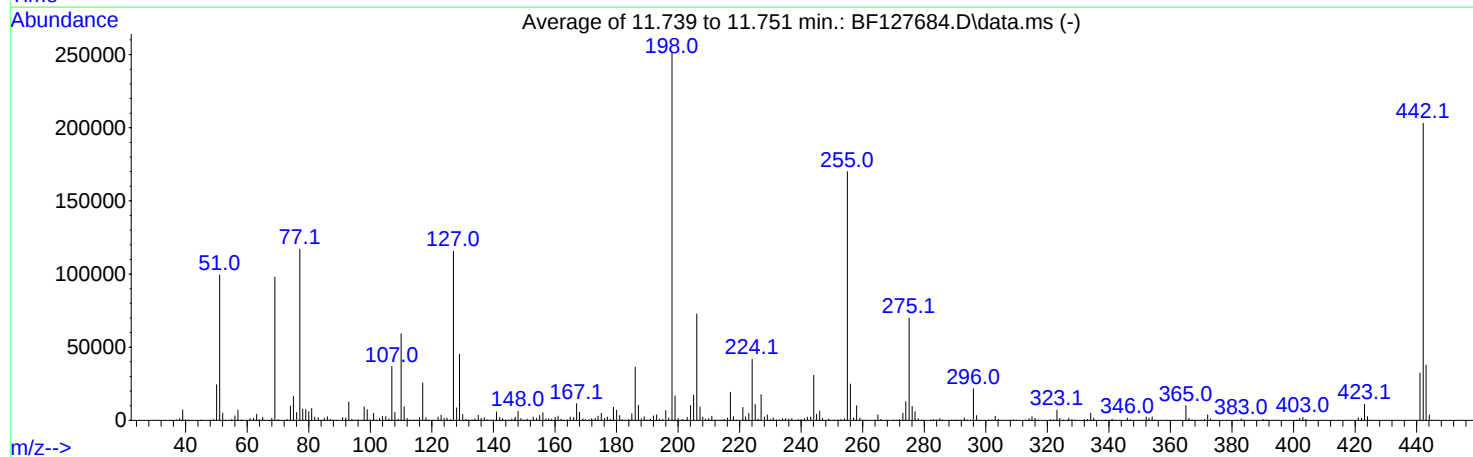


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040722\  
 Data File : BF127684.D  
 Acq On : 07 Apr 2022 15:22  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Apr 06 13:55:27 2022

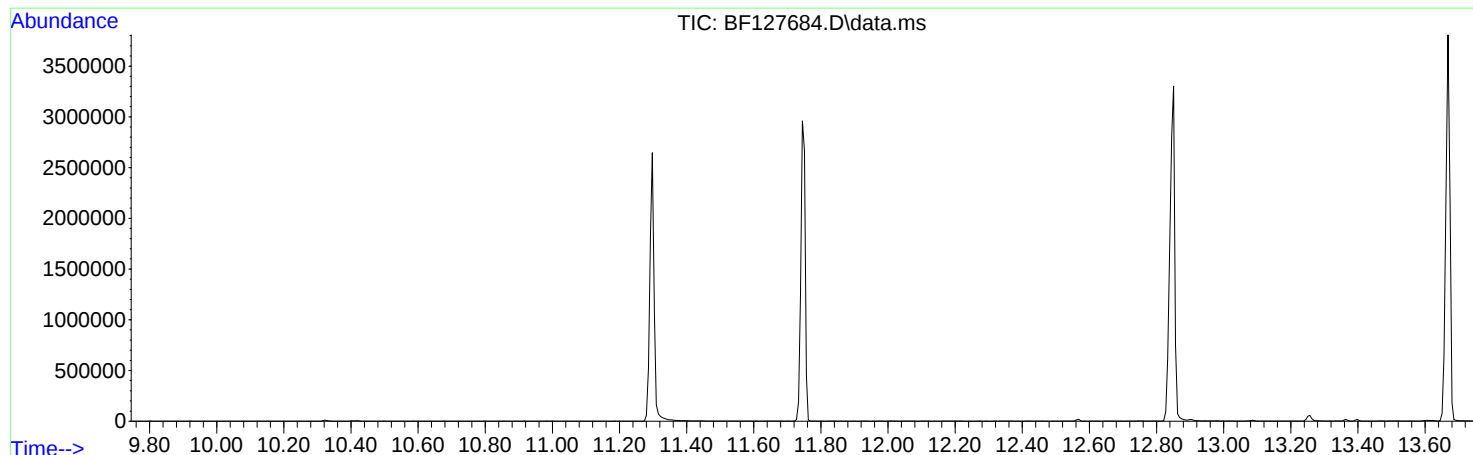




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 39.5         | 99416      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 1486       | PASS                |
| 69             | 198             | 0.00            | 100             | 38.9         | 97872      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 565        | PASS                |
| 127            | 198             | 10              | 80              | 46.0         | 115555     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.7          | 1788       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 251413     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 16729      | PASS                |
| 275            | 198             | 10              | 60              | 27.7         | 69749      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 10207      | PASS                |
| 441            | 198             | 0.01            | 100             | 12.9         | 32354      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 203133     | PASS                |
| 443            | 442             | 15              | 24              | 18.6         | 37774      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040722\  
Data File : BF127684.D  
Acq On : 07 Apr 2022 15:22  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Apr 07 17:02:05 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 06 13:55:27 2022  
Response via : Initial Calibration

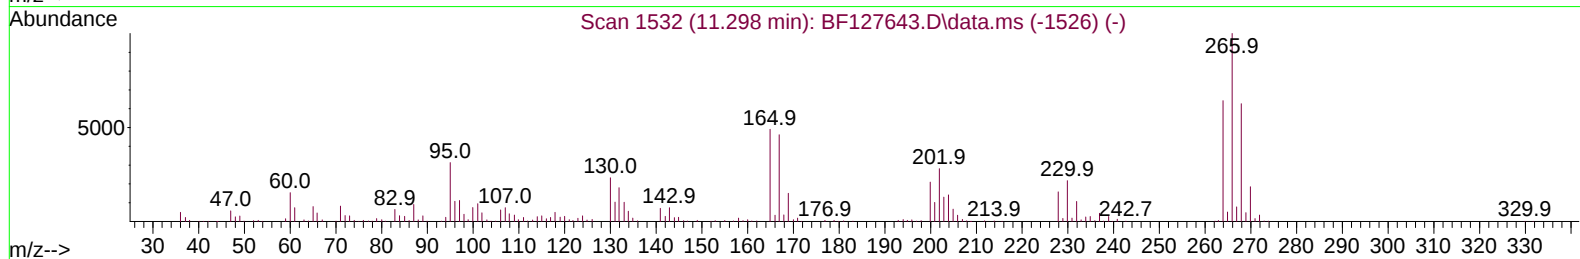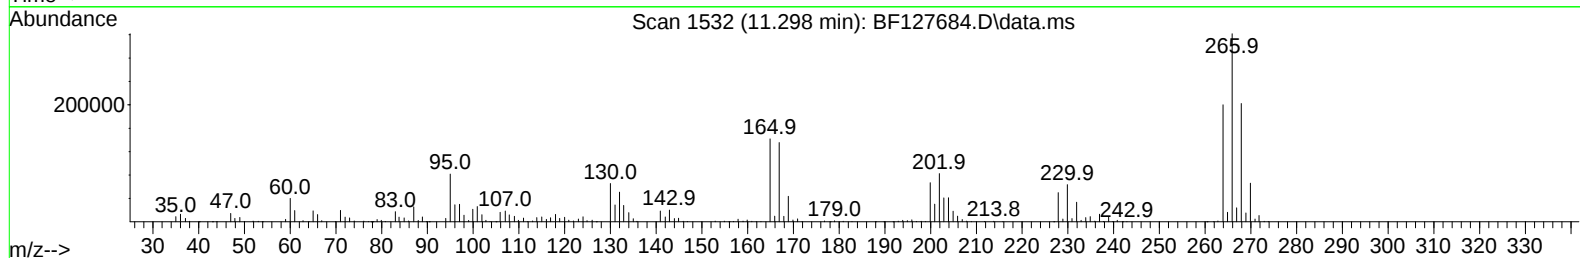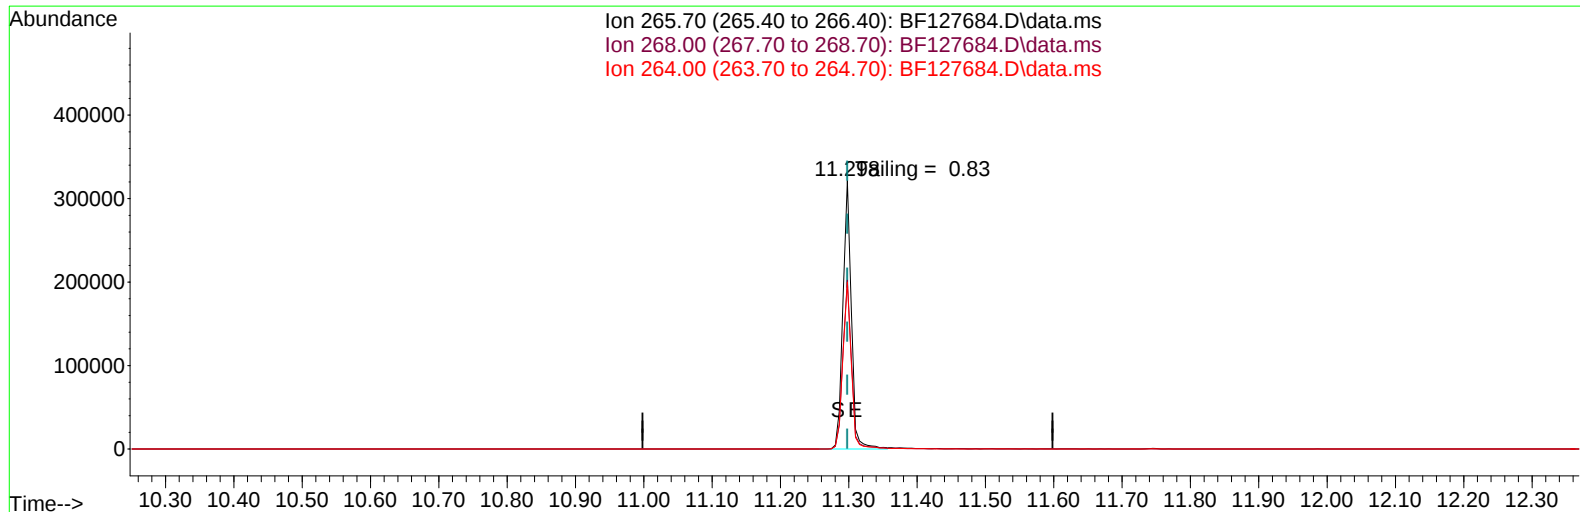

TIC: BF127684.D\data.ms

**(70) Pentachlorophenol (C)**

**11.298min (-0.000) 369666.59 ng**




**response 278267**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 62.92  |
| 264.00 | 60.60  | 62.20  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040722\  
Data File : BF127684.D  
Acq On : 07 Apr 2022 15:22  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Apr 07 17:02:05 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 06 13:55:27 2022  
Response via : Initial Calibration

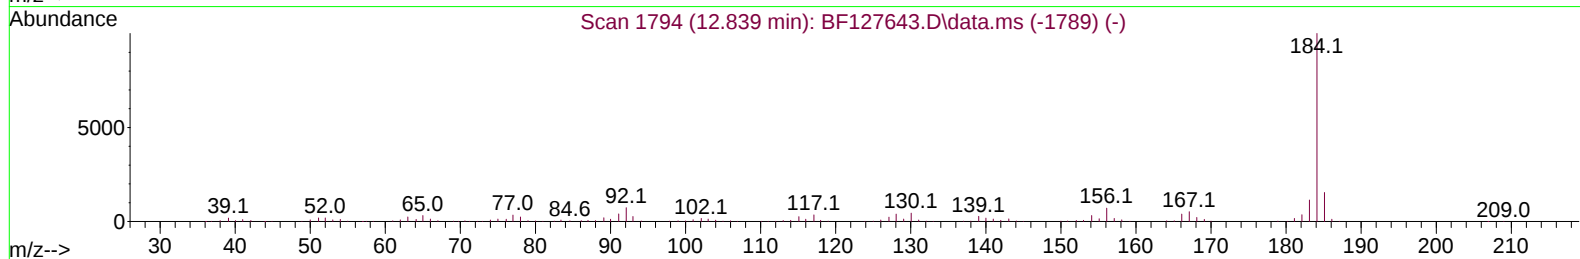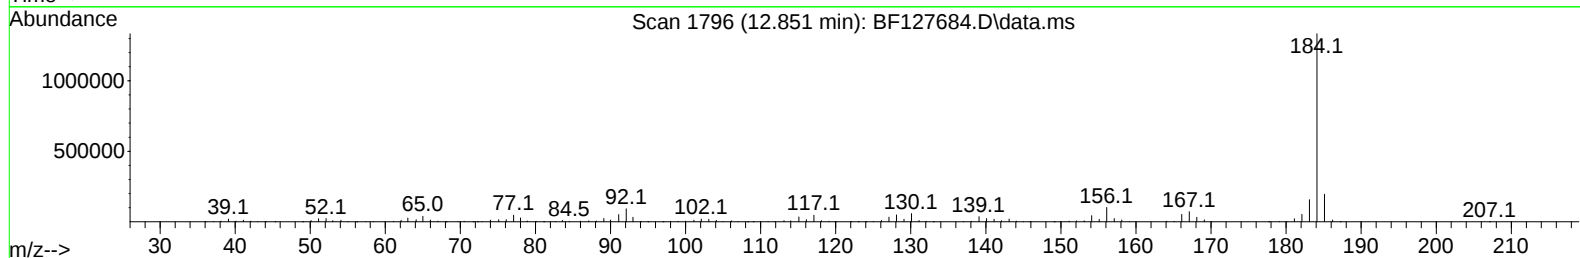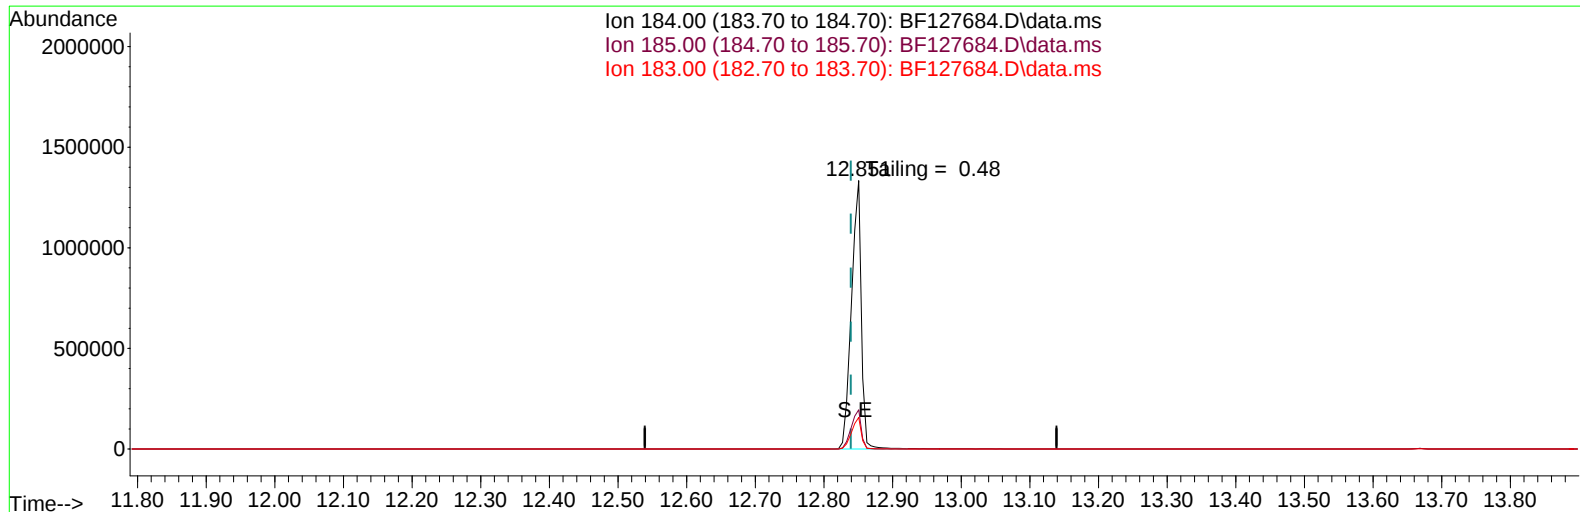

TIC: BF127684.D\data.ms

(77) Benzidine

12.851min (+ 0.012) 5528.51 ng m

response 1328119

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.20  | 14.61  |
| 183.00 | 11.70  | 11.77  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/7/2022      | BNA_F            | <u>BF127684.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 625857           | 13.66              |
| DDD           | 3039             | 13.36              |
| DDE           | 278              | 13.02              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3317          | 629174           | 0.53               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP