
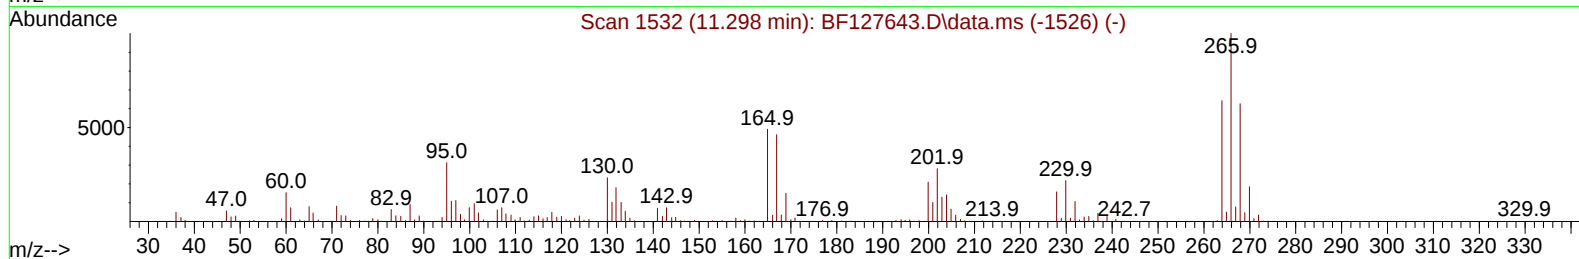
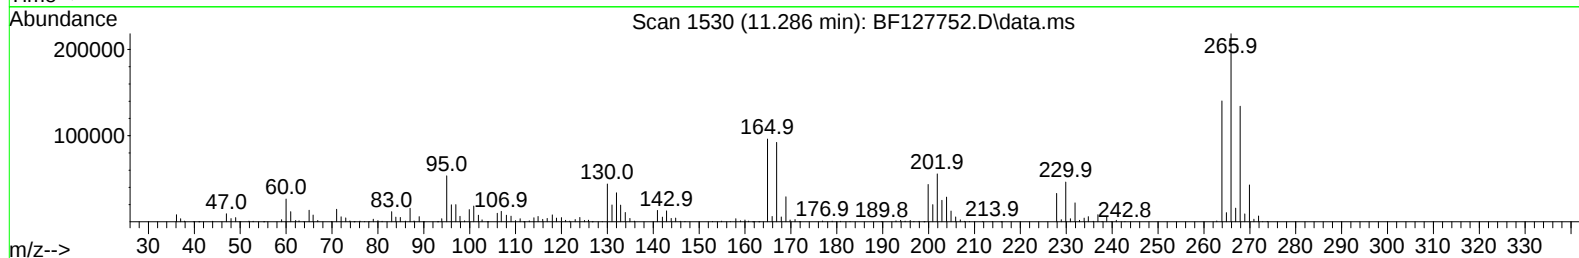


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
Data File : BF127752.D
Acq On : 12 Apr 2022 11:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:52:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 07:19:18 2022
Response via : Initial Calibration

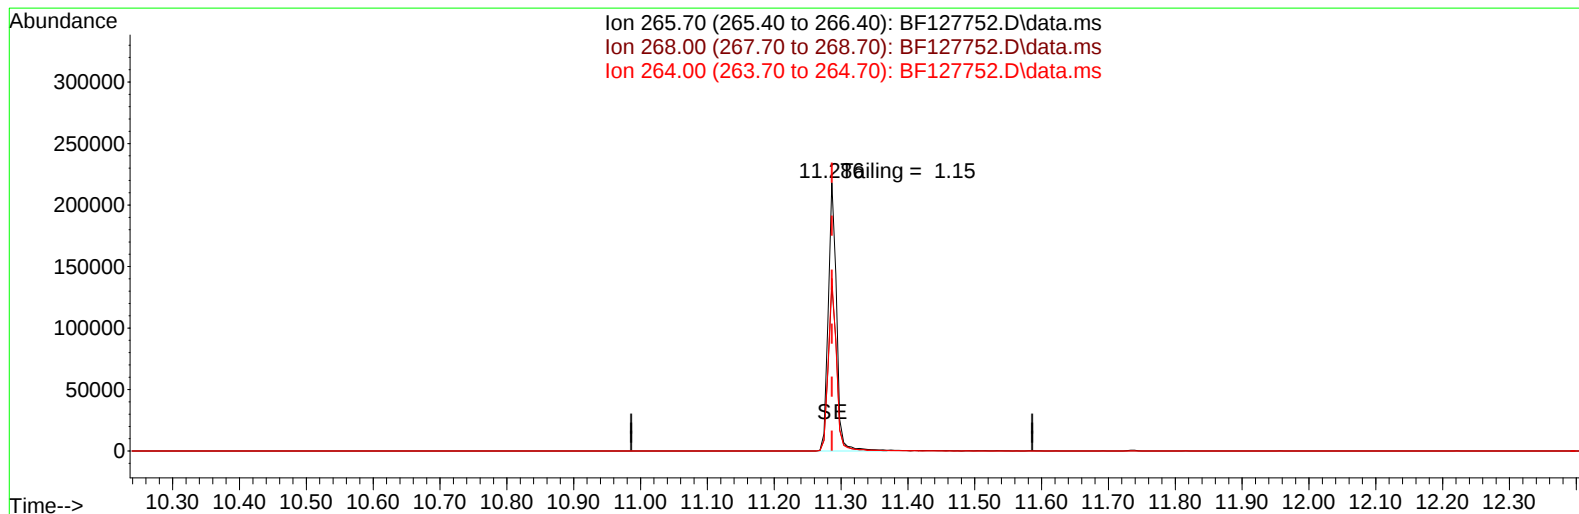

TIC: BF127752.D\data.ms

(70) Pentachlorophenol (C)




11.286min (-0.000) 25958.29 ng m

response 187791

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.47
264.00	60.60	64.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
 Data File : BF127752.D
 Acq On : 12 Apr 2022 11:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:52:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 07:19:18 2022
 Response via : Initial Calibration

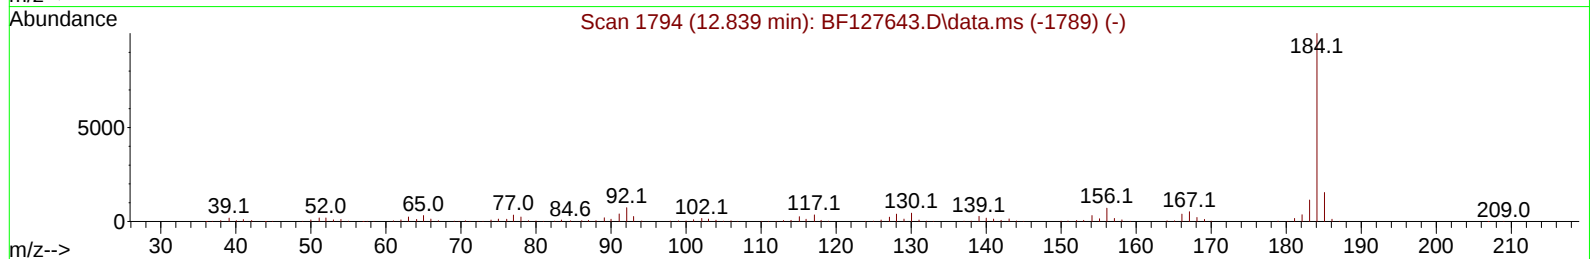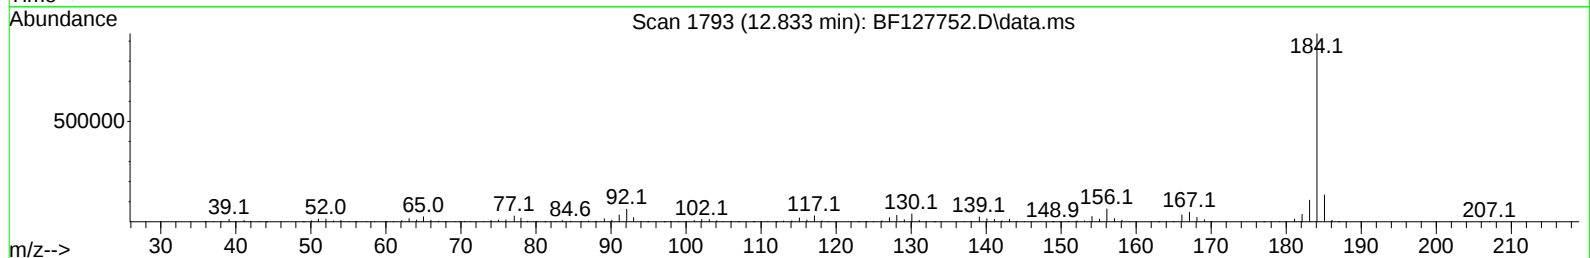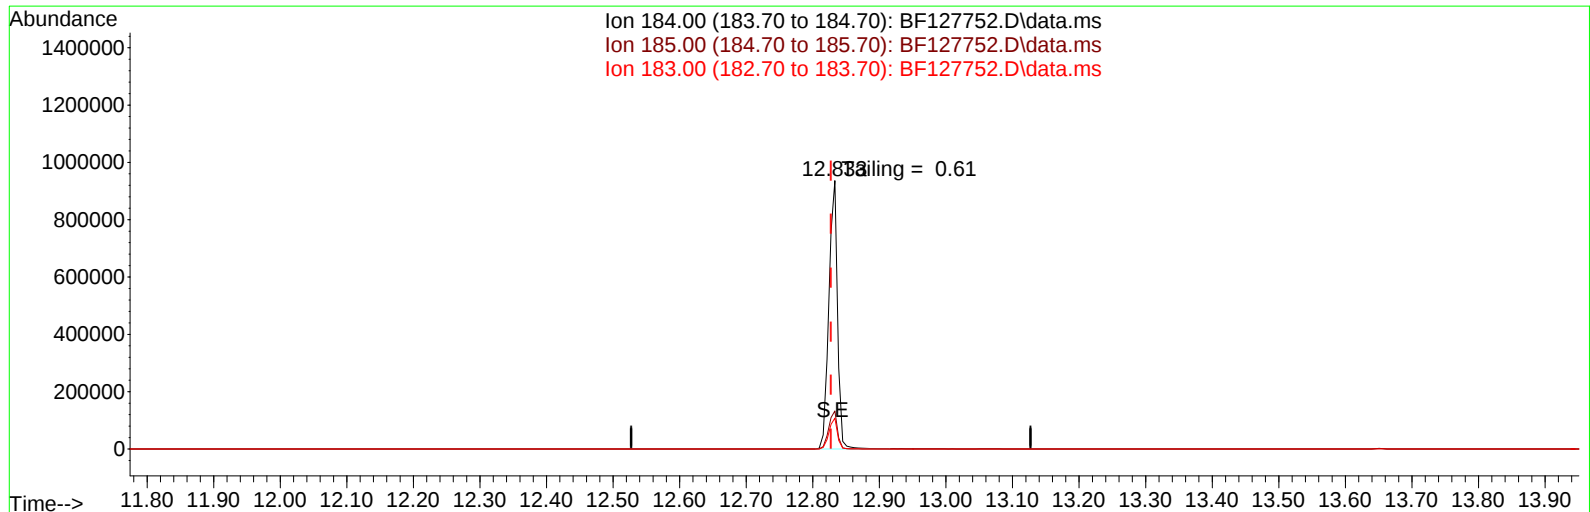

TIC: BF127752.D\data.ms

(77) Benzidine

12.833min (+ 0.006) 0.00 ng

response 851690

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.23
183.00	11.70	11.54
0.00	0.00	0.00