

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
 Data File : BF127758.D
 Acq On : 12 Apr 2022 15:05
 Operator : CG\JU
 Sample : N2340-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP-08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.575	555	559	562	rBV	1276940	1146208	24.19%	5.124%
2	6.563	724	727	731	rBV	791947	710405	14.99%	3.176%
3	6.957	790	794	797	rBV	955892	769837	16.25%	3.442%
4	7.004	799	802	811	rBV	39817	56832	1.20%	0.254%
5	7.522	884	890	893	rBV	2619105	2592010	54.71%	11.588%
6	8.239	1008	1012	1015	rBV	1185356	991358	20.92%	4.432%
7	9.316	1190	1195	1198	rBV	5141603	4738113	100.00%	21.183%
8	9.998	1307	1311	1314	rBV	1484181	1179336	24.89%	5.272%
9	10.786	1441	1445	1448	rBV	2529416	2164955	45.69%	9.679%
10	11.486	1561	1564	1568	rBV	1358343	1229660	25.95%	5.497%
11	13.080	1830	1835	1838	rBV	4926627	4585444	96.78%	20.500%
12	13.998	1987	1991	2004	rBV4	78710	175734	3.71%	0.786%
13	14.133	2010	2014	2018	rVB	1136674	953416	20.12%	4.262%
14	14.227	2025	2030	2038	rBV	155210	160846	3.39%	0.719%
15	15.657	2267	2273	2281	rVB	685778	913578	19.28%	4.084%




Sum of corrected areas: 22367732

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
Data File : BF127758.D
Acq On : 12 Apr 2022 15:05
Operator : CG\JU
Sample : N2340-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

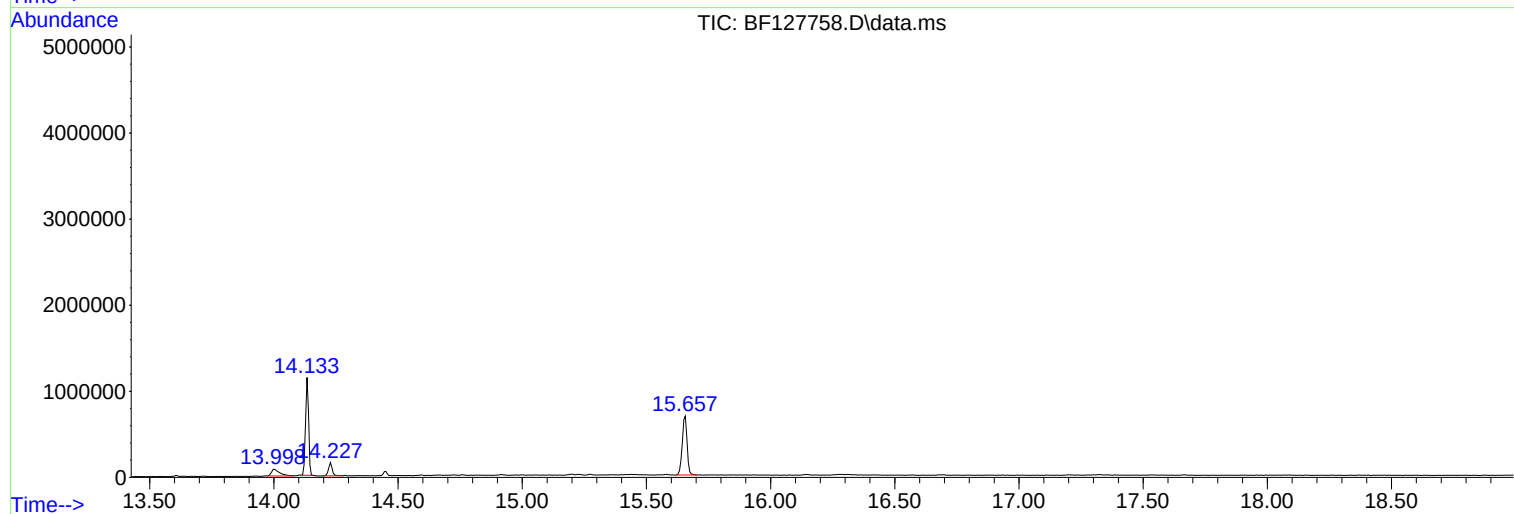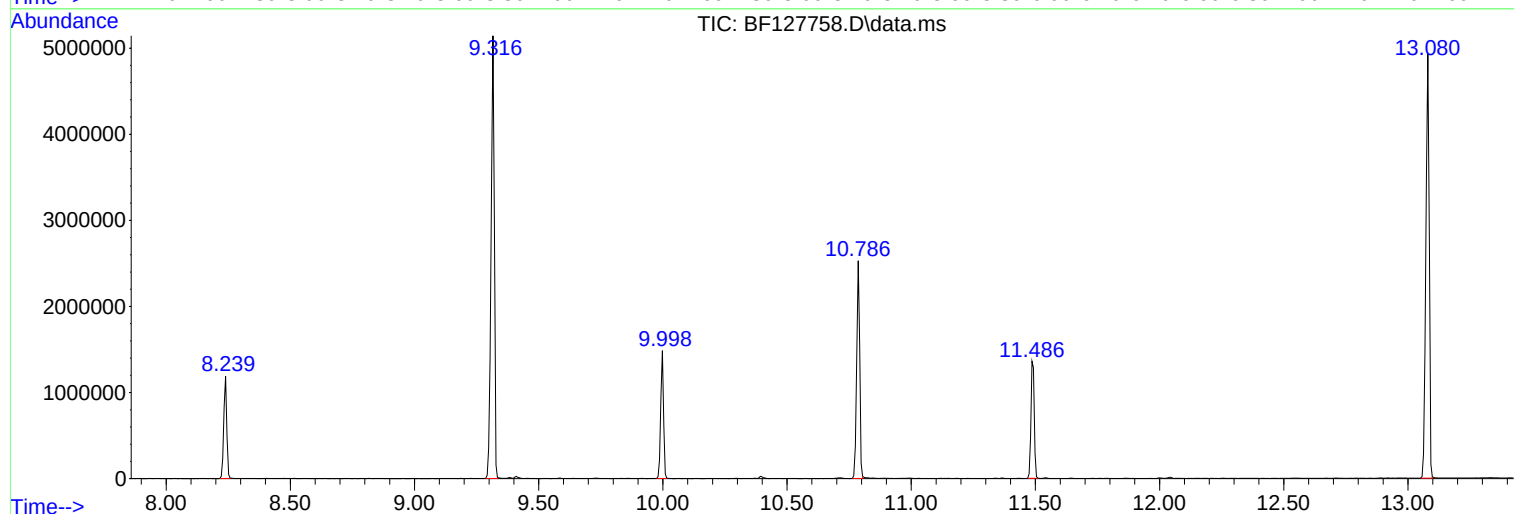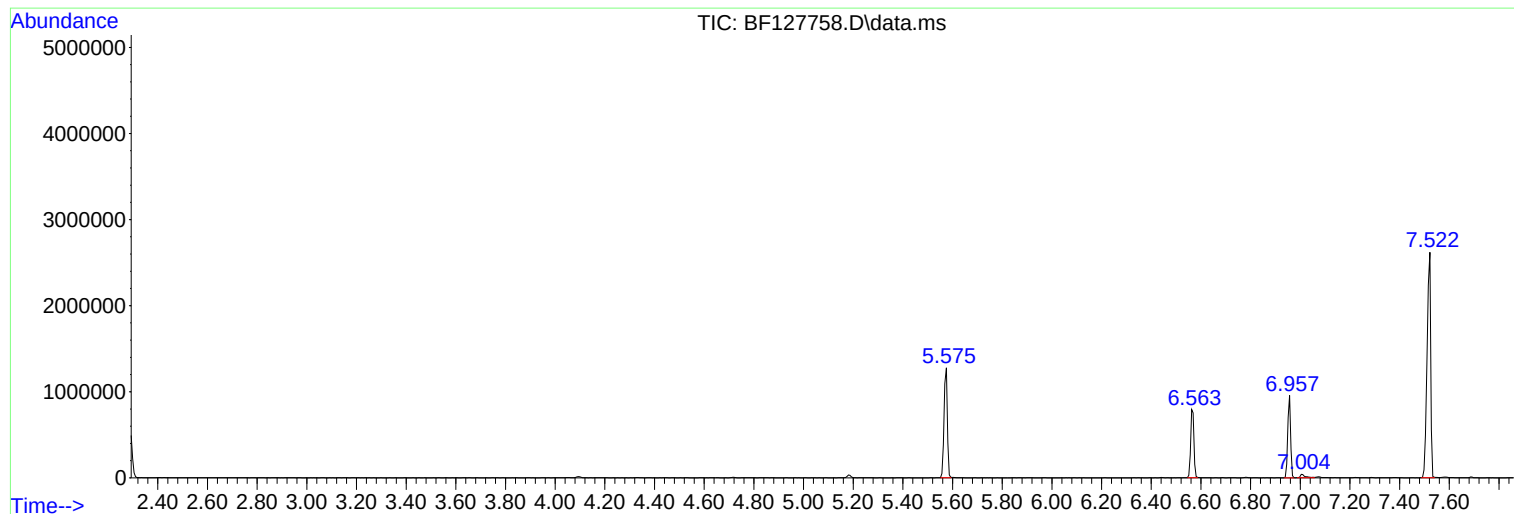

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
Data File : BF127758.D
Acq On : 12 Apr 2022 15:05
Operator : CG\JU
Sample : N2340-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP-08










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Behenic alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.998	3.69 ng	175734	Chrysene-d12	14.133

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Behenic alcohol	326	C22H46O	000661-19-8	93
2			1-Heneicosanol	312	C21H44O	015594-90-8	93
3			n-Nonadecanol-1	284	C19H40O	001454-84-8	93
4			n-Tetracosanol-1	354	C24H50O	000506-51-4	91
5			1-Hexacosanol	382	C26H54O	000506-52-5	81

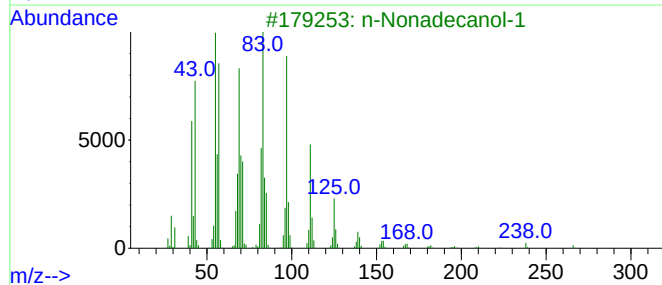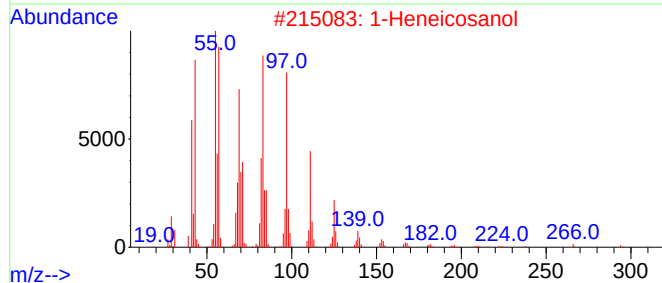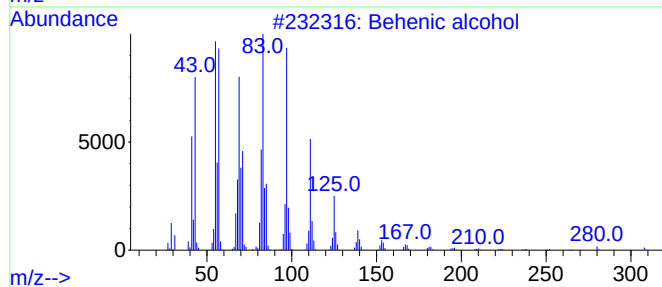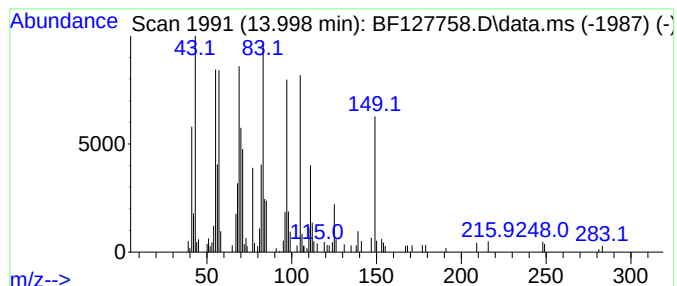

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
Data File : BF127758.D
Acq On : 12 Apr 2022 15:05
Operator : CG\JU
Sample : N2340-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP-08










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.227	3.37 ng	160846	Chrysene-d12	14.133

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			1H-Indole-3-acetic acid, 5-[(tri...	277	C14H19NO3Si	072101-35-0	32
5			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	28

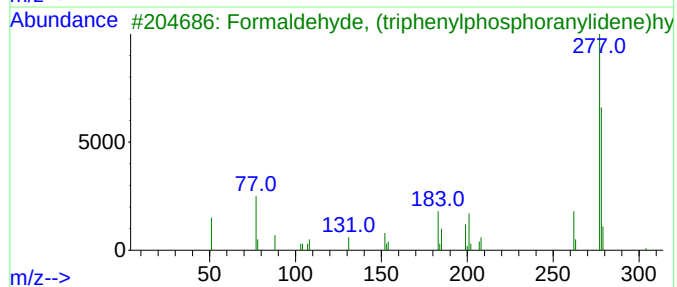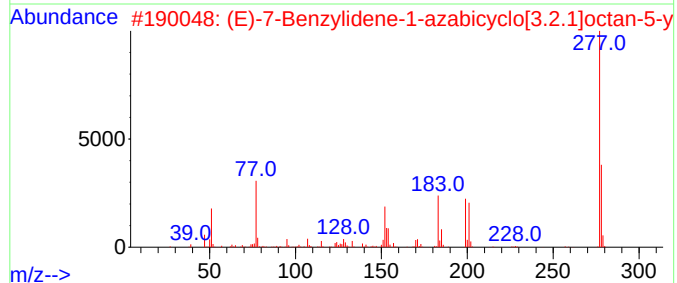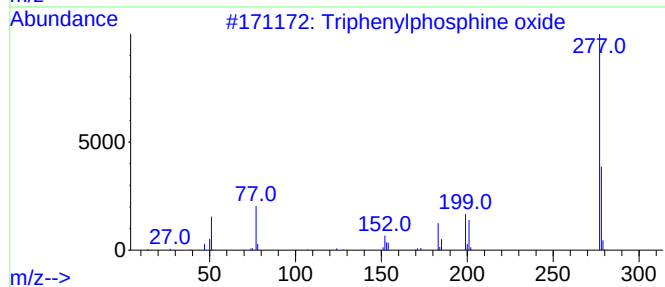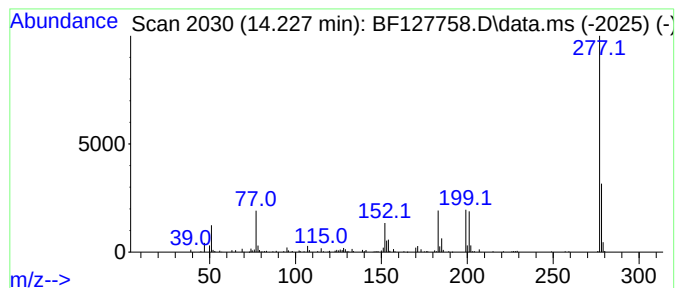

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
Data File : BF127758.D
Acq On : 12 Apr 2022 15:05
Operator : CG\JU
Sample : N2340-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Behenic alcohol	13.998	3.7	ng	175734	5	14.133	953416	20.0
Triphenylphosph...	14.227	3.4	ng	160846	5	14.133	953416	20.0