

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
 Data File : BF127768.D
 Acq On : 12 Apr 2022 20:01
 Operator : CG\JU
 Sample : N2334-07 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-19R

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.075	299	304	310	rVB3	11154	14551	1.33%	0.151%
2	5.175	487	491	494	rBV	17935	17109	1.57%	0.177%
3	5.563	554	557	561	rBV	398359	355352	32.53%	3.683%
4	6.563	724	727	735	rVB	274335	223440	20.45%	2.316%
5	6.957	790	794	797	rBV	903563	763190	69.86%	7.910%
6	7.516	884	889	892	rBV	596776	548189	50.18%	5.682%
7	8.239	1007	1012	1015	rBV	1152757	945198	86.52%	9.797%
8	9.310	1190	1194	1197	rBV	1410614	1092400	100.00%	11.322%
9	9.998	1307	1311	1314	rBV	1296736	1069169	97.87%	11.082%
10	10.780	1441	1444	1448	rBV	725399	613836	56.19%	6.362%
11	11.486	1560	1564	1568	rBV	1248383	1025228	93.85%	10.626%
12	13.074	1830	1834	1837	rBV	1056380	960500	87.93%	9.955%
13	13.815	1953	1960	1964	rBV9	11464	22419	2.05%	0.232%
14	13.992	1986	1990	1996	rVB3	18734	31883	2.92%	0.330%
15	14.104	2006	2009	2010	rBV	31908	25088	2.30%	0.260%
16	14.133	2010	2014	2018	rVB	1028940	889068	81.39%	9.215%
17	14.227	2026	2030	2034	rBV	76520	74794	6.85%	0.775%
18	14.909	2144	2146	2152	rVB7	9829	14094	1.29%	0.146%
19	15.651	2266	2272	2282	rVB	738382	962604	88.12%	9.977%


Sum of corrected areas: 9648112

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
Data File : BF127768.D
Acq On : 12 Apr 2022 20:01
Operator : CG\JU
Sample : N2334-07 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-19R

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

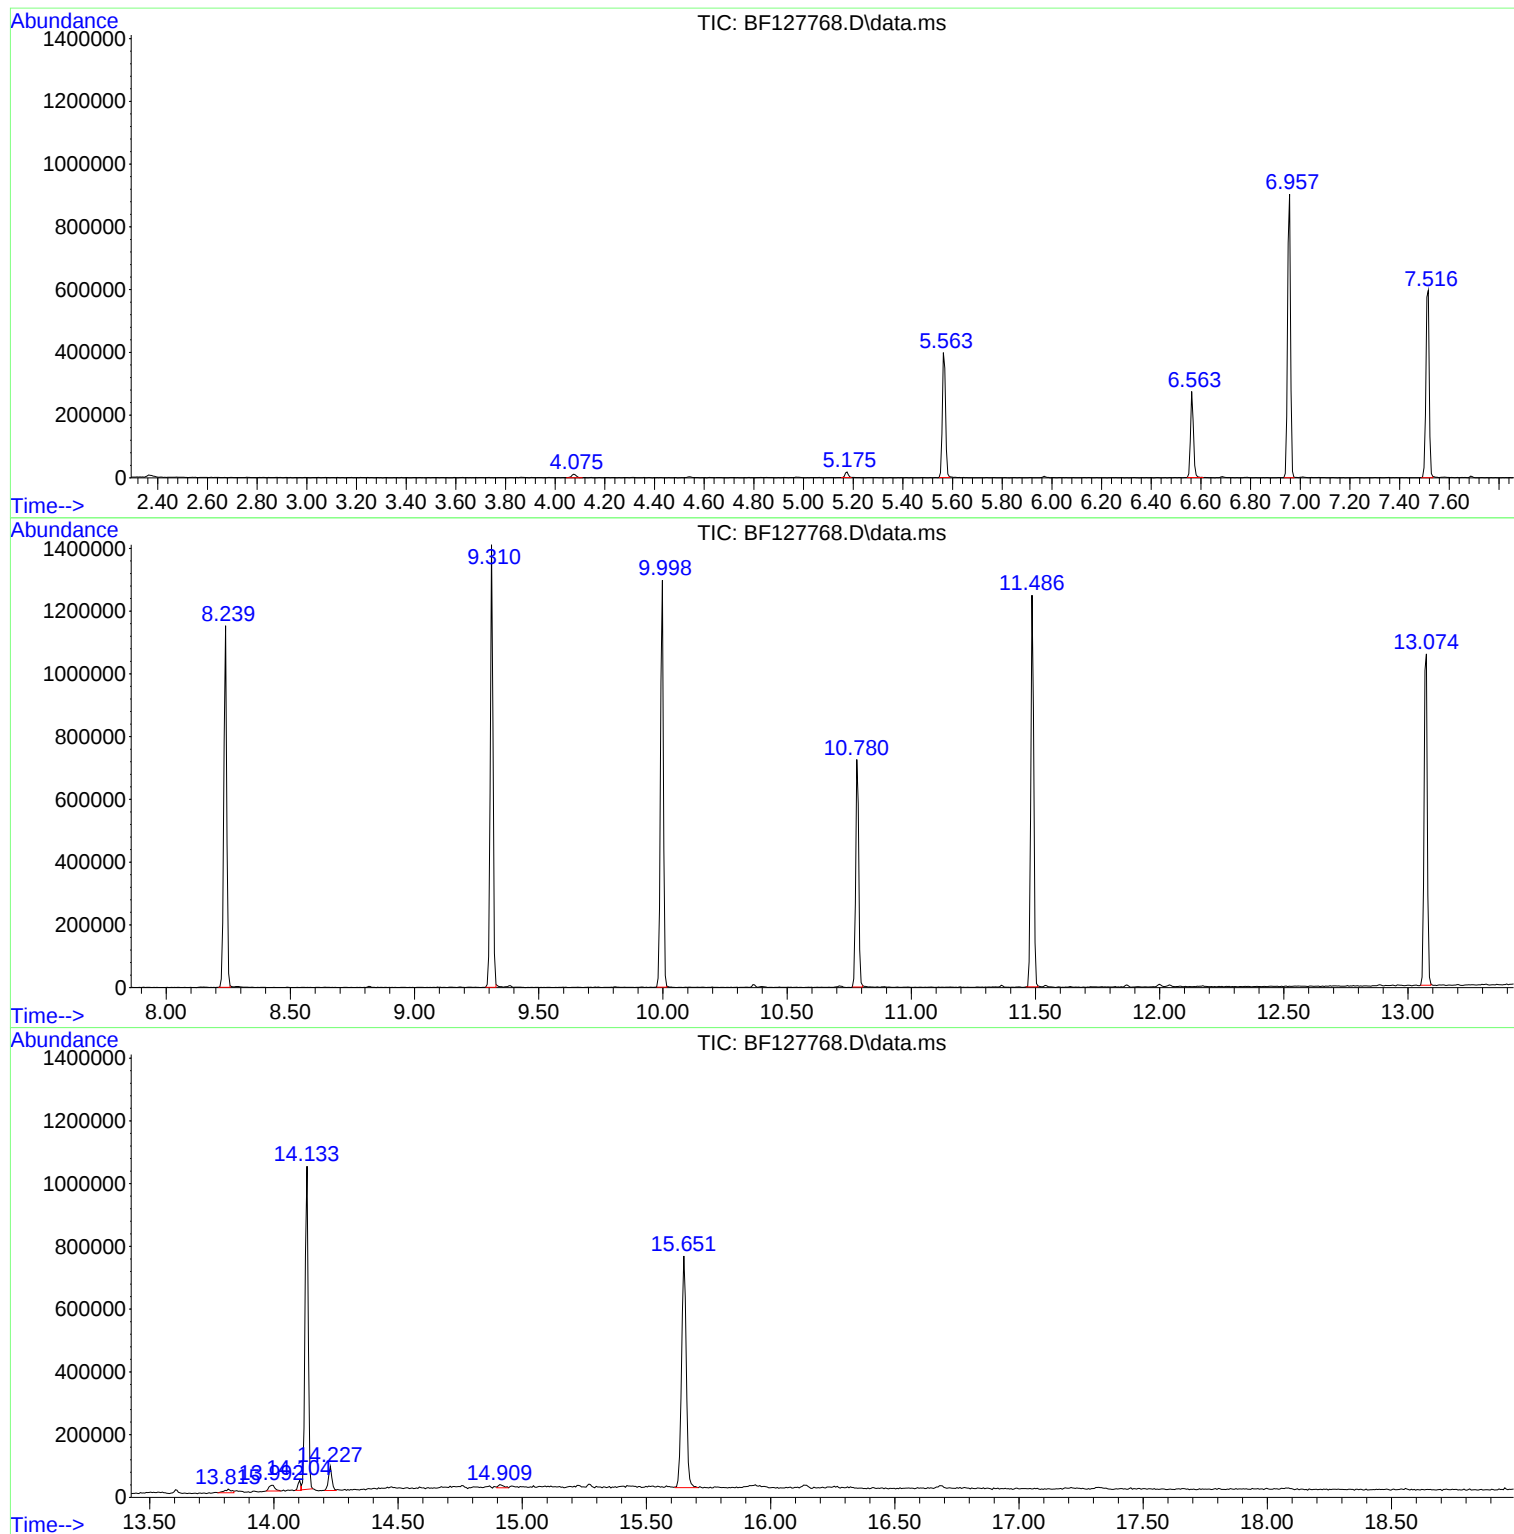

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
Data File : BF127768.D
Acq On : 12 Apr 2022 20:01
Operator : CG\JU
Sample : N2334-07 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-19R

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
Data File : BF127768.D
Acq On : 12 Apr 2022 20:01
Operator : CG\JU
Sample : N2334-07 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-19R

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------