


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
 Data File : BF127752.D
 Acq On : 12 Apr 2022 11:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 07:19:18 2022

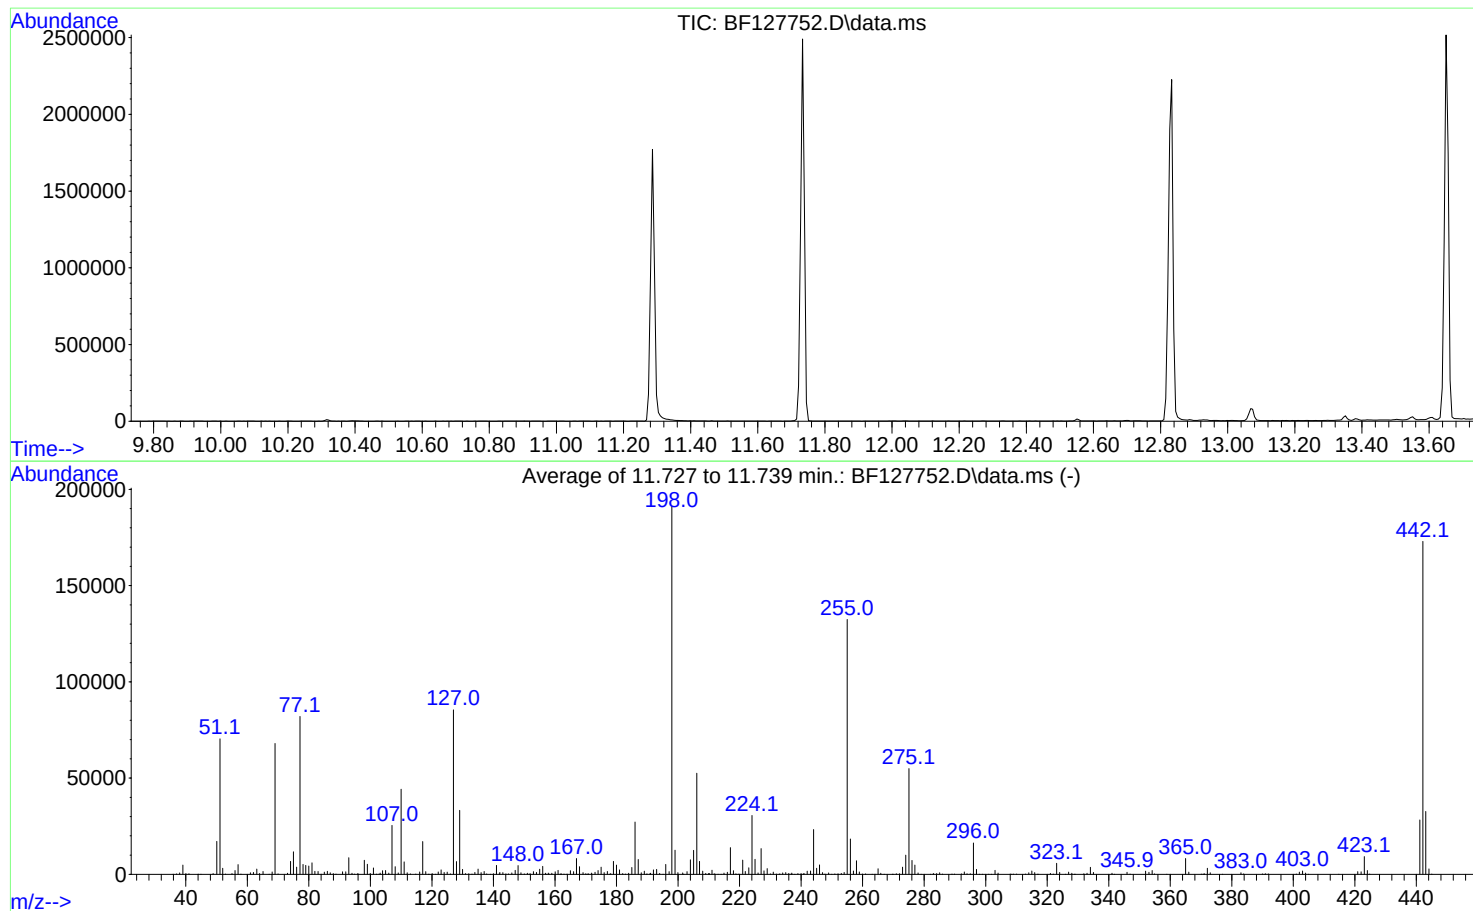


AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	70368	PASS
68	69	0.00	2	1.9	1286	PASS
69	198	0.00	100	35.6	68027	PASS
70	69	0.00	2	0.4	270	PASS
127	198	10	80	44.7	85451	PASS
197	198	0.00	2	0.7	1422	PASS
198	198	100	100	100.0	191083	PASS
199	198	5	9	6.6	12593	PASS
275	198	10	60	28.7	54920	PASS
365	198	1	100	4.3	8257	PASS
441	198	0.01	100	14.8	28276	PASS
442	442	50	100	100.0	172947	PASS
443	442	15	24	18.9	32626	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
 Data File : BF127752.D
 Acq On : 12 Apr 2022 11:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 13 08:52:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 07:19:18 2022
 Response via : Initial Calibration

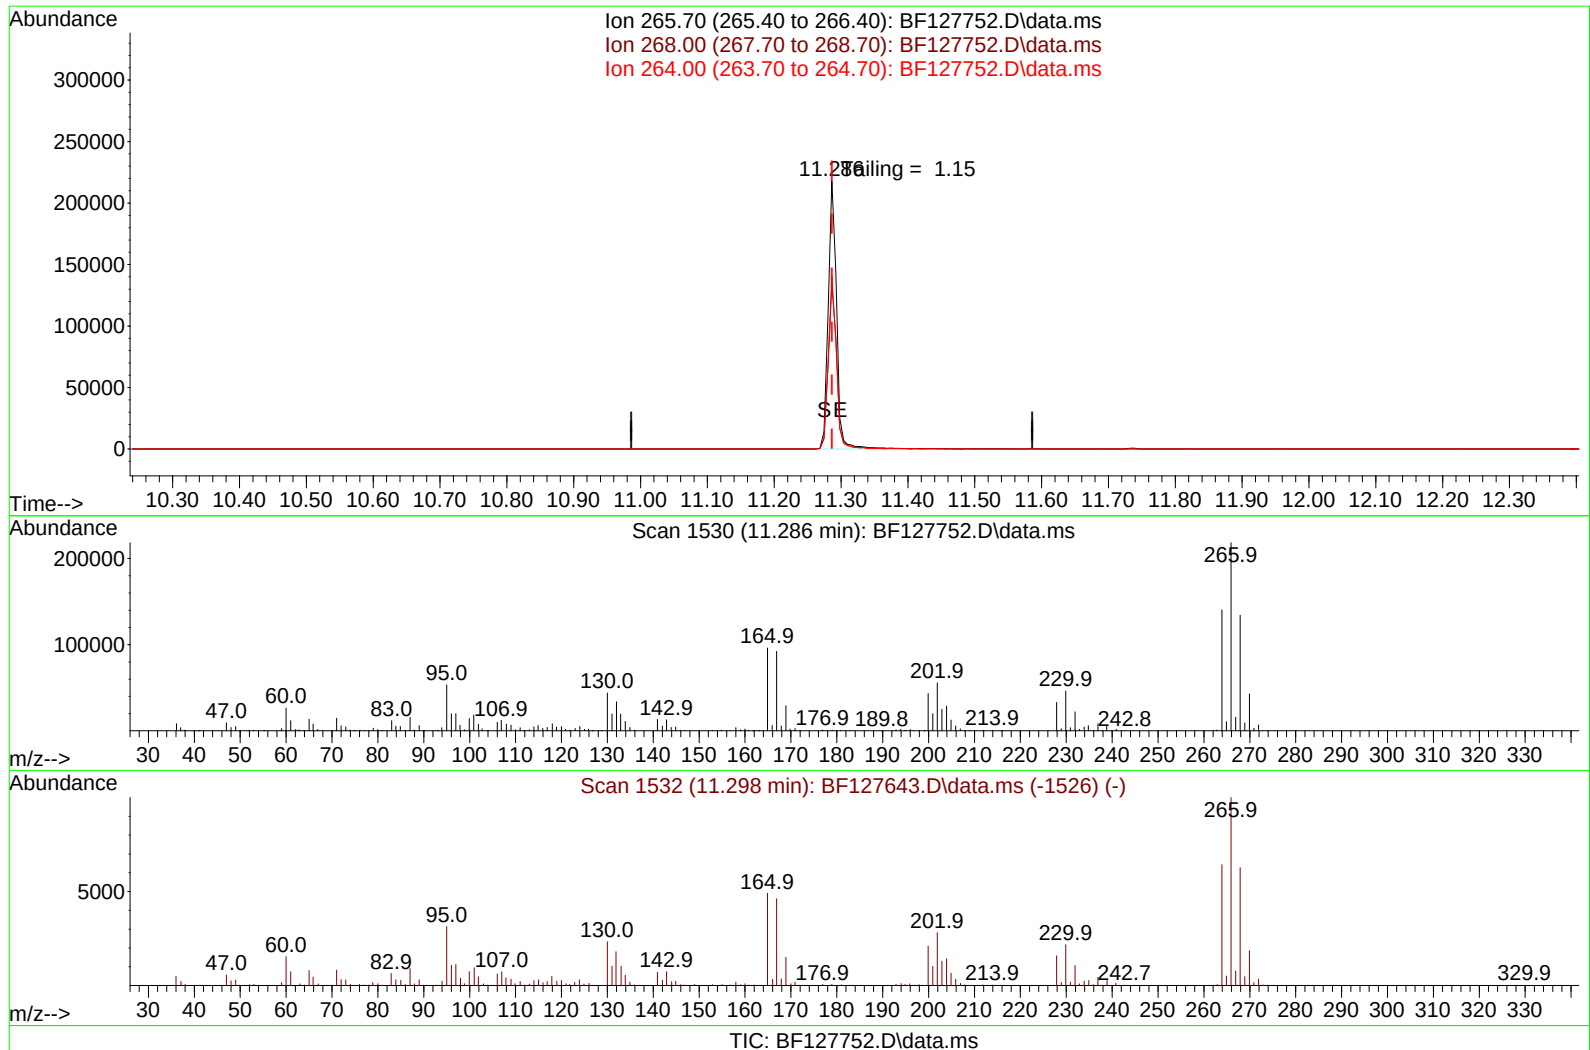

TIC: BF127752.D\data.ms

(70) Pentachlorophenol (C)

11.286min (-0.000) 25958.29 ng m




response 187791

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.47
264.00	60.60	64.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041222\
Data File : BF127752.D
Acq On : 12 Apr 2022 11:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 13 08:52:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 07:19:18 2022
Response via : Initial Calibration

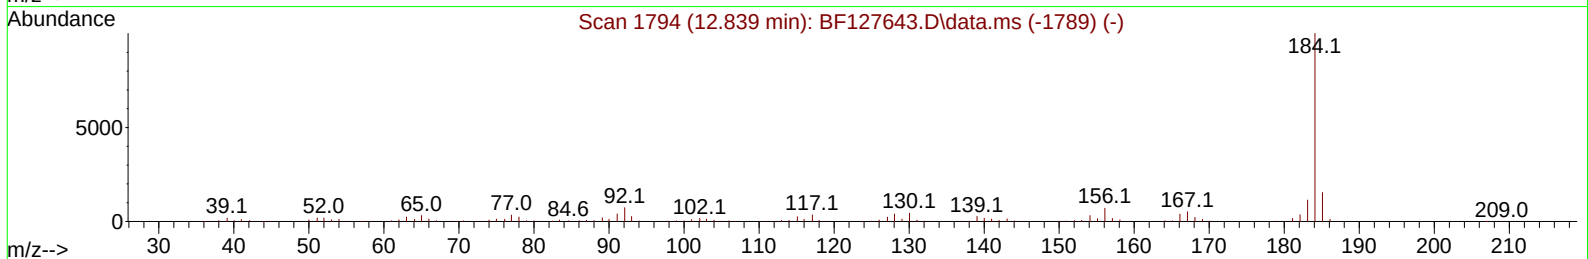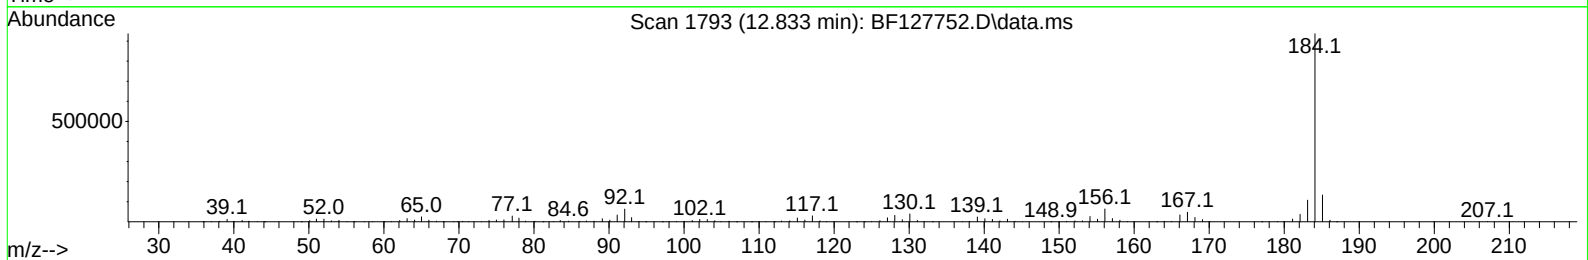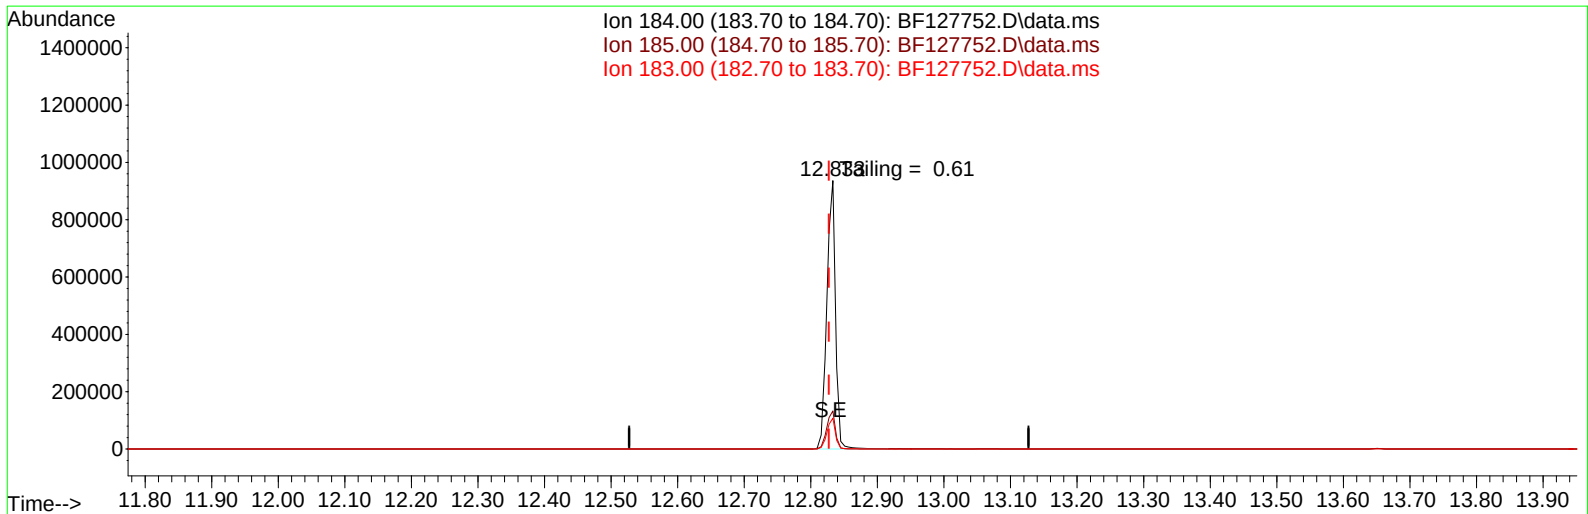

TIC: BF127752.D\data.ms

(77) Benzidine

12.833min (+ 0.006) 0.00 ng

response 851690

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.23
183.00	11.70	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/12/2022	BNA_F	<u>BF127752.D</u>
Compound Name	Response	Retention Time
DDT	413934	13.651
DDD	7131	13.351
DDE	361	13.015
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7492	421426	1.78

Instrument :
BNA_F
ClientSampleId :
DFTPP