
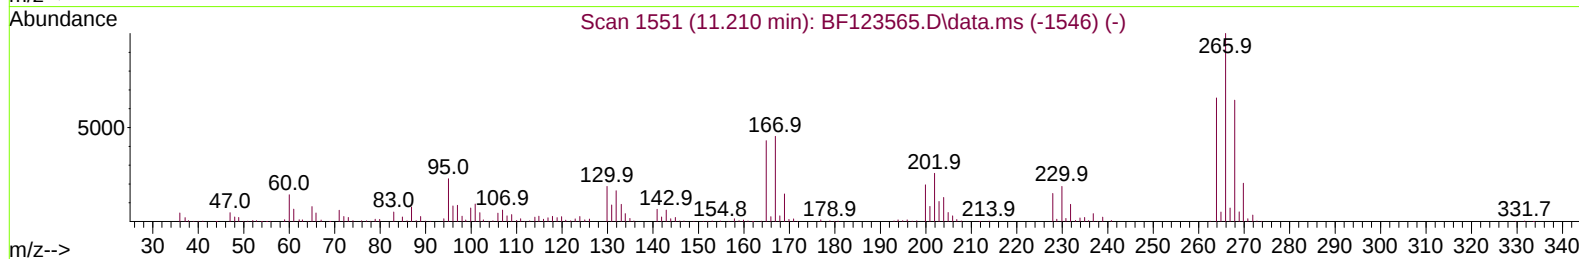
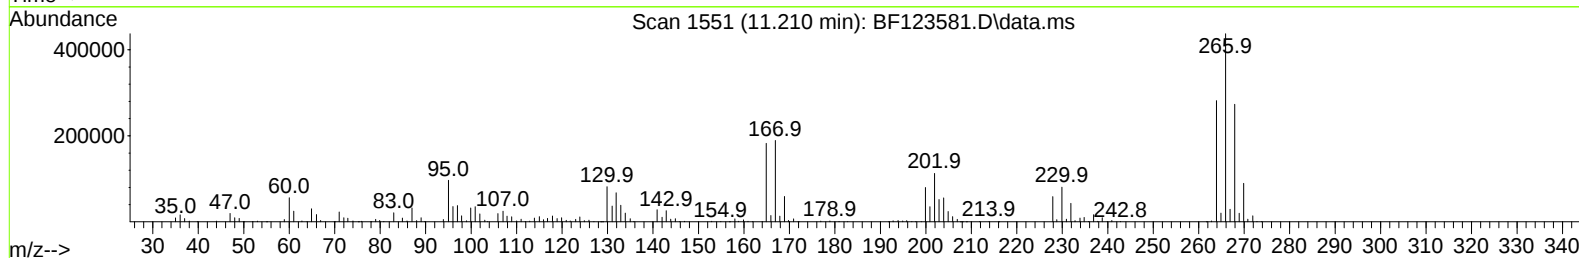


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
 Data File : BF123581.D
 Acq On : 16 Apr 2021 8:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:54:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 10:31:33 2021
 Response via : Initial Calibration

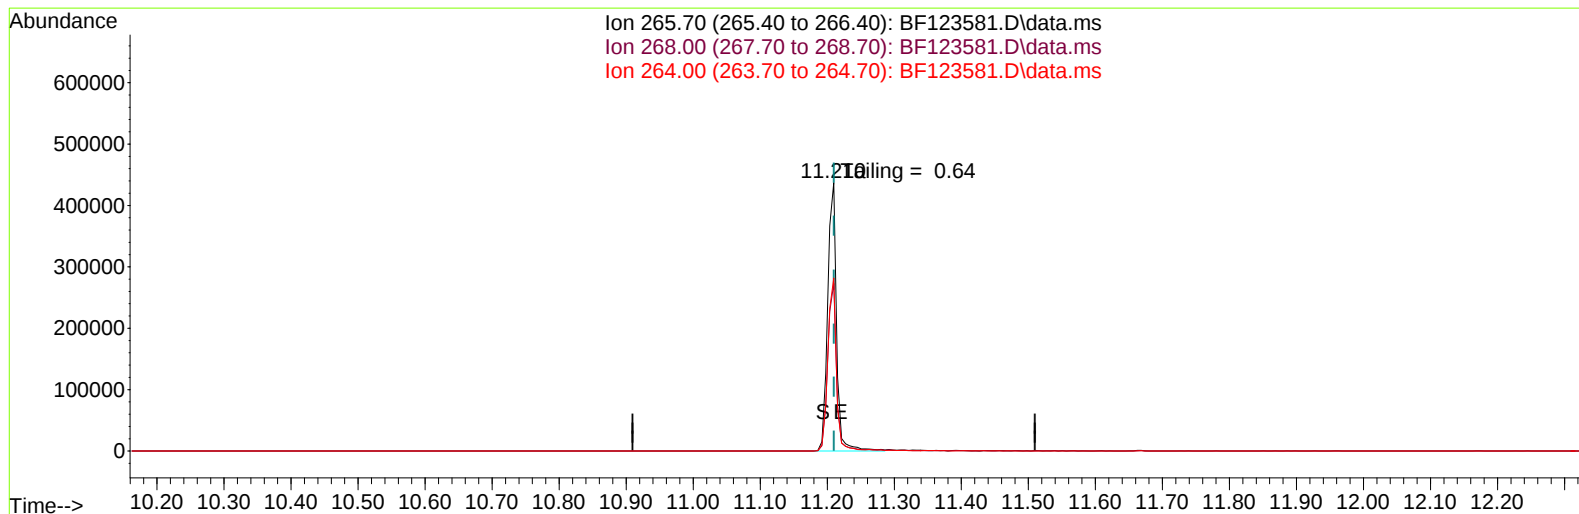




TIC: BF123581.D\data.ms

(70) Pentachlorophenol (C)**11.210min (-0.000) 39206.74 ng****response 405474**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.46
264.00	65.70	64.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
 Data File : BF123581.D
 Acq On : 16 Apr 2021 8:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:54:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 10:31:33 2021
 Response via : Initial Calibration

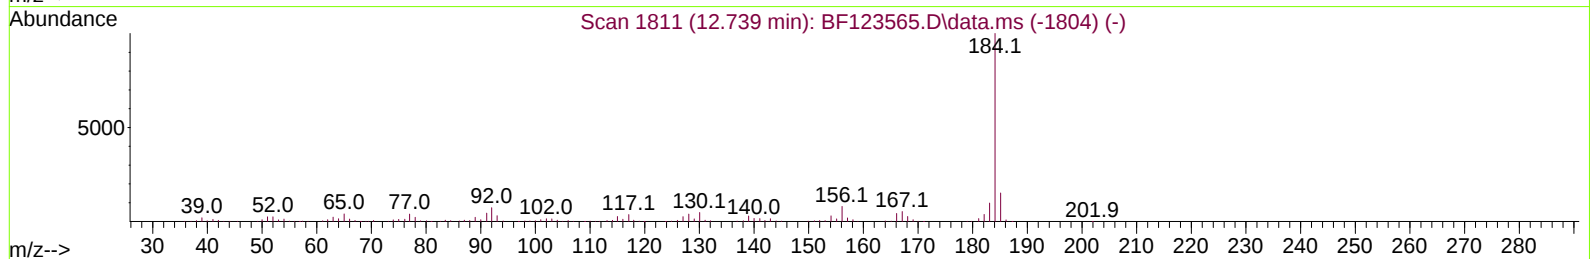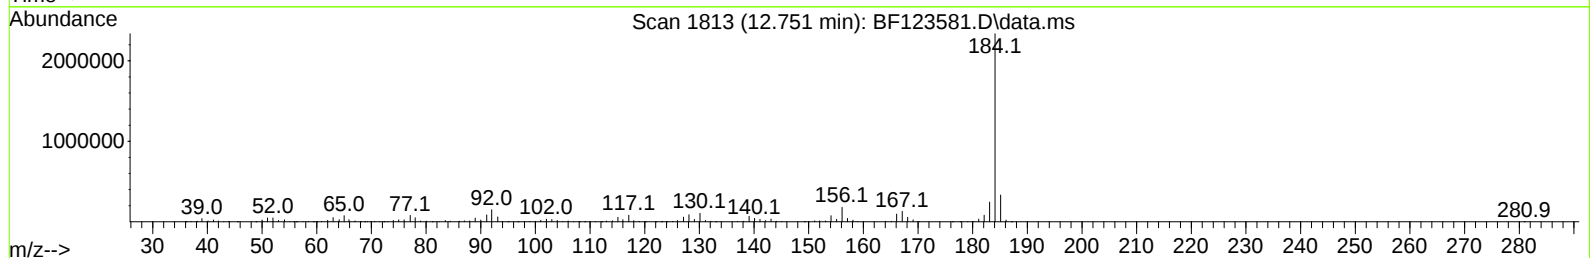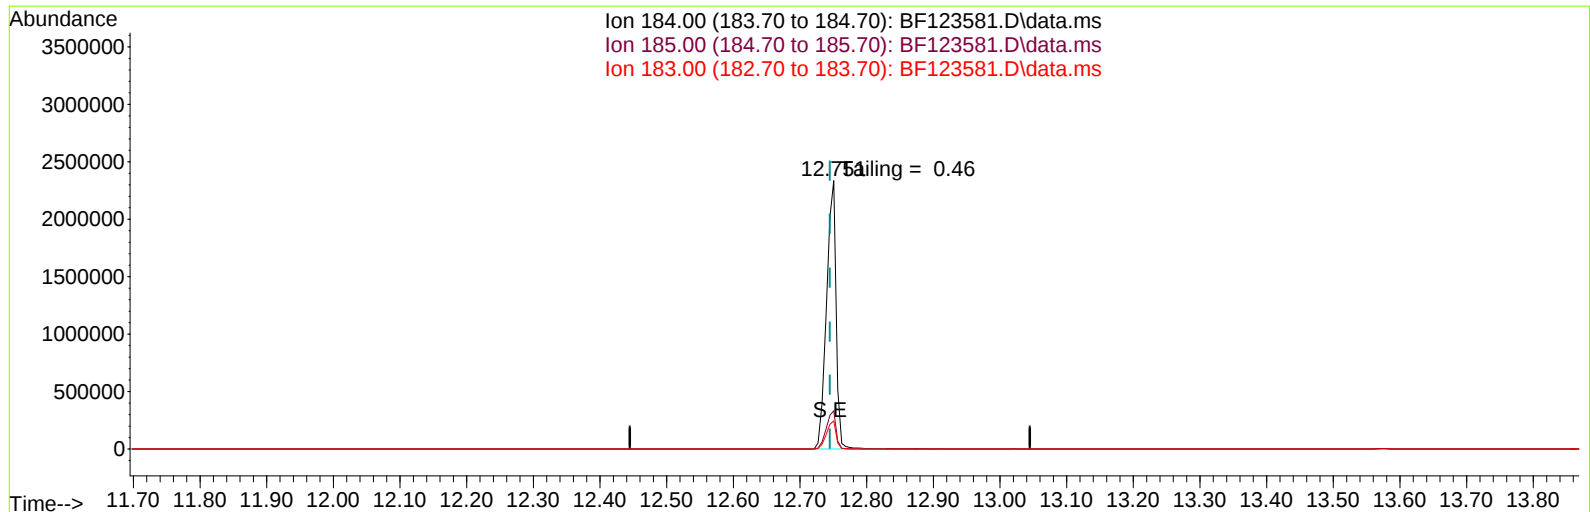

TIC: BF123581.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 2332184

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.24
183.00	9.80	10.51
0.00	0.00	0.00