
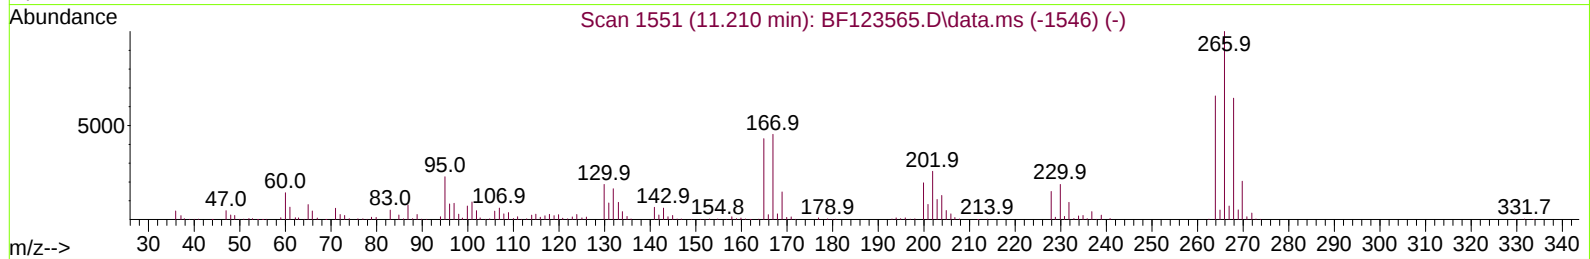
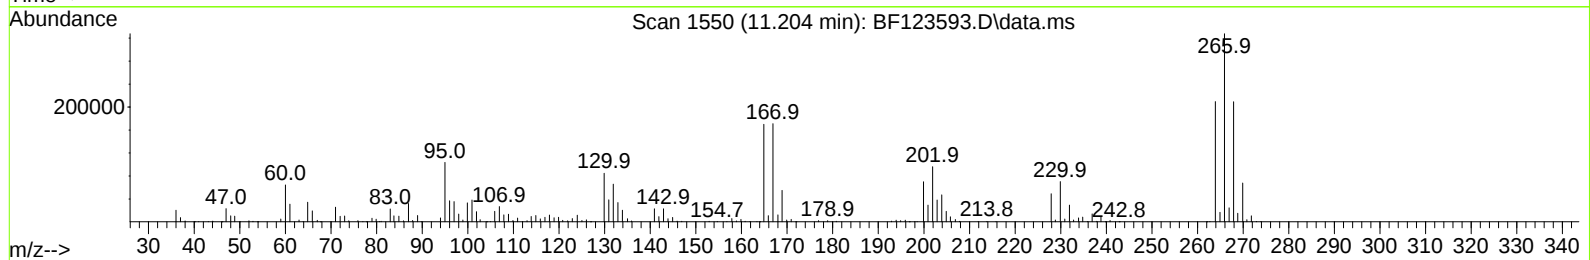


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
Data File : BF123593.D
Acq On : 16 Apr 2021 15:32
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:58:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 10:31:33 2021
Response via : Initial Calibration

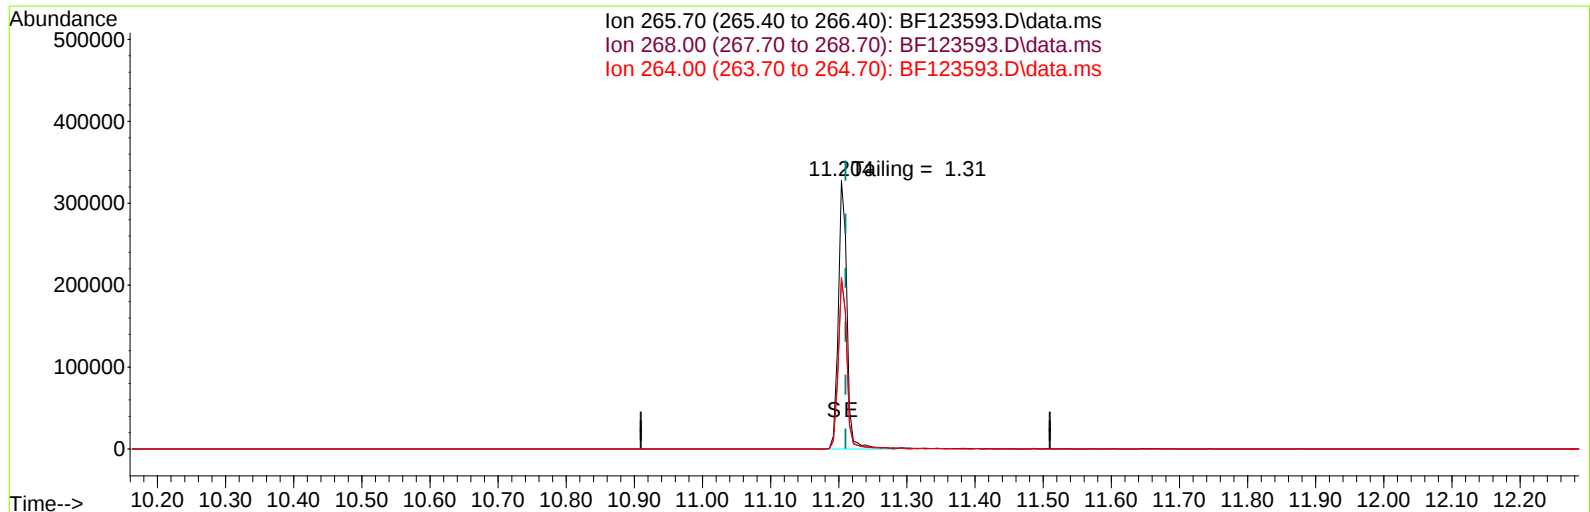

TIC: BF123593.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.006) 38186.39 ng

response 288904

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.86
264.00	65.70	63.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
Data File : BF123593.D
Acq On : 16 Apr 2021 15:32
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:58:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 10:31:33 2021
Response via : Initial Calibration

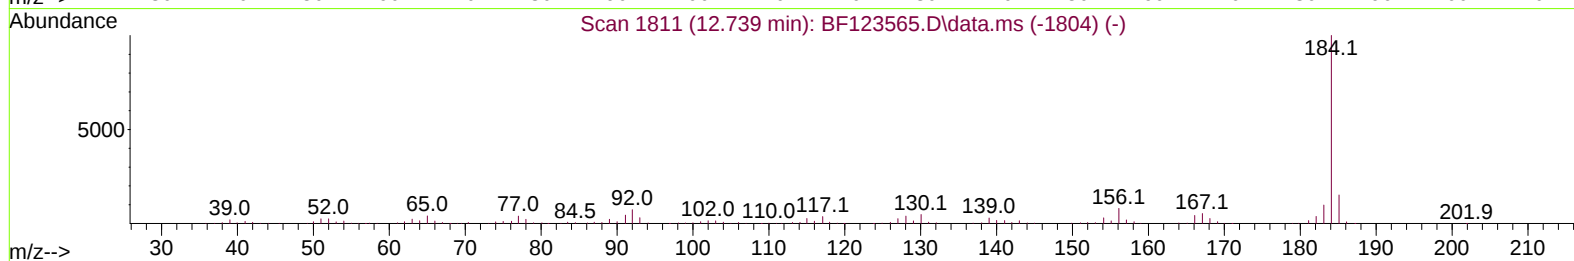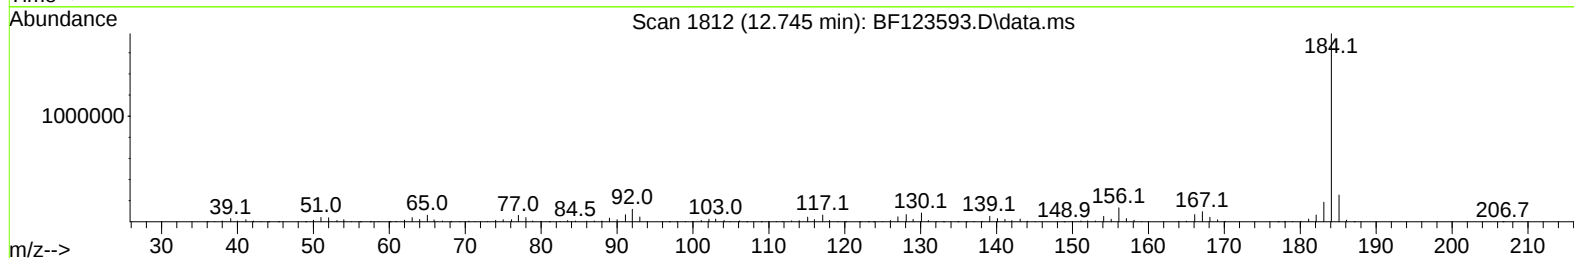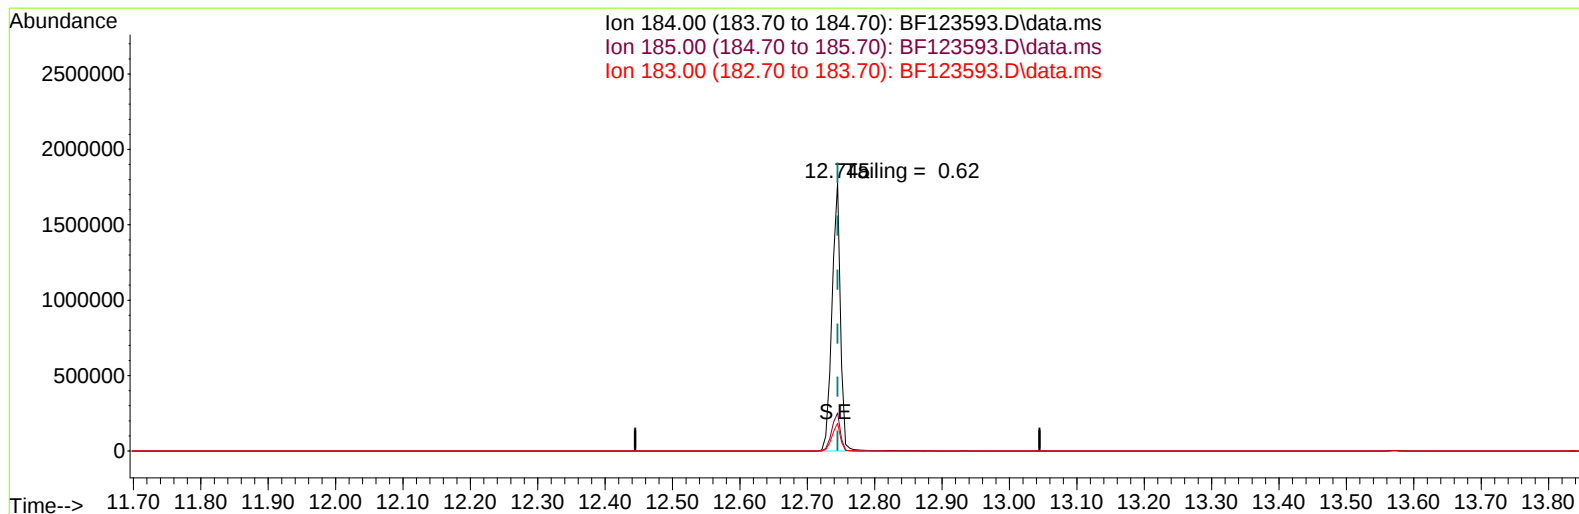

TIC: BF123593.D\data.ms

(77) Benzidine

12.745min (-0.000) 0.00 ng

response 1540069

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.20
183.00	9.80	10.41
0.00	0.00	0.00