

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
 Data File : BF123604.D
 Acq On : 16 Apr 2021 21:50
 Operator : JU/CG
 Sample : M2050-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

mohammad
 4/19/2021 11:45:25 AM

Quant Time: Apr 17 01:26:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 10:31:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.869	152	291378	20.00	ng	0.00
21) Naphthalene-d8	8.151	136	1096164	20.00	ng	0.00
39) Acenaphthene-d10	9.916	164	529803	20.00	ng	0.00
64) Phenanthrene-d10	11.404	188	909151	20.00	ng	0.00
76) Chrysene-d12	14.051	240	496024	20.00	ng	0.00
86) Perylene-d12	15.545	264	460185	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	1955910	108.49	ng	0.02
7) Phenol-d6	6.510	99	2539105	101.64	ng	0.01
23) Nitrobenzene-d5	7.433	82	1867008	78.30	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	689424	114.91	ng	0.00
45) 2-Fluorobiphenyl	9.233	172	2758020	77.60	ng	0.00
79) Terphenyl-d14	12.998	244	2076282	81.35	ng	0.00
Target Compounds						Qvalue
10) Phenol	6.522	94	61274	2.31	ng	92
71) Phenanthrene	11.427	178	372846	7.86	ng	99
75) Fluoranthene	12.621	202	606640	11.63	ng	97
78) Pyrene	12.851	202	550787	15.21	ng	99
81) Benzo(a)anthracene	14.039	228	244001	8.03	ng	97
83) Chrysene	14.074	228	234159	7.67	ng	98
87) Indeno(1,2,3-cd)pyrene	17.027	276	150125	6.11	ng	98
88) Benzo(b)fluoranthene	15.104	252	305966m	9.42	ng	
90) Benzo(a)pyrene	15.474	252	215835	8.35	ng	# 96
92) Benzo(g,h,i)perylene	17.480	276	146047	8.57	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
Data File : BF123604.D
Acq On : 16 Apr 2021 21:50
Operator : JU/CG
Sample : M2050-17
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
TP-6

Manual Integrations
APPROVED


mohammad
4/19/2021 11:45:25 AM

Quant Time: Apr 17 01:26:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 10:31:33 2021
Response via : Initial Calibration



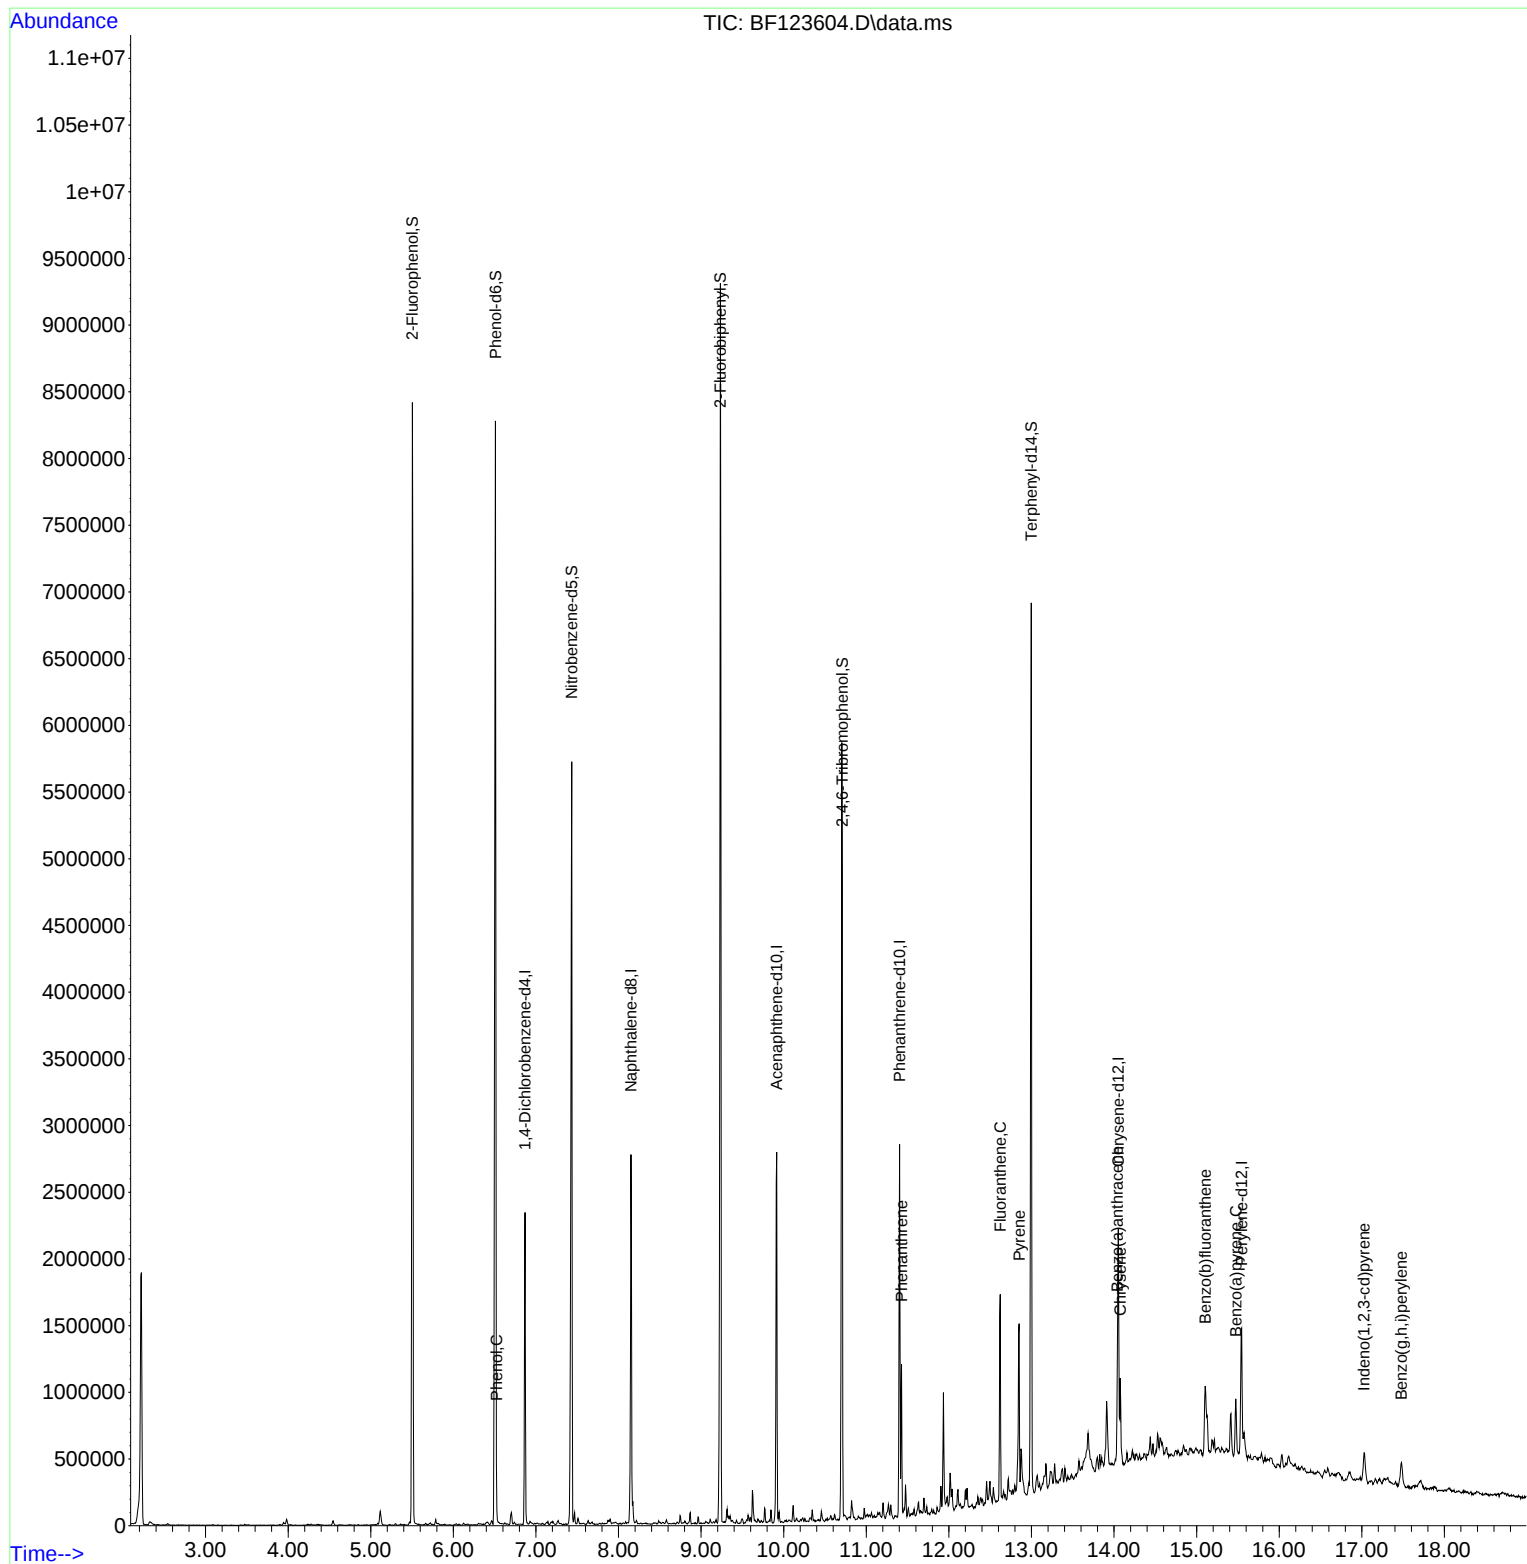


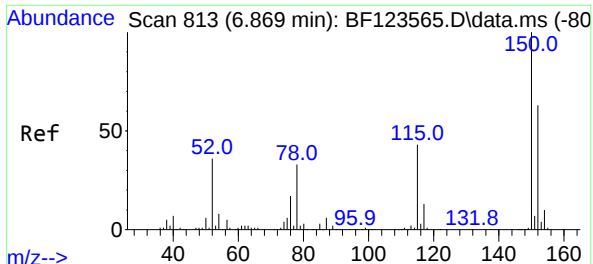


#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.869 min Scan# 813
Delta R.T. -0.000 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

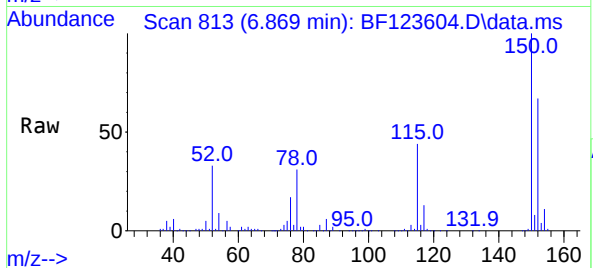



Tgt Ion:152 Resp: 291378
Ion Ratio Lower Upper
152 100
150 149.6 127.0 190.6
115 66.2 54.3 81.5

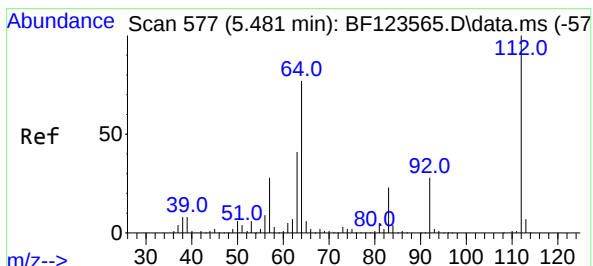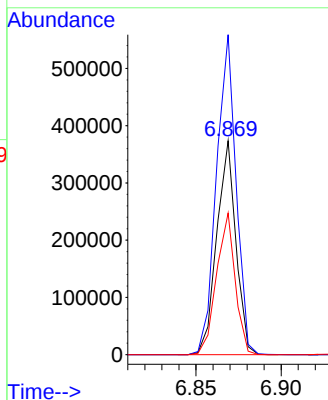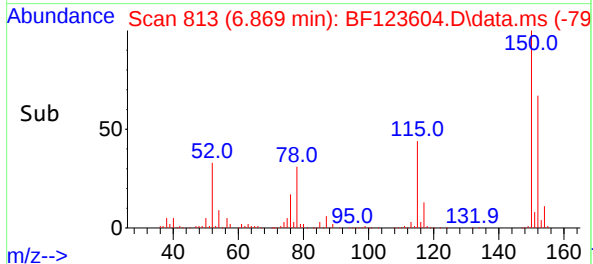

#5
2-Fluorophenol
Concen: 108.49 ng
RT: 5.504 min Scan# 581
Delta R.T. 0.023 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

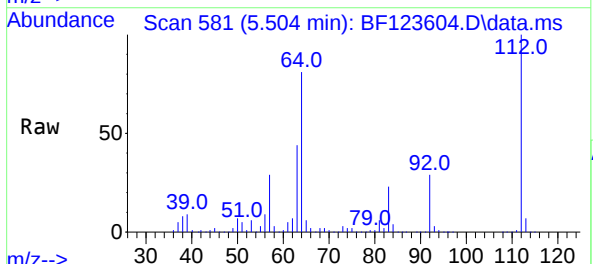


Tgt Ion:112 Resp: 1955910
Ion Ratio Lower Upper
112 100
64 81.3 61.4 92.0
63 44.1 33.0 49.4

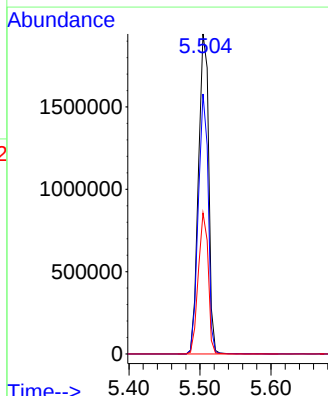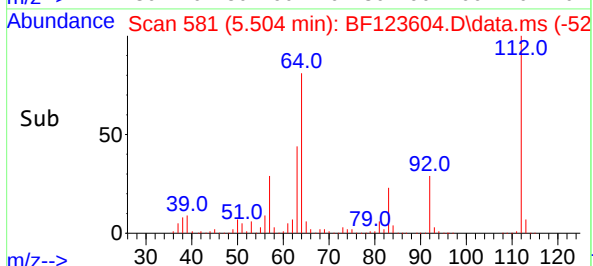


Instrument :
BNA_F
ClientSampled :
TP-6

Manual Integrations
APPROVED

mohammad
4/19/2021 11:45:25 AM




#7
Phenol-d6
Concen: 101.64 ng
RT: 6.510 min Scan# 752
Delta R.T. 0.012 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50



Tgt Ion: 99 Resp: 2539105


Ion	Ratio	Lower	Upper
99	100		
42	25.1	19.8	29.8
71	42.8	31.1	46.7

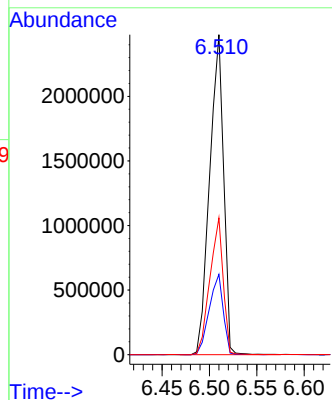


Instrument :
BNA_F
ClientSampled :
TP-6

Manual Integrations
APPROVED

mohammad
4/19/2021 11:45:25 AM






#10
Phenol
Concen: 2.31 ng
RT: 6.522 min Scan# 754
Delta R.T. 0.012 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

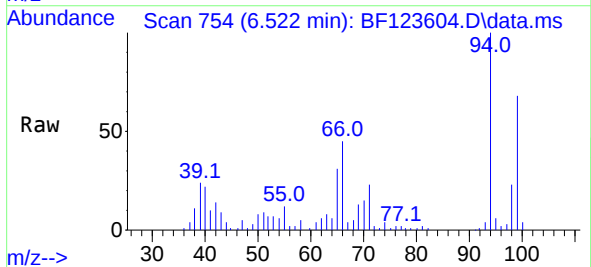

Tgt Ion: 94 Resp: 61274


Ion	Ratio	Lower	Upper
94	100		
65	31.2	18.1	58.1
66	45.2	29.0	69.0

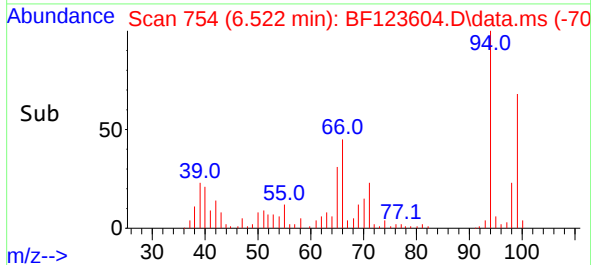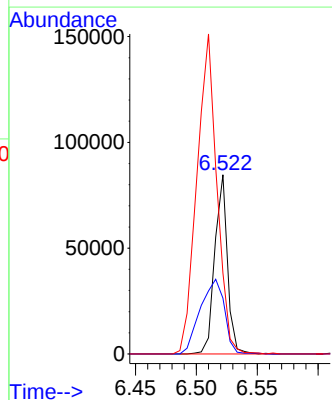



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.151 min Scan# 1031
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50



Instrument :
BNA_F
ClientSampled :
TP-6




Tgt Ion:136 Resp: 1096164
Ion Ratio Lower Upper
136 100
137 11.7 8.7 13.1
54 13.0 9.8 14.6
68 5.9 4.1 6.1

Manual Integrations
APPROVED



mohammad
4/19/2021 11:45:25 AM

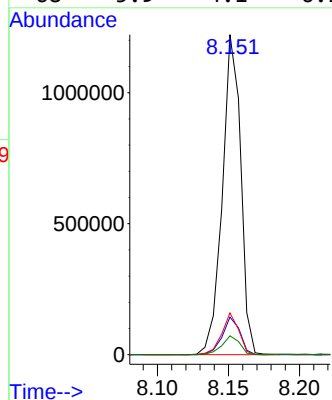


#23
Nitrobenzene-d5
Concen: 78.30 ng
RT: 7.433 min Scan# 909
Delta R.T. -0.000 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50




Tgt Ion: 82 Resp: 1867008
Ion Ratio Lower Upper
82 100
128 38.8 29.4 44.2
54 64.7 54.1 81.1


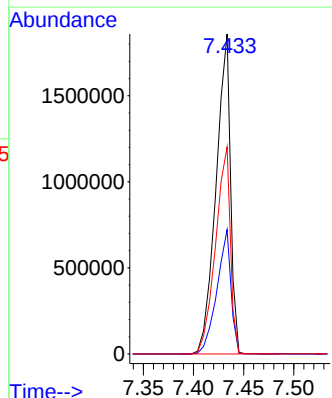






#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.916 min Scan# 1331
Delta R.T. -0.000 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50





Tgt Ion:164 Resp: 529803
Ion Ratio Lower Upper
164 100
162 103.0 80.7 121.1
160 49.0 37.3 55.9

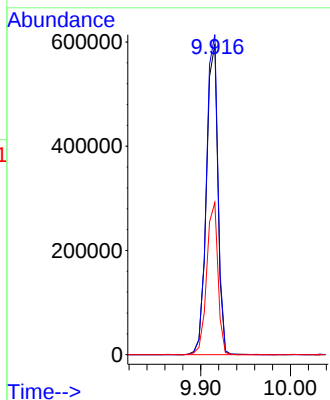

#42
2,4,6-Tribromophenol
Concen: 114.91 ng
RT: 10.710 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

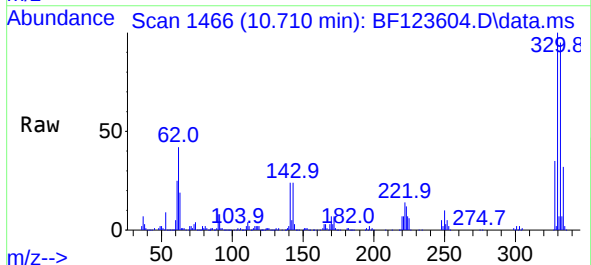


Tgt Ion:330 Resp: 689424
Ion Ratio Lower Upper
330 100
332 95.7 77.1 115.7
141 33.7 27.9 41.9

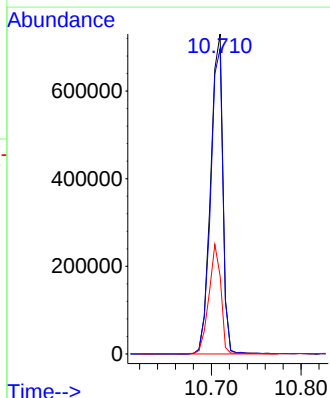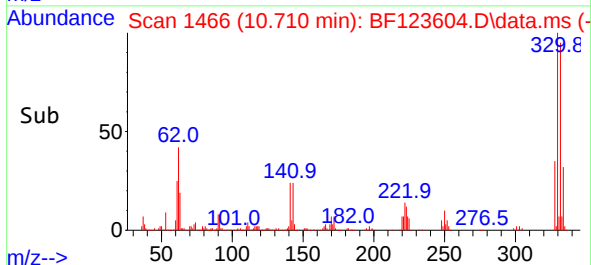

Instrument :
BNA_F
ClientSampled :
TP-6

Manual Integrations
APPROVED

mohammad
4/19/2021 11:45:25 AM







#45
2-Fluorobiphenyl
Concen: 77.60 ng
RT: 9.233 min Scan# 1215
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

Tgt Ion:172 Resp: 2758020
Ion Ratio Lower Upper
172 100
171 36.4 28.1 42.1
170 24.3 19.2 28.8

Instrument :
BNA_F
ClientSampled :
TP-6




Manual Integrations
APPROVED


mohammad
4/19/2021 11:45:25 AM

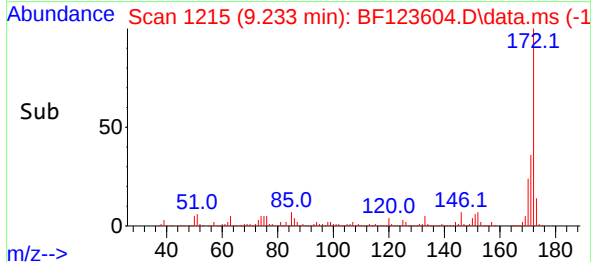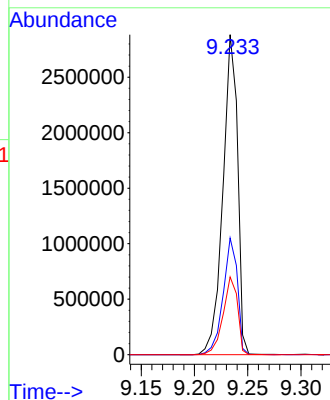

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.404 min Scan# 1584
Delta R.T. -0.000 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50


Tgt Ion:188 Resp: 909151
Ion Ratio Lower Upper
188 100
94 8.3 6.9 10.3
80 9.5 8.2 12.2

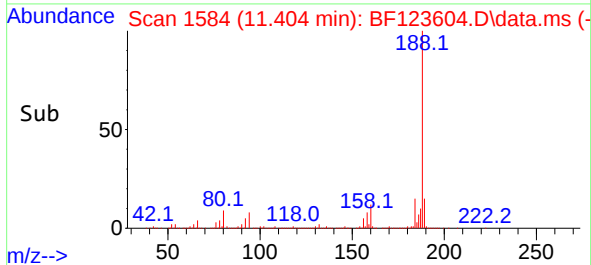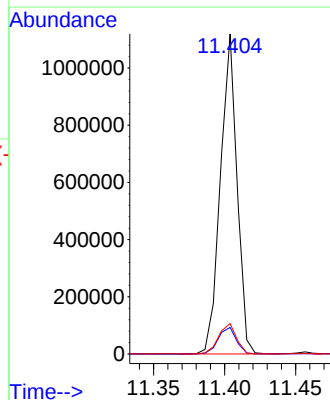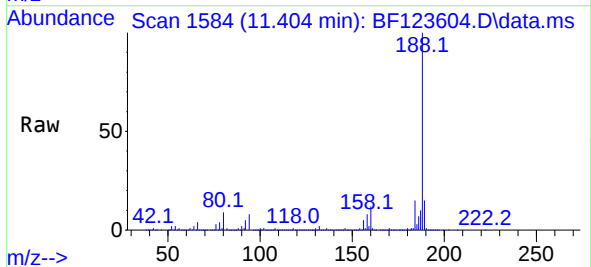



#71
Phenanthrene
Concen: 7.86 ng
RT: 11.427 min Scan# 1588
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50




Instrument :
BNA_F
ClientSampled :
TP-6




Tgt Ion:178 Resp: 372846
Ion Ratio Lower Upper
178 100
176 18.5 15.6 23.4
179 15.7 12.5 18.7

Manual Integrations
APPROVED



mohammad
4/19/2021 11:45:25 AM

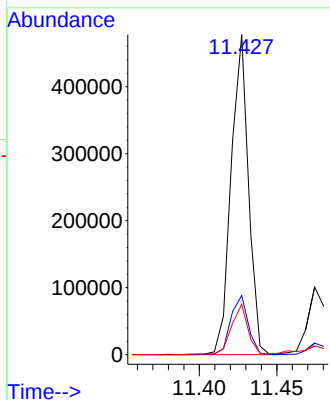


#75
Fluoranthene
Concen: 11.63 ng
RT: 12.621 min Scan# 1791
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50




Tgt Ion:202 Resp: 606640
Ion Ratio Lower Upper
202 100
101 8.8 0.0 30.9
203 17.0 0.0 37.5


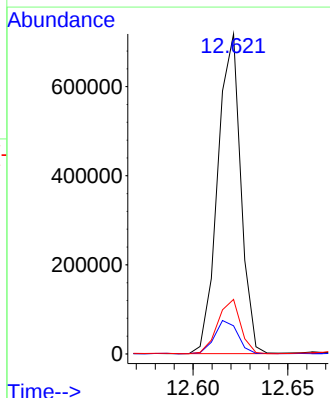






#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.051 min Scan# 2034
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

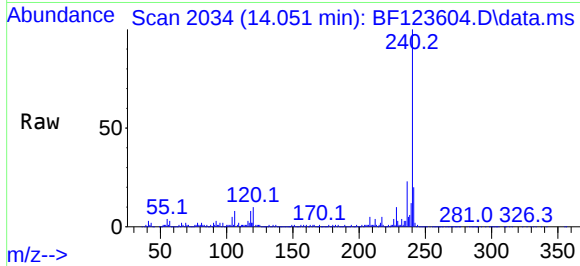



Tgt Ion:240 Resp: 496024
Ion Ratio Lower Upper
240 100
120 9.8 7.2 10.8
236 23.5 19.0 28.4

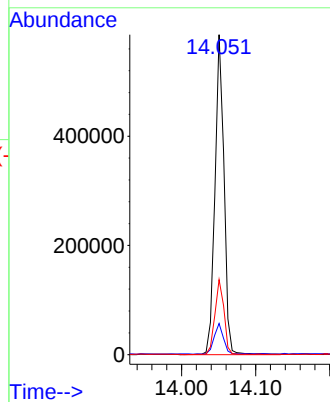

#78
Pyrene
Concen: 15.21 ng
RT: 12.851 min Scan# 1830
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

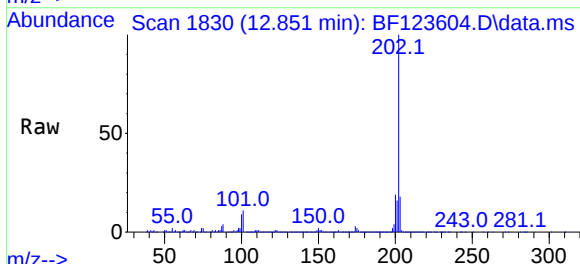


Tgt Ion:202 Resp: 550787
Ion Ratio Lower Upper
202 100
200 19.1 16.1 24.1
203 18.2 14.8 22.2

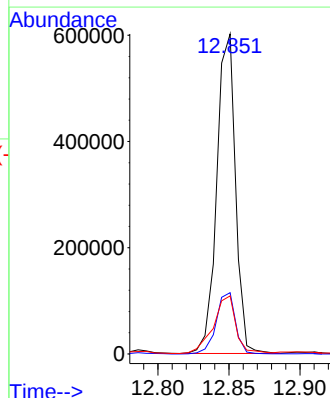

Instrument :
BNA_F
ClientSampled :
TP-6


Manual Integrations
APPROVED

mohammad
4/19/2021 11:45:25 AM



#79
Terphenyl-d14
Concen: 81.35 ng
RT: 12.998 min Scan# 1855
Delta R.T. -0.000 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50




Instrument :
BNA_F
ClientSampled :
TP-6

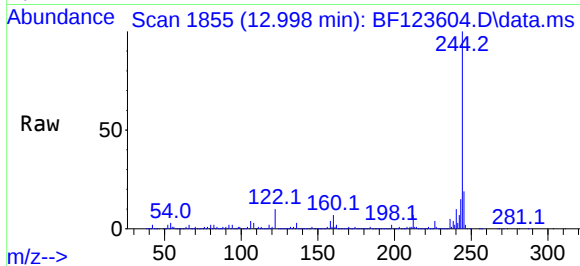


Tgt Ion:244 Resp: 2076282
Ion Ratio Lower Upper
244 100
212 7.2 5.7 8.5
122 9.8 9.7 14.5

Manual Integrations
APPROVED



mohammad
4/19/2021 11:45:25 AM

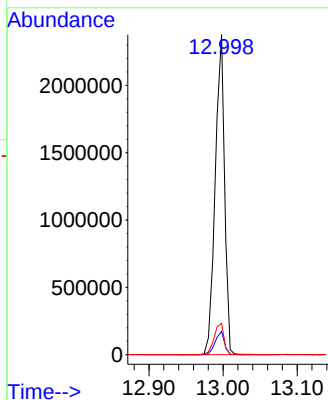


#81
Benzo(a)anthracene
Concen: 8.03 ng
RT: 14.039 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

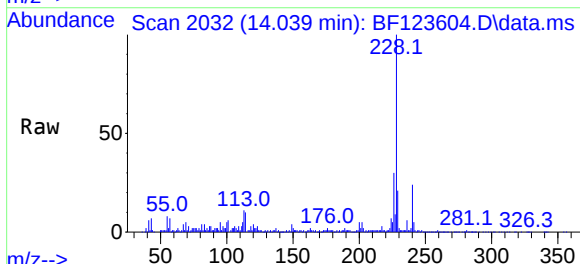

Tgt Ion:228 Resp: 244001
Ion Ratio Lower Upper
228 100
226 29.7 22.4 33.6
229 21.1 16.0 24.0

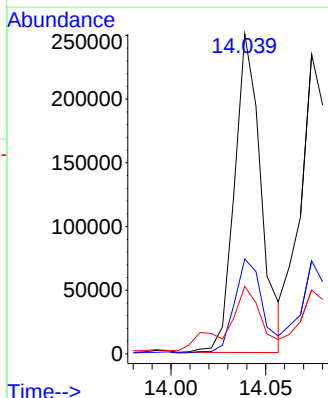







#83
Chrysene
Concen: 7.67 ng
RT: 14.074 min Scan# 2038
Delta R.T. -0.012 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

Tgt Ion:	228	Resp:	234159
Ion Ratio	Lower	Upper	
228	100		
226	31.1	24.3	36.5
229	21.4	16.2	24.2

Instrument :
BNA_F
ClientSampled :
TP-6




Manual Integrations
APPROVED


mohammad
4/19/2021 11:45:25 AM

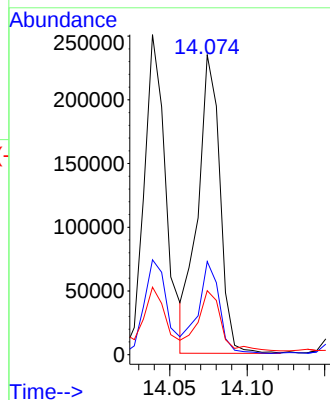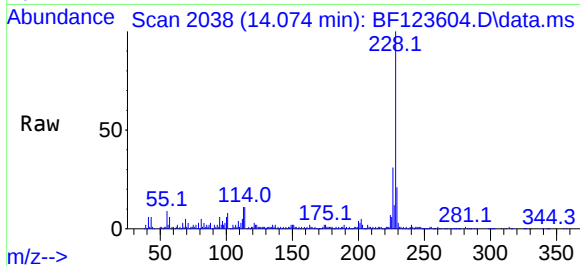

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.545 min Scan# 2288
Delta R.T. 0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

Tgt Ion:	264	Resp:	460185
Ion Ratio	Lower	Upper	
264	100		
260	24.9	18.7	28.1
265	22.4	17.8	26.8

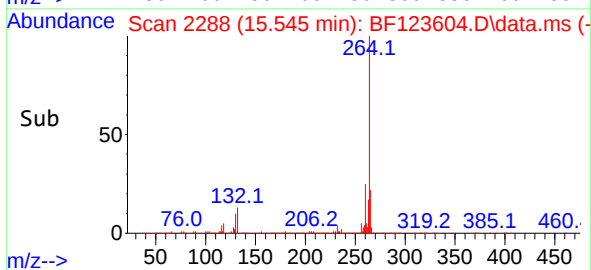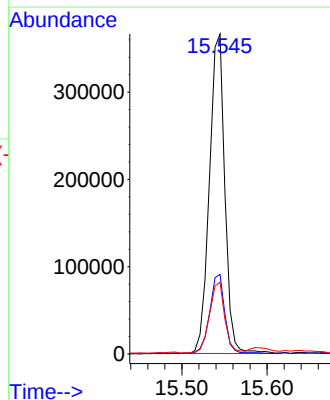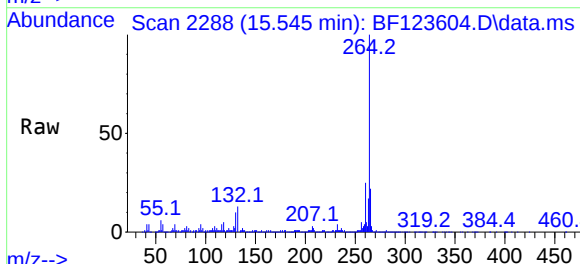







#87
Indeno(1,2,3-cd)pyrene
Concen: 6.11 ng
RT: 17.027 min Scan# 2540
Delta R.T. -0.012 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

Tgt Ion: 276 Resp: 150125
Ion Ratio Lower Upper
276 100
138 20.3 16.2 24.2
277 23.6 20.1 30.1

Instrument :
BNA_F
ClientSampled :
TP-6




Manual Integrations
APPROVED


mohammad
4/19/2021 11:45:25 AM

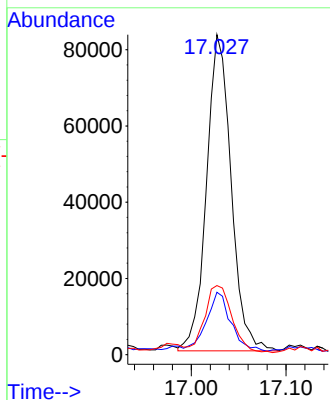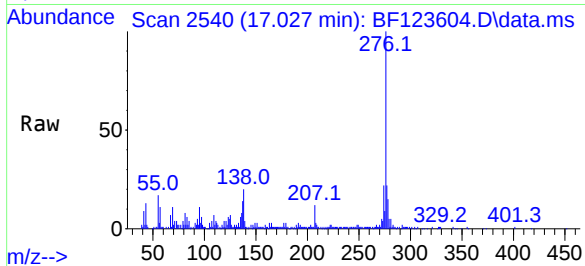

#88
Benzo(b)fluoranthene
Concen: 9.42 ng m
RT: 15.104 min Scan# 2213
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

Tgt Ion: 252 Resp: 305966
Ion Ratio Lower Upper
252 100
253 23.6 18.1 27.1
125 12.4 6.2 9.4#

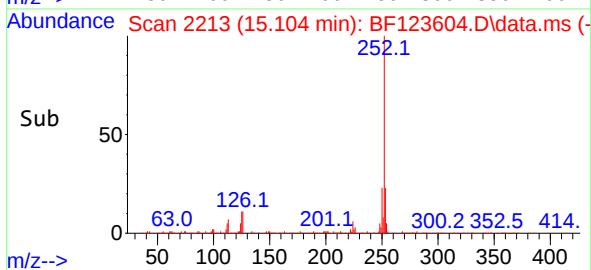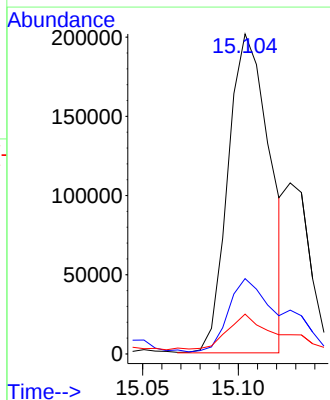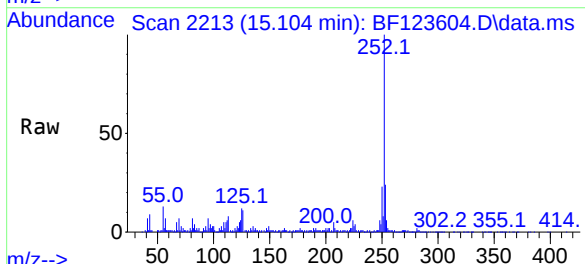







#90
Benzo(a)pyrene
Concen: 8.35 ng
RT: 15.474 min Scan# 2276
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

Tgt Ion:252 Resp: 215835
Ion Ratio Lower Upper
252 100
253 23.9 18.4 27.6
125 13.5 8.0 12.0#

Instrument :
BNA_F
ClientSampled :
TP-6

Manual Integrations
APPROVED

mohammad
4/19/2021 11:45:25 AM

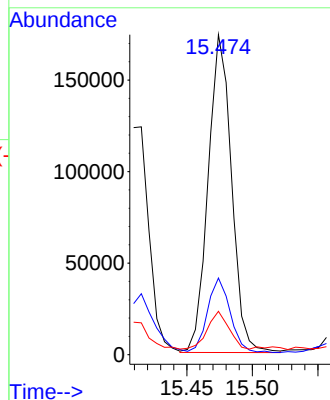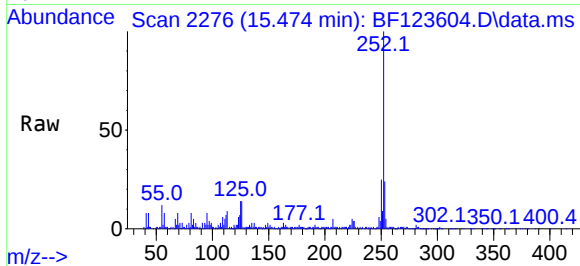

#92
Benzo(g,h,i)perylene
Concen: 8.57 ng
RT: 17.480 min Scan# 2617
Delta R.T. -0.006 min
Lab File: BF123604.D
Acq: 16 Apr 2021 21:50

Tgt Ion:276 Resp: 146047
Ion Ratio Lower Upper
276 100
277 25.3 18.2 27.2
138 18.8 13.8 20.6

