


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
 Data File : BF123581.D
 Acq On : 16 Apr 2021 8:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 10:31:33 2021

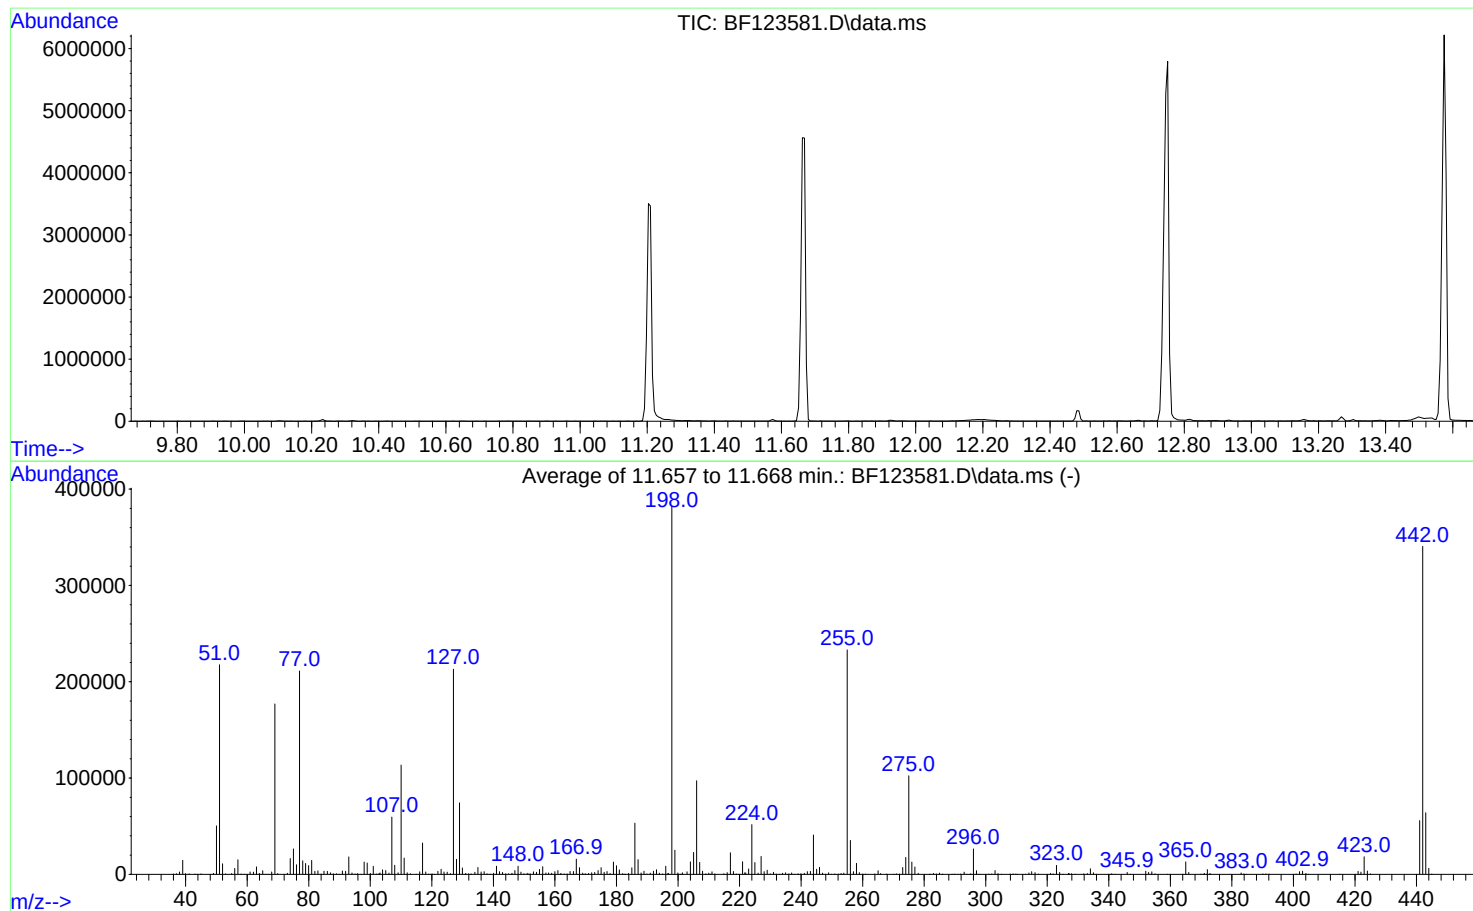




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.0	217621	PASS
68	69	0.00	2	1.4	2504	PASS
69	198	0.00	100	46.3	177032	PASS
70	69	0.00	2	0.5	829	PASS
127	198	10	80	55.8	213024	PASS
197	198	0.00	2	0.2	954	PASS
198	198	100	100	100.0	381973	PASS
199	198	5	9	6.6	25173	PASS
275	198	10	60	26.8	102347	PASS
365	198	1	100	3.4	12951	PASS
441	198	0.01	100	14.6	55814	PASS
442	442	50	100	100.0	340544	PASS
443	442	15	24	18.8	64047	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
Data File : BF123581.D
Acq On : 16 Apr 2021 8:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 17 05:54:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 10:31:33 2021
Response via : Initial Calibration

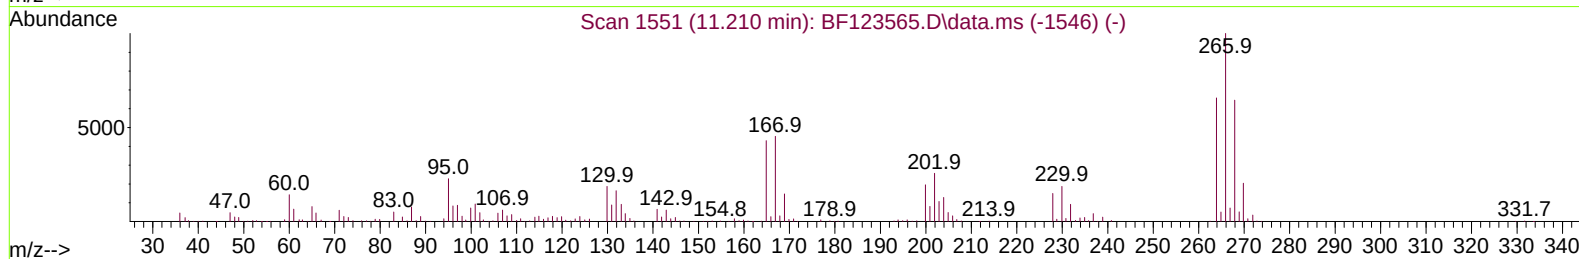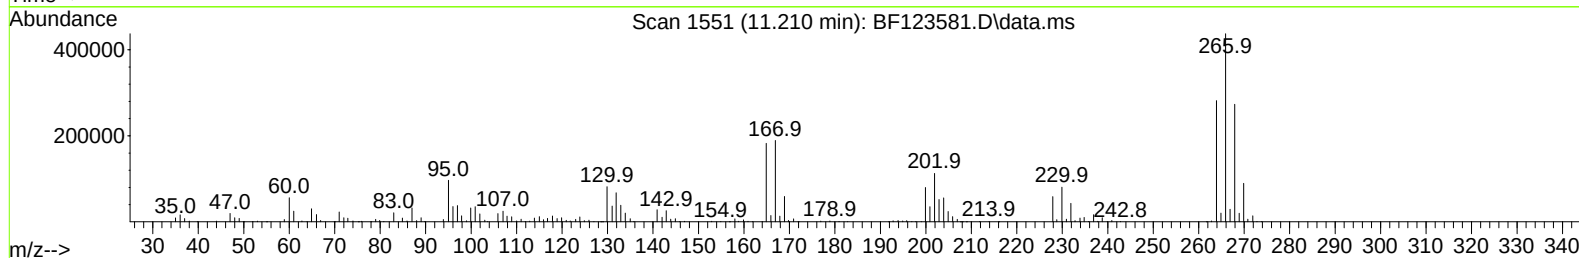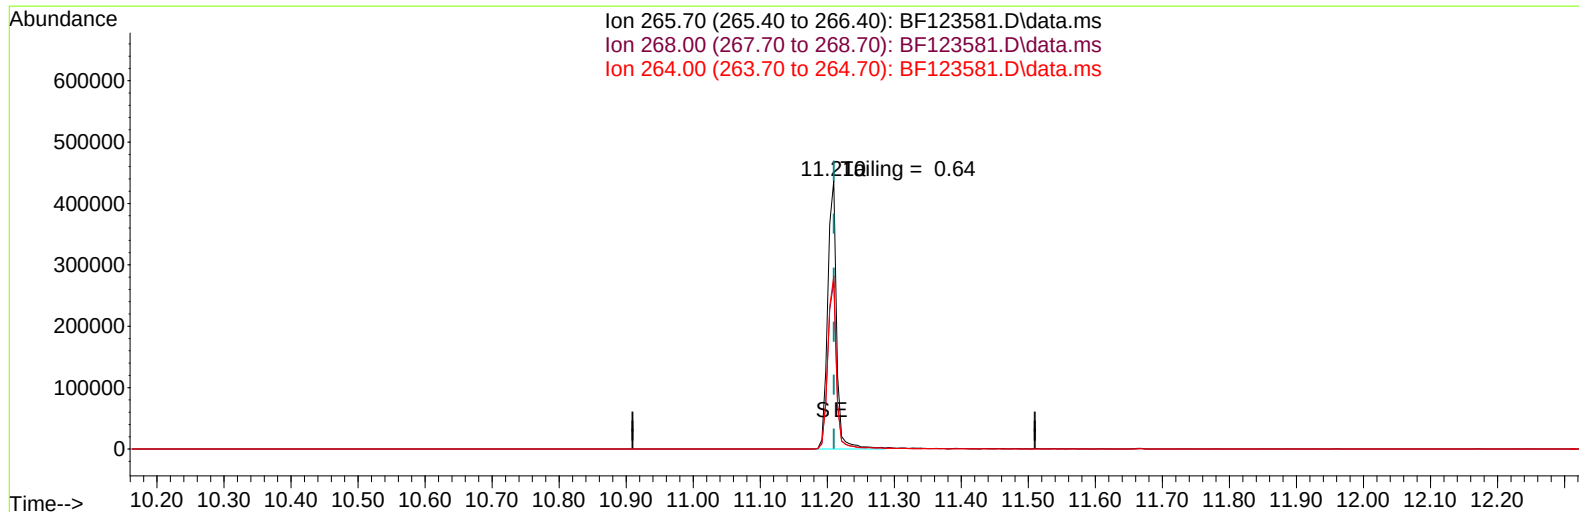

TIC: BF123581.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 39206.74 ng




response 405474

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.46
264.00	65.70	64.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
 Data File : BF123581.D
 Acq On : 16 Apr 2021 8:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 17 05:54:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 10:31:33 2021
 Response via : Initial Calibration

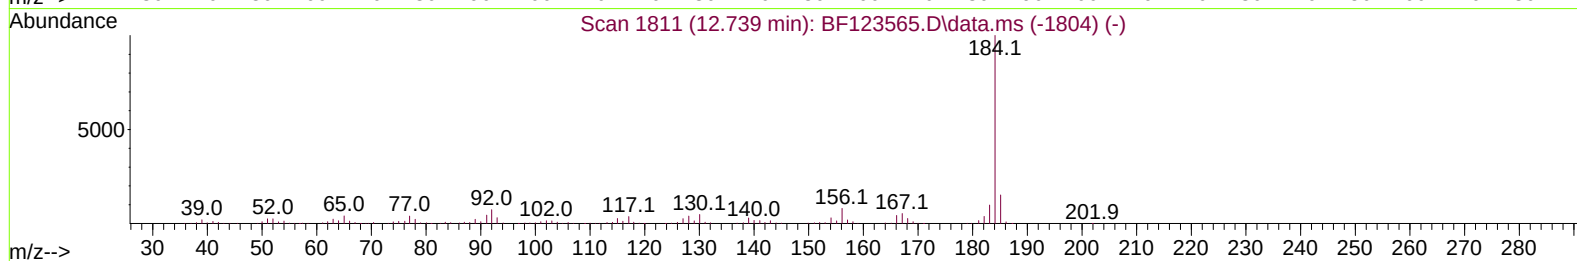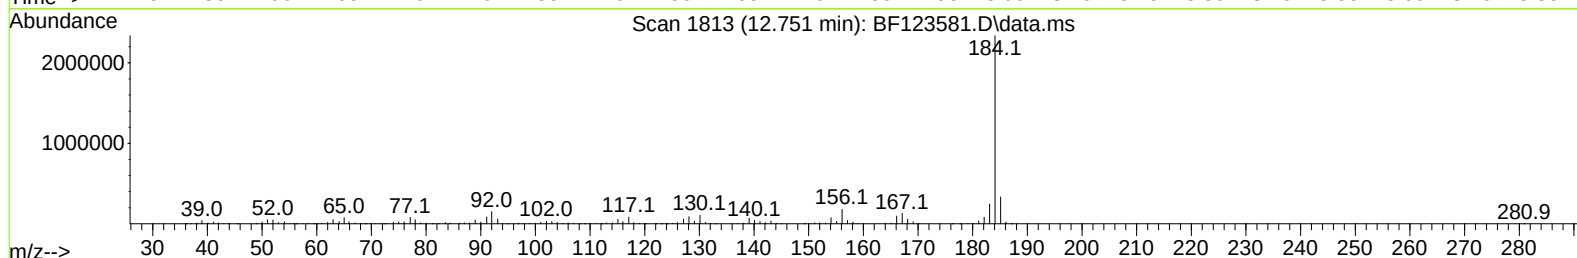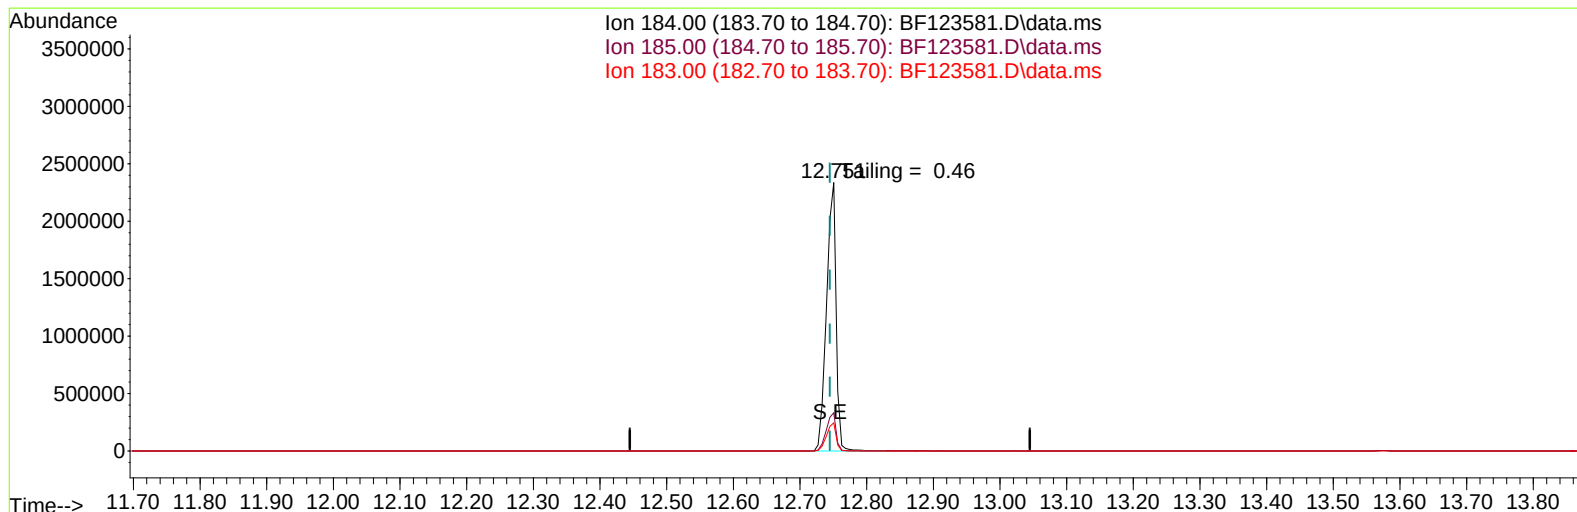

TIC: BF123581.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 2332184

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.24
183.00	9.80	10.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/16/2021	BNA_F	<u>BF123581.D</u>
Compound Name	Response	Retention Time
DDT	993193	13.574
DDD	13421	13.268
DDE	1749	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15170	1008363	1.50