
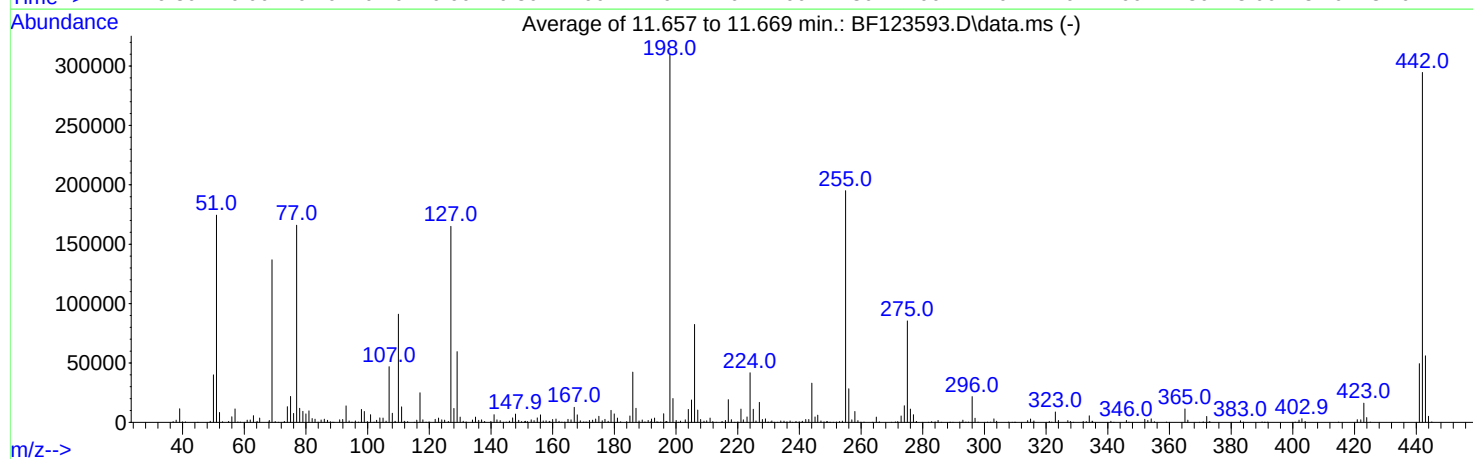


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
 Data File : BF123593.D
 Acq On : 16 Apr 2021 15:32
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 10:31:33 2021

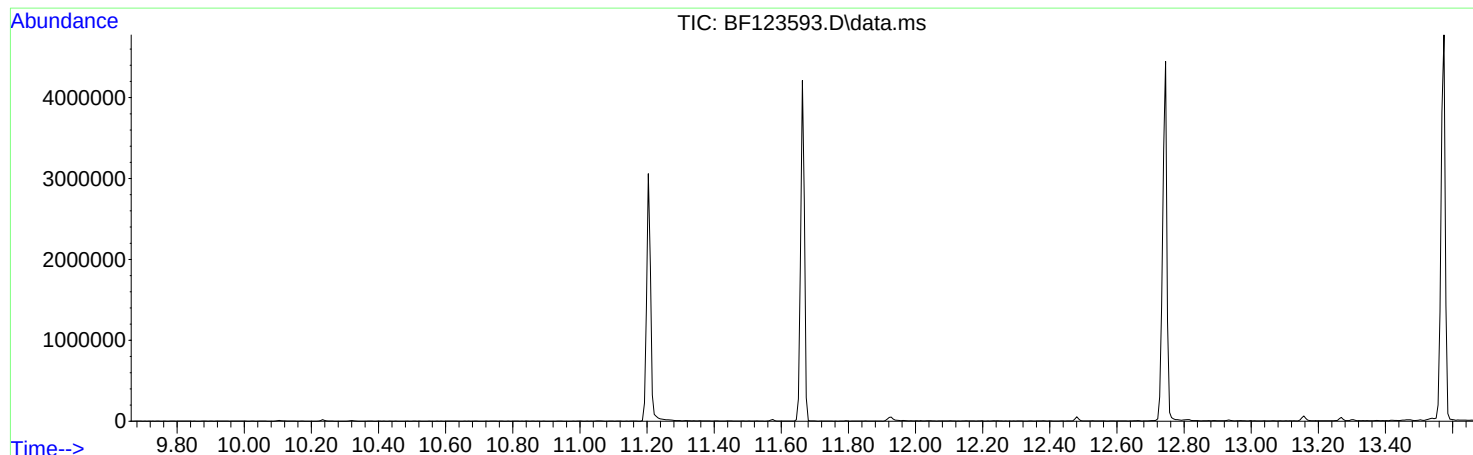




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.3	174515	PASS
68	69	0.00	2	1.2	1628	PASS
69	198	0.00	100	44.2	136896	PASS
70	69	0.00	2	0.5	749	PASS
127	198	10	80	53.3	165099	PASS
197	198	0.00	2	0.3	817	PASS
198	198	100	100	100.0	309717	PASS
199	198	5	9	6.5	20109	PASS
275	198	10	60	27.6	85384	PASS
365	198	1	100	3.7	11309	PASS
441	198	0.01	100	16.0	49519	PASS
442	442	50	100	100.0	294619	PASS
443	442	15	24	19.0	56037	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
 Data File : BF123593.D
 Acq On : 16 Apr 2021 15:32
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 17 05:58:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 10:31:33 2021
 Response via : Initial Calibration

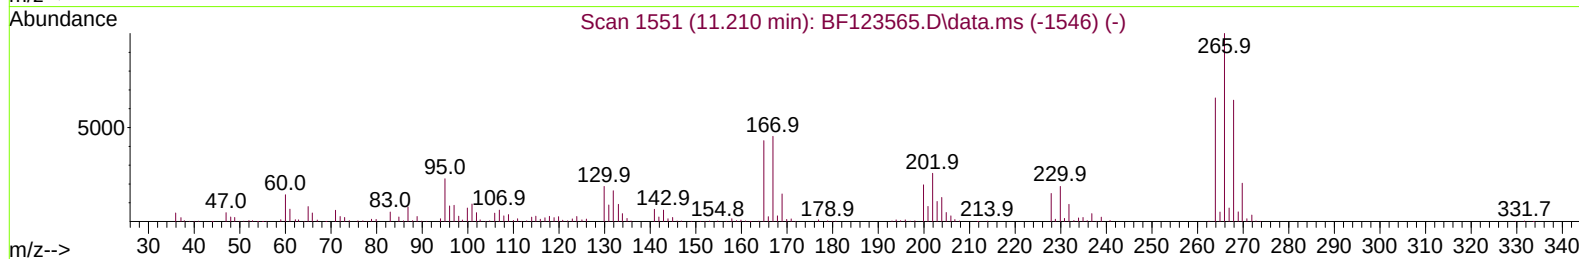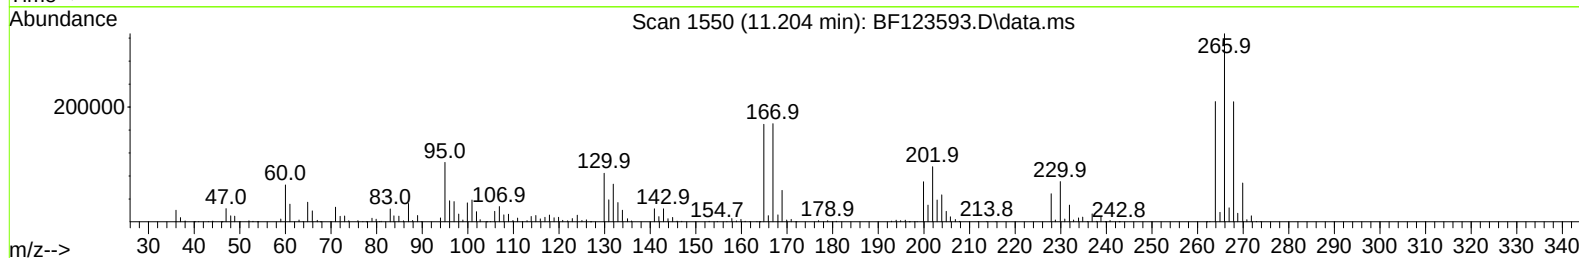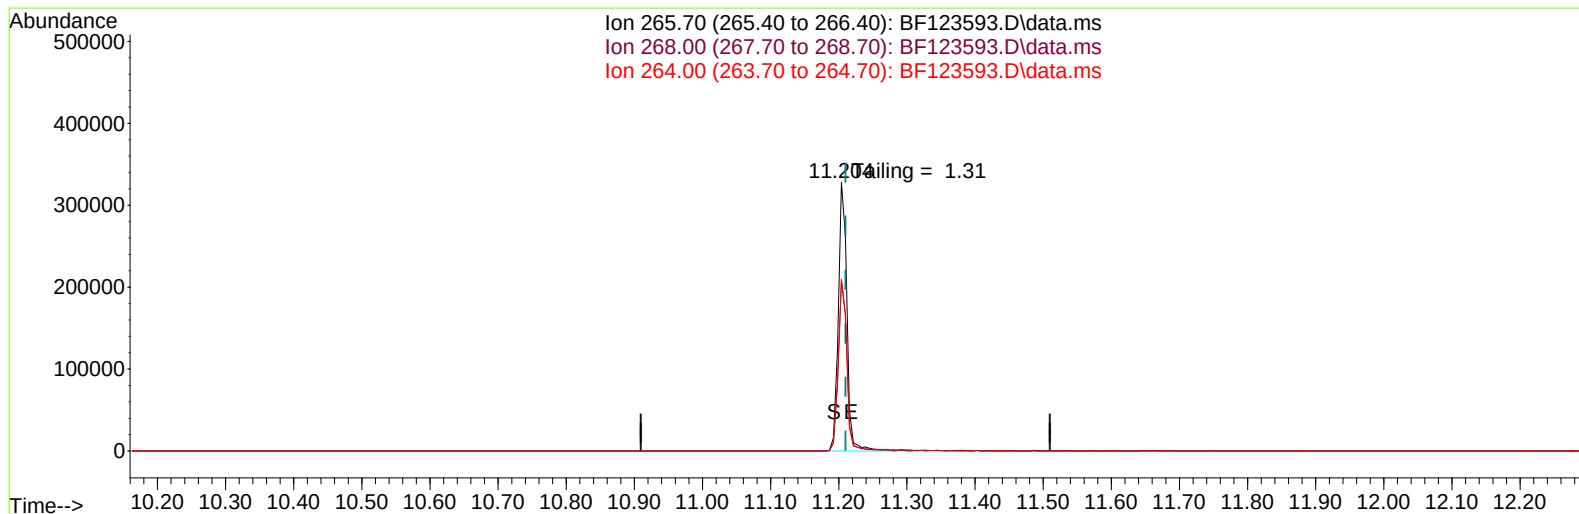

TIC: BF123593.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 38186.39 ng




response 288904

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.86
264.00	65.70	63.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041621\
Data File : BF123593.D
Acq On : 16 Apr 2021 15:32
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 17 05:58:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 10:31:33 2021
Response via : Initial Calibration

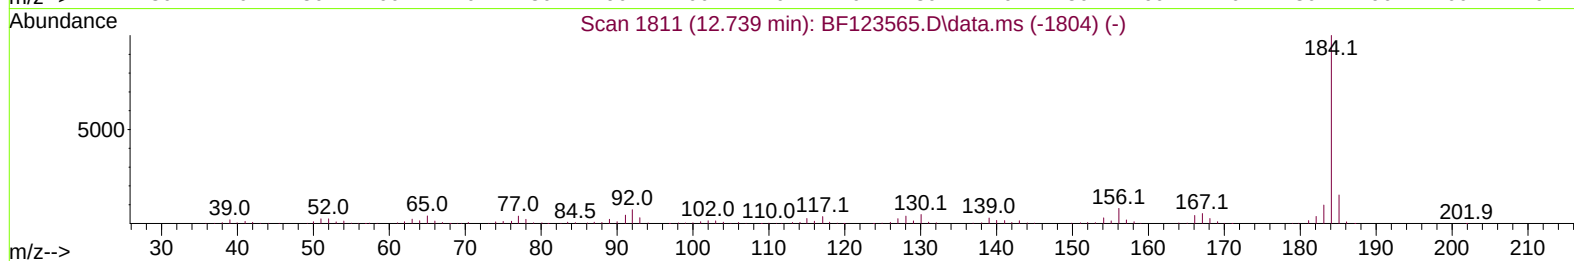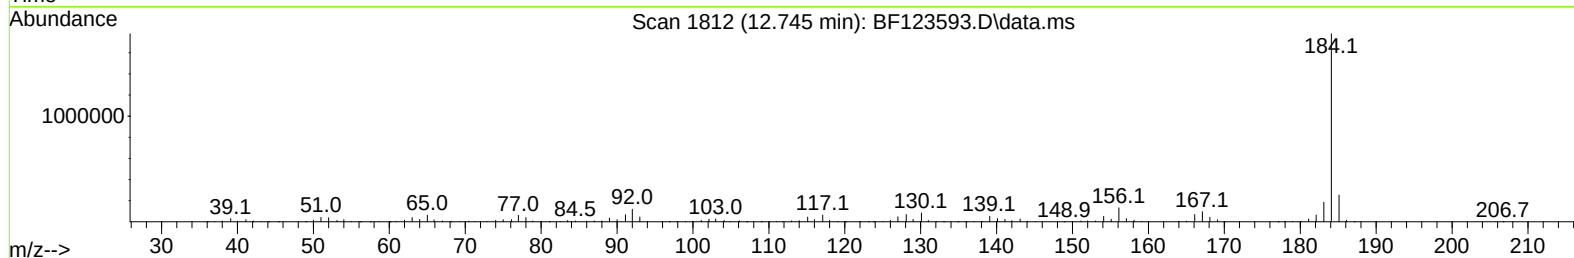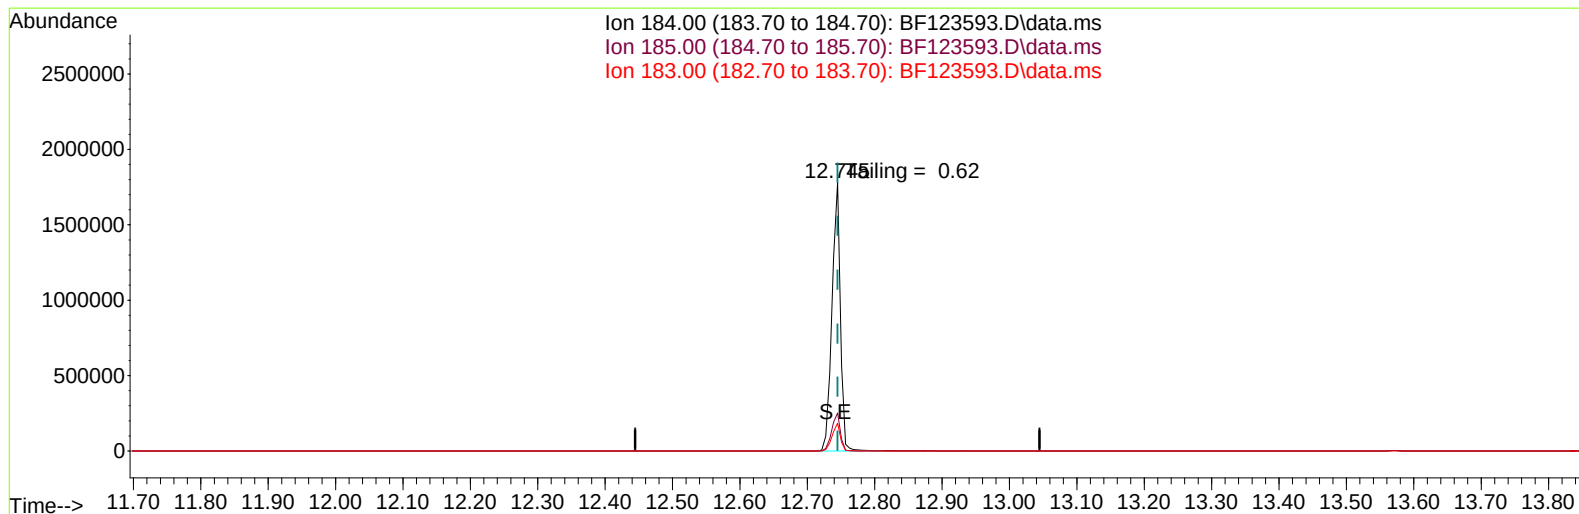

TIC: BF123593.D\data.ms

(77) Benzidine

12.745min (-0.000) 0.00 ng

response 1540069

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.20
183.00	9.80	10.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/16/2021	BNA_F	<u>BF123593.D</u>
Compound Name	Response	Retention Time
DDT	763540	13.574
DDD	9592	13.268
DDE	1566	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11158	774698	1.44

Instrument :
BNA_F
ClientSampleId :
DFTPP