
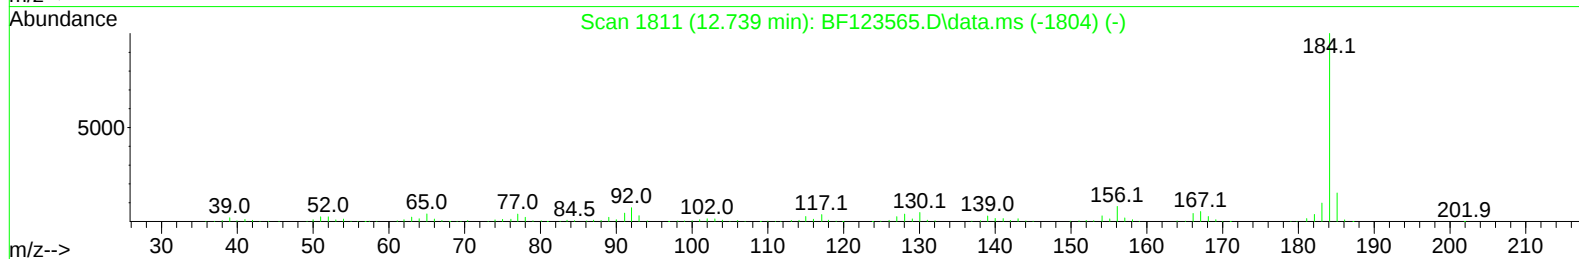
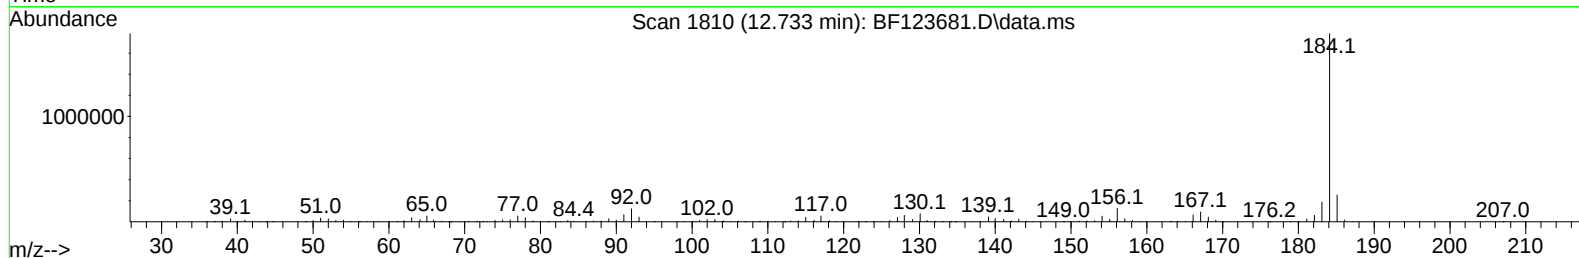


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042221\
Data File : BF123681.D
Acq On : 22 Apr 2021 8:44
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 11:14:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 15:49:40 2021
Response via : Initial Calibration

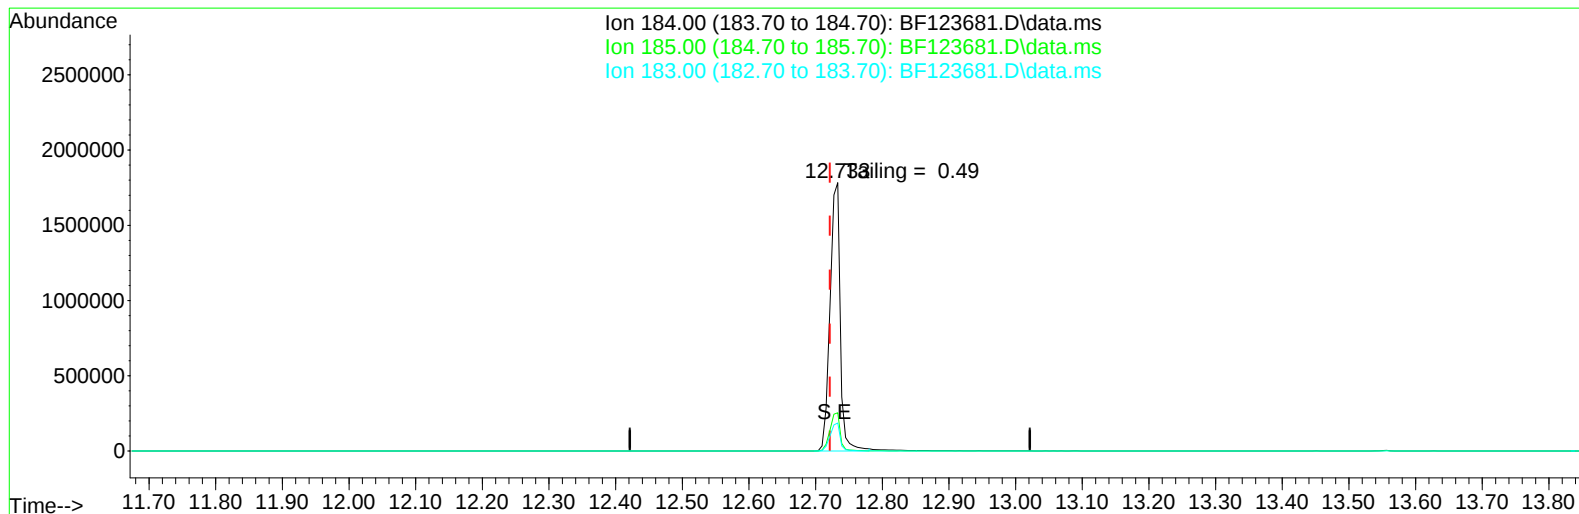

TIC: BF123681.D\data.ms

(77) Benzidine




12.733min (+ 0.012) 593313.02 ng

response 1919287

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.26
183.00	9.80	10.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042221\
Data File : BF123681.D
Acq On : 22 Apr 2021 8:44
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 11:14:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 15:49:40 2021
Response via : Initial Calibration

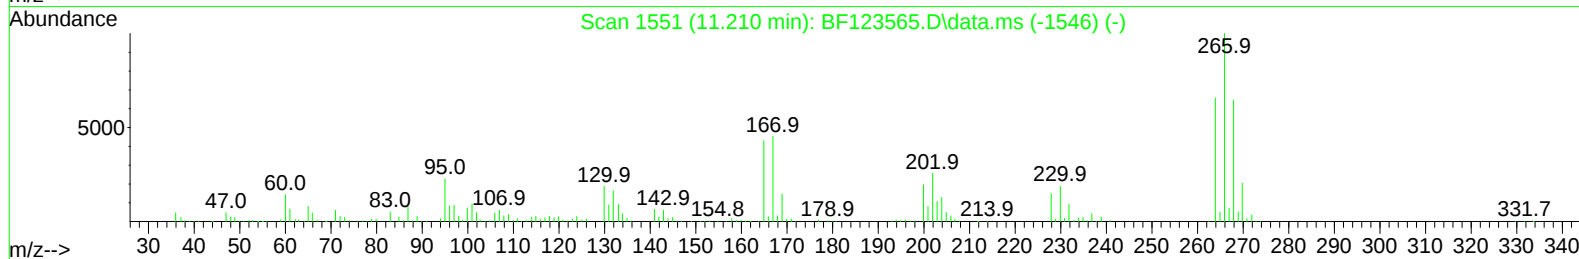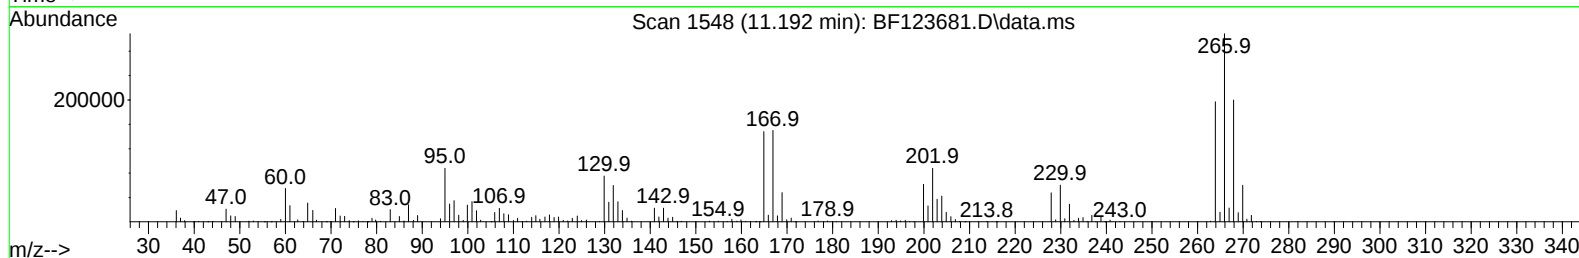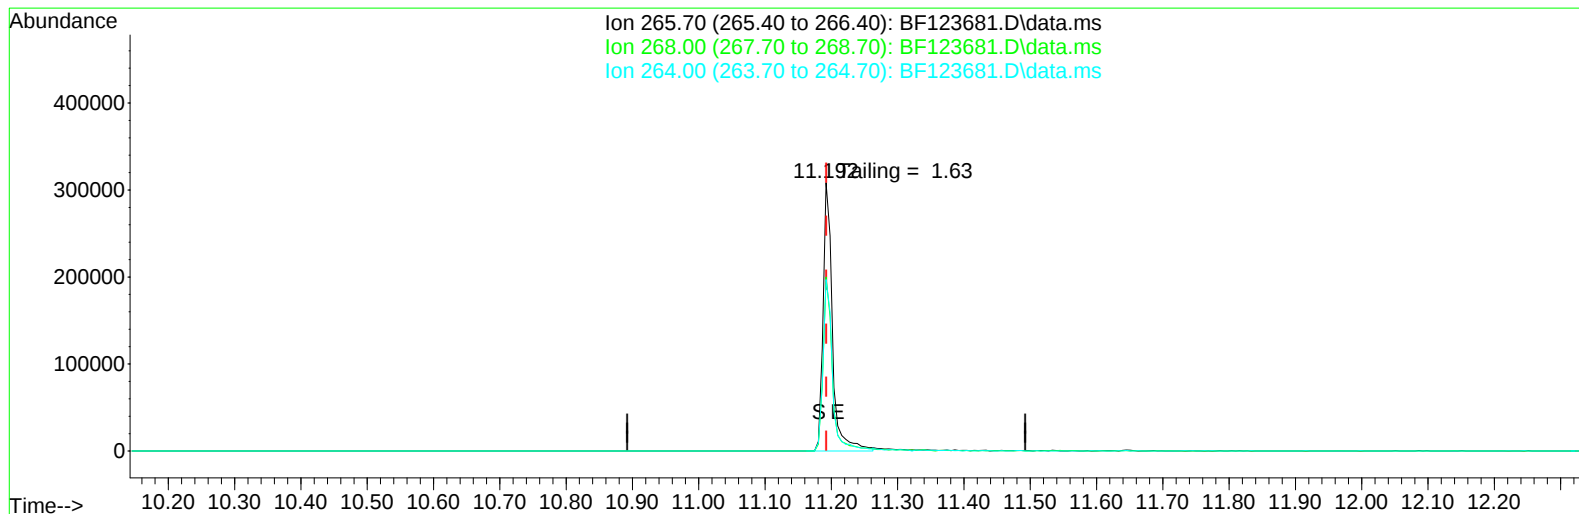

TIC: BF123681.D\data.ms

(70) Pentachlorophenol (C)**11.192min (-0.000) 35168.27 ng****response 312183**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.81
264.00	65.70	63.88
0.00	0.00	0.00