

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042221\
 Data File : BF123683.D
 Acq On : 22 Apr 2021 9:57
 Operator : JU/CG
 Sample : PB135894BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB135894BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.222	19	23	28	rVB2	101374	140599	1.29%	0.206%
2	5.492	574	579	582	rBV	9216483	9405401	86.46%	13.770%
3	6.492	743	749	752	rBV	8480301	9537700	87.68%	13.963%
4	6.851	806	810	813	rBV	2408244	1868699	17.18%	2.736%
5	7.416	900	906	909	rBV	5693146	6632785	60.97%	9.710%
6	8.139	1023	1029	1032	rBV	2472023	2463296	22.64%	3.606%
7	9.216	1206	1212	1216	rBV	9506907	10320385	94.87%	15.109%
8	9.898	1322	1328	1331	rBV	2964346	2675848	24.60%	3.917%
9	10.692	1455	1463	1466	rBV	7351627	7110730	65.37%	10.410%
10	11.386	1577	1581	1584	rBV	3472666	2879041	26.47%	4.215%
11	12.986	1847	1853	1856	rBV	10802042	10878455	100.00%	15.926%
12	14.033	2027	2031	2035	rBV	2320036	2197617	20.20%	3.217%
13	14.504	2105	2111	2116	rBV2	78607	120520	1.11%	0.176%
14	14.815	2159	2164	2167	rBV	94196	111286	1.02%	0.163%
15	15.157	2219	2222	2226	rVB	91690	110212	1.01%	0.161%
16	15.515	2278	2283	2293	rBV2	1204404	1740229	16.00%	2.548%
17	15.992	2360	2364	2369	rVB3	71022	112529	1.03%	0.165%




Sum of corrected areas: 68305332

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042221\
Data File : BF123683.D
Acq On : 22 Apr 2021 9:57
Operator : JU/CG
Sample : PB135894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135894BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

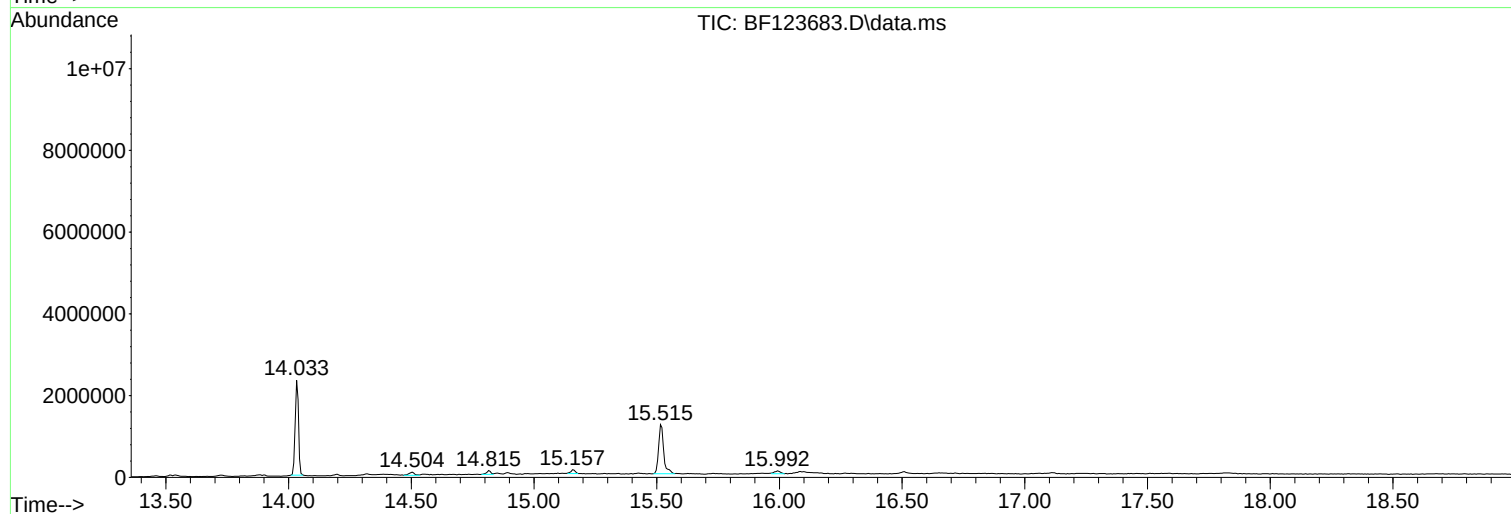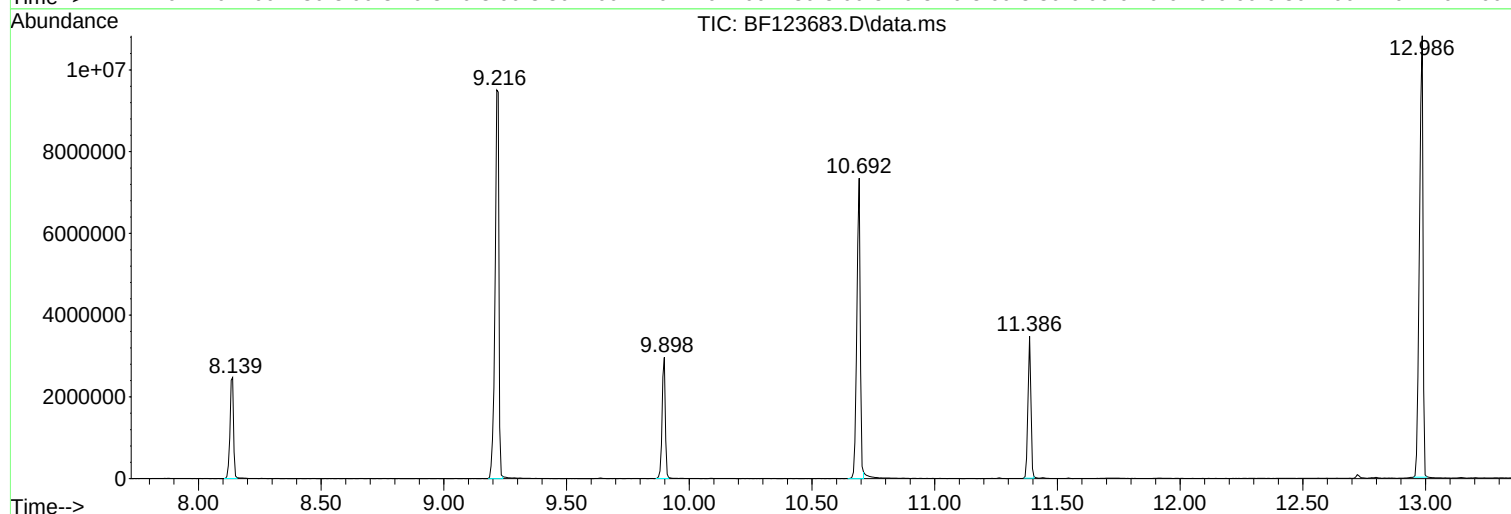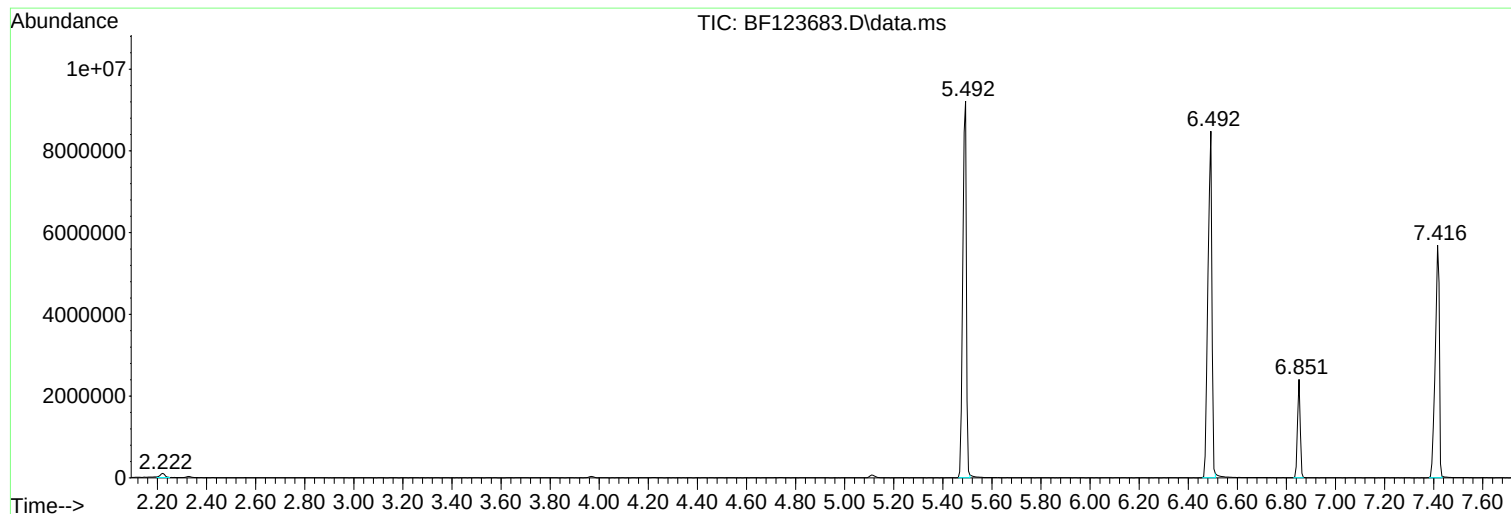

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042221\
Data File : BF123683.D
Acq On : 22 Apr 2021 9:57
Operator : JU/CG
Sample : PB135894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135894BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042221\
Data File : BF123683.D
Acq On : 22 Apr 2021 9:57
Operator : JU/CG
Sample : PB135894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135894BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------