
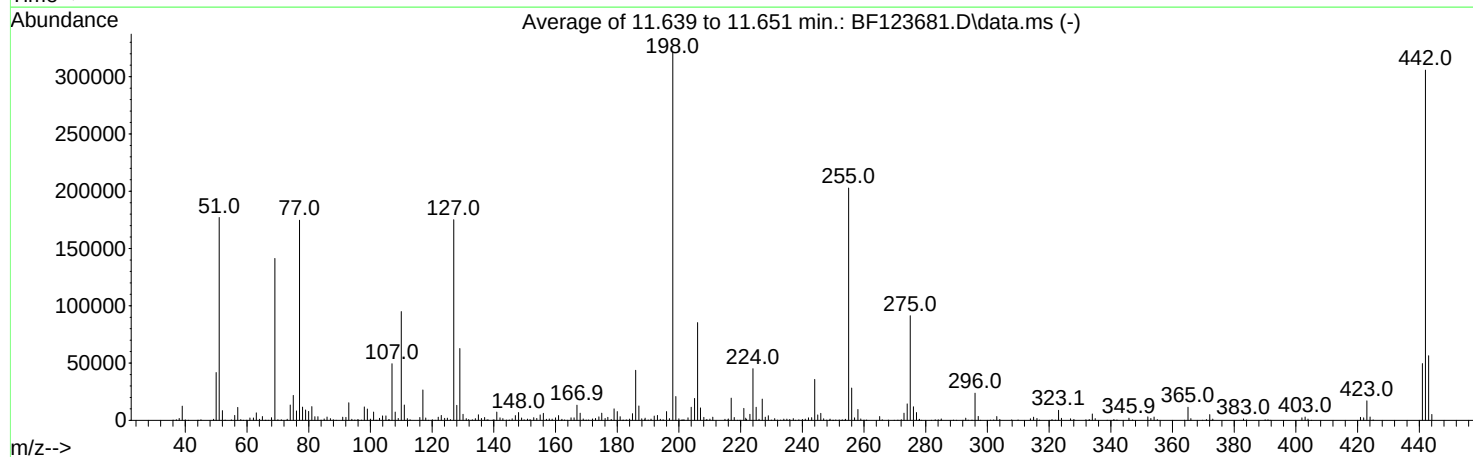


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042221\
 Data File : BF123681.D
 Acq On : 22 Apr 2021 8:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 20 15:49:40 2021

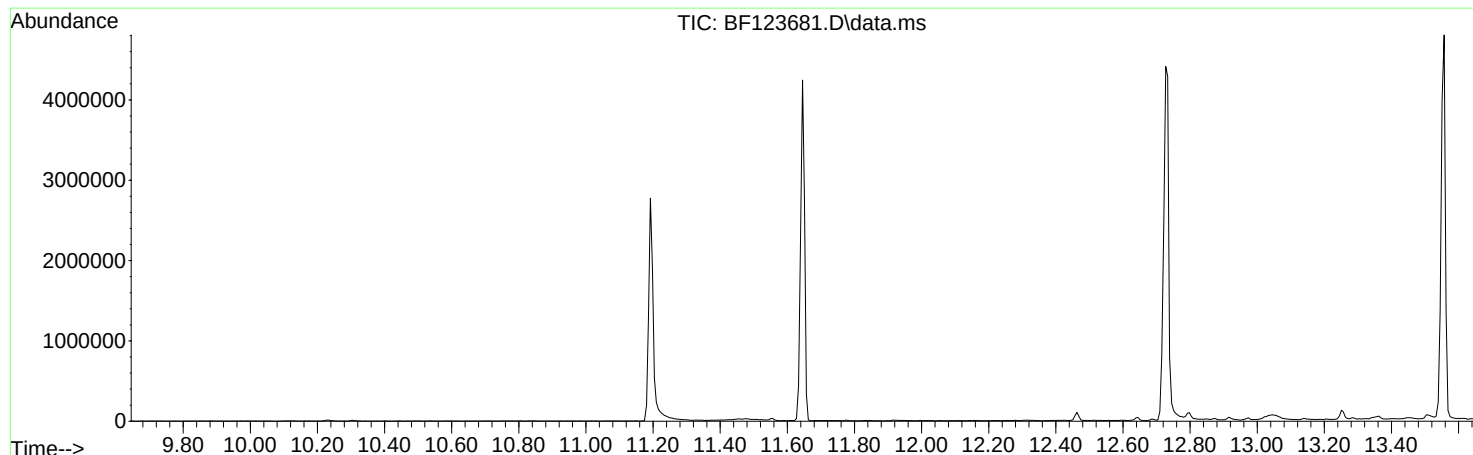




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	177160	PASS
68	69	0.00	2	1.7	2359	PASS
69	198	0.00	100	44.0	141388	PASS
70	69	0.00	2	0.4	623	PASS
127	198	10	80	54.5	175152	PASS
197	198	0.00	2	0.5	1543	PASS
198	198	100	100	100.0	321109	PASS
199	198	5	9	6.5	20821	PASS
275	198	10	60	28.4	91285	PASS
365	198	1	100	3.6	11488	PASS
441	198	0.01	100	15.4	49587	PASS
442	442	50	100	100.0	305733	PASS
443	442	15	24	18.4	56368	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042221\
Data File : BF123681.D
Acq On : 22 Apr 2021 8:44
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 22 11:14:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 15:49:40 2021
Response via : Initial Calibration

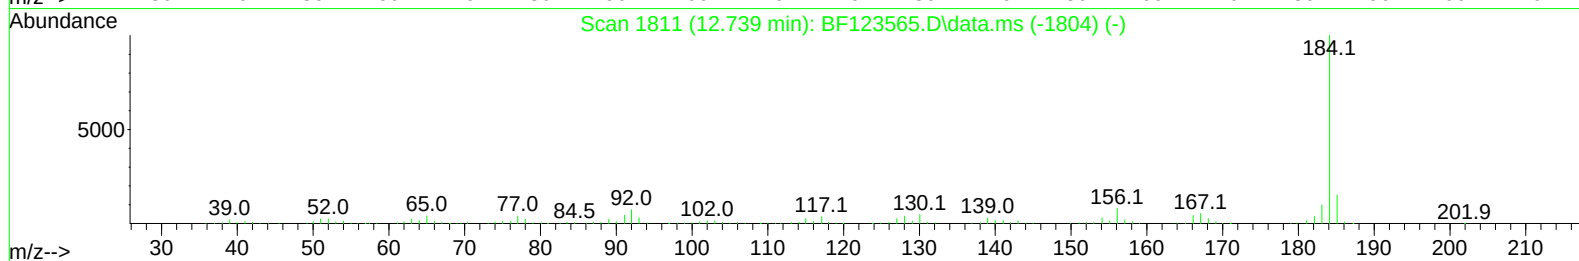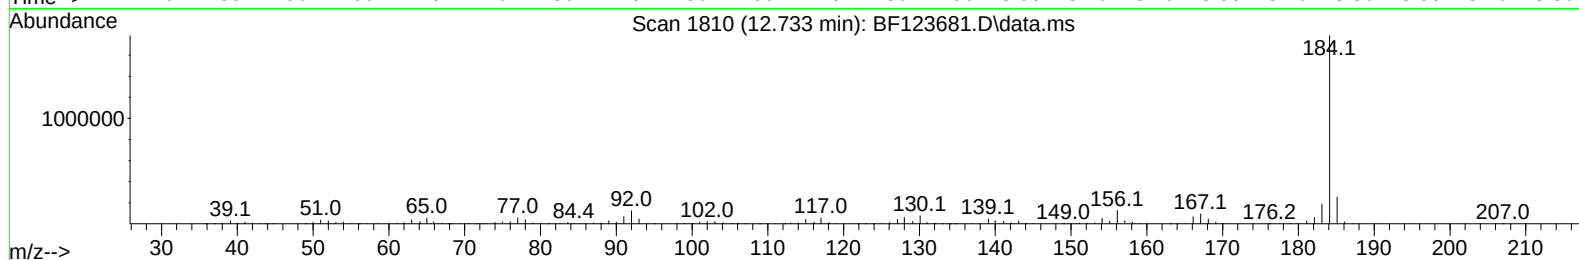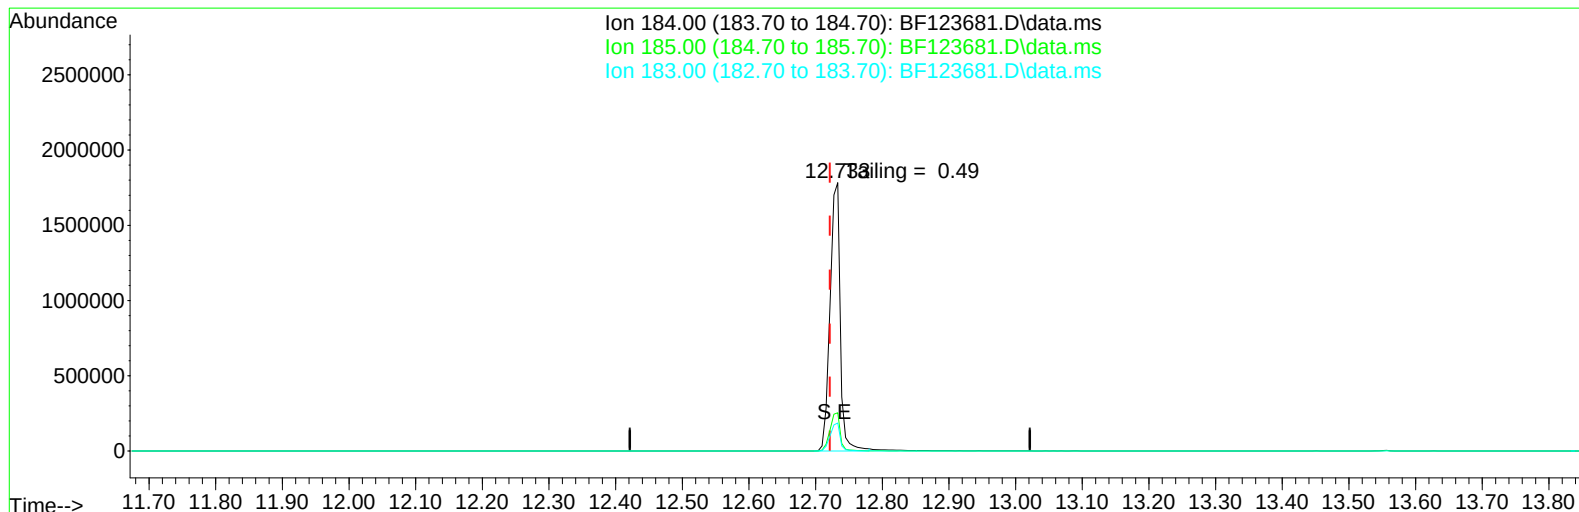

TIC: BF123681.D\data.ms

(77) Benzidine

12.733min (+ 0.012) 593313.02 ng




response 1919287

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.26
183.00	9.80	10.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042221\
Data File : BF123681.D
Acq On : 22 Apr 2021 8:44
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 22 11:14:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 15:49:40 2021
Response via : Initial Calibration

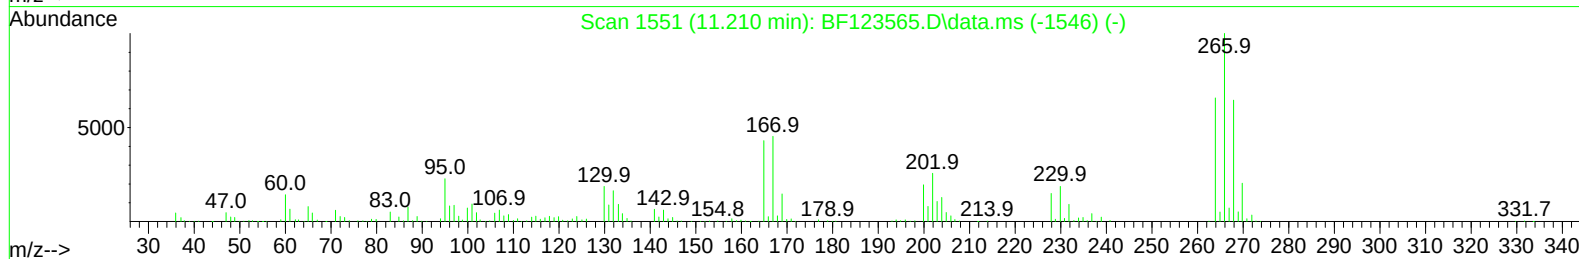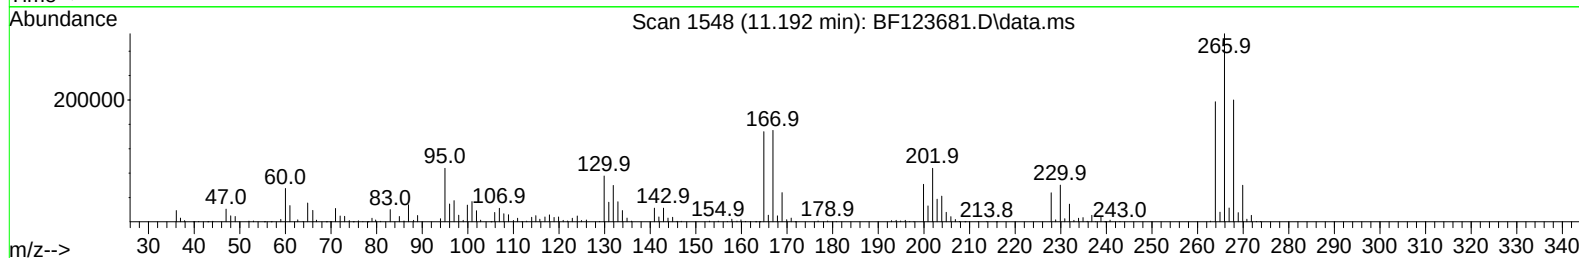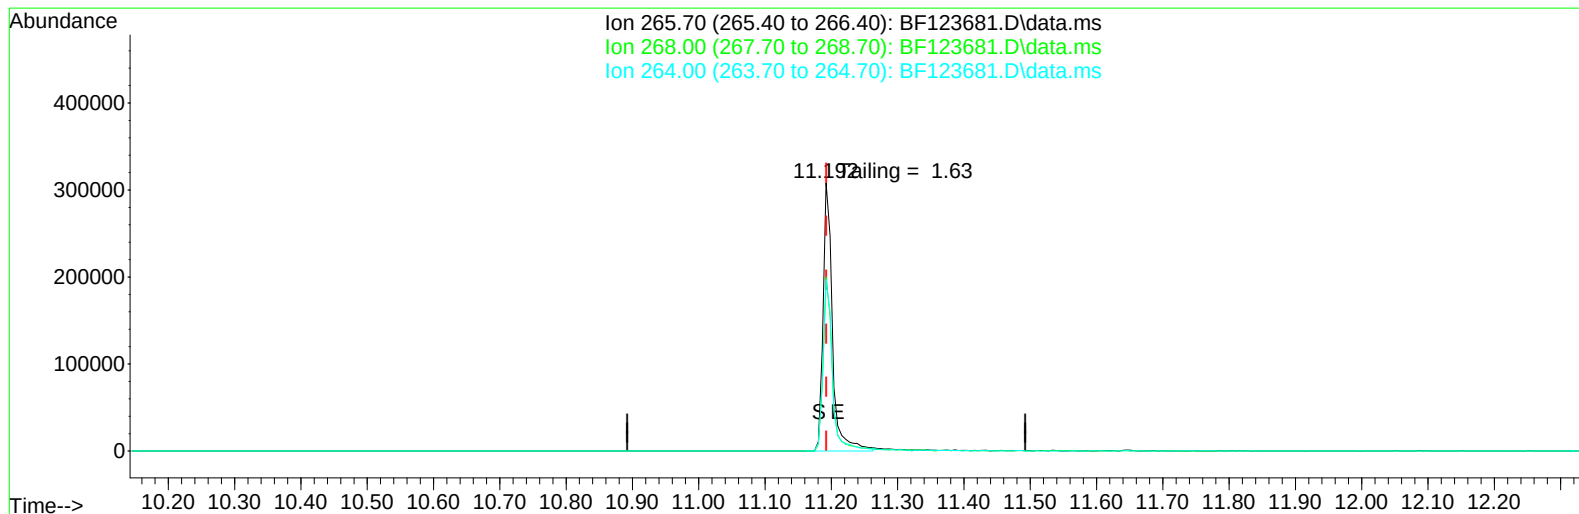

TIC: BF123681.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.000) 35168.27 ng

response 312183

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.81
264.00	65.70	63.88
0.00	0.00	0.00

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/22/2021	BNA_F	<u>BF123681.D</u>
Compound Name	Response	Retention Time
DDT	774546	13.55
DDD	21329	13.25
DDE	4286	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25615	800161	3.20