
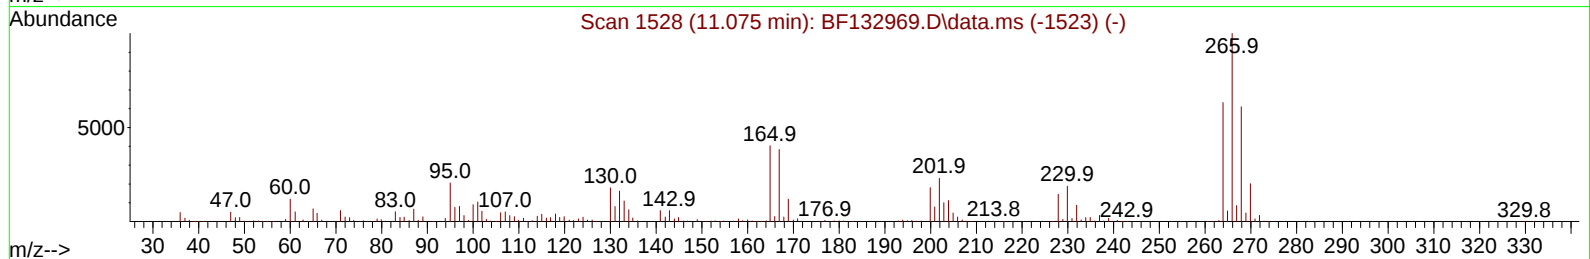
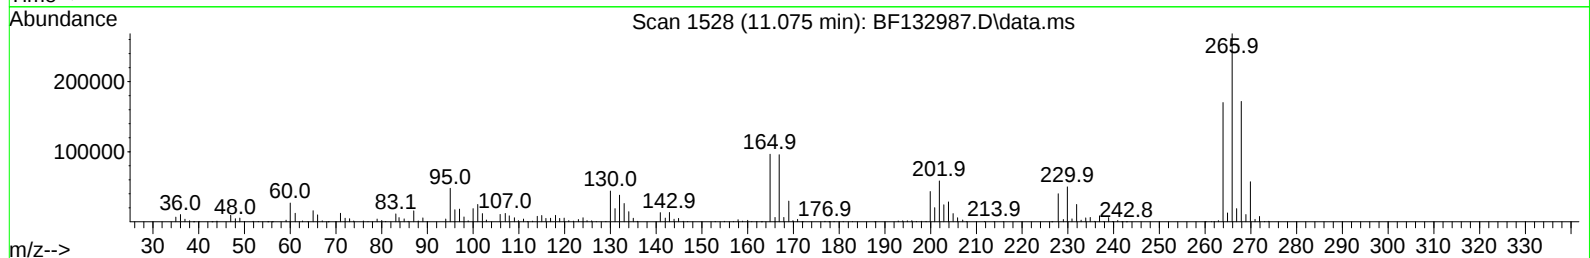


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042423\
Data File : BF132987.D
Acq On : 24 Apr 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 06:12:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

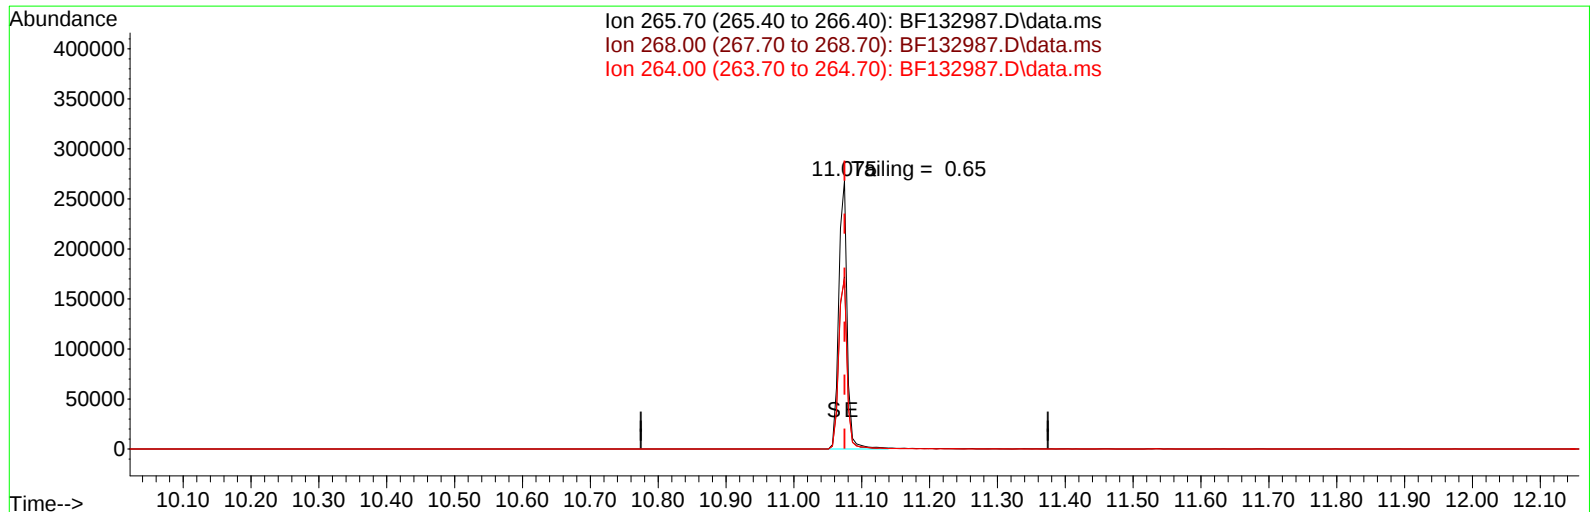

TIC: BF132987.D\data.ms

(70) Pentachlorophenol (C)




11.075min (0.000) 303360.47 ng

response 230501

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.03
264.00	63.30	63.43
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042423\  
Data File : BF132987.D  
Acq On    : 24 Apr 2023  10:25  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 25 06:12:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

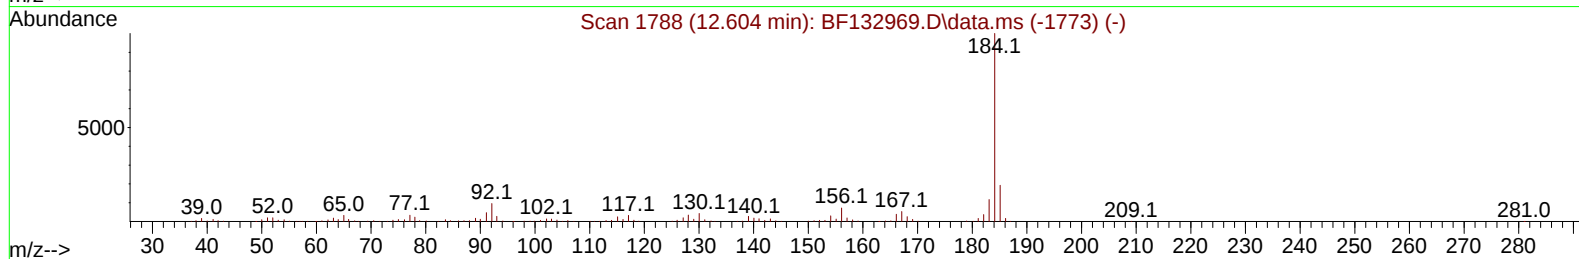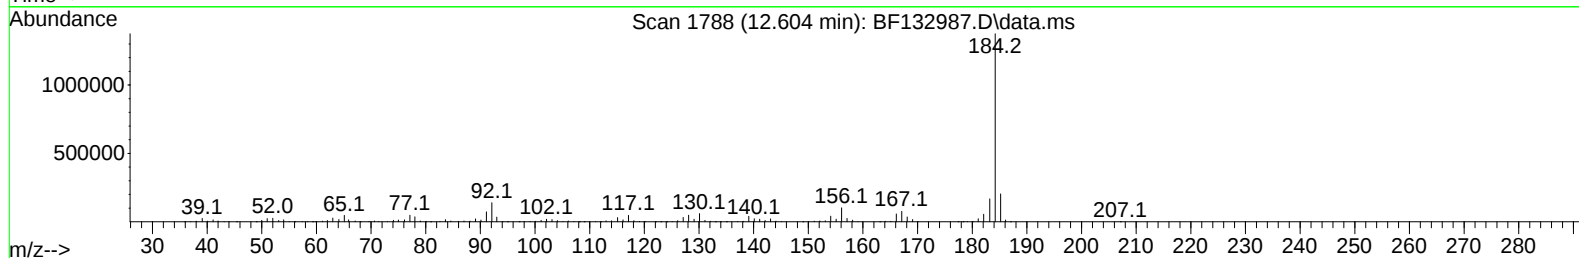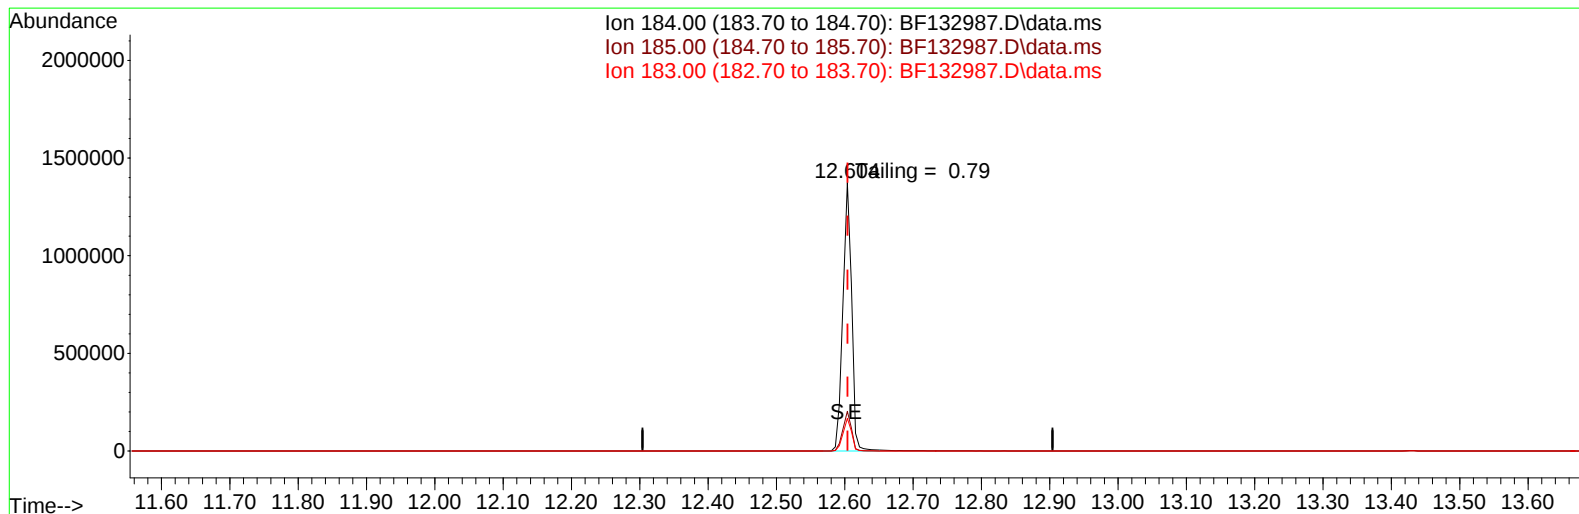

TIC: BF132987.D\data.ms

(77) Benzidine

12.604min (-0.000) 10332.41 ng

response **1226755**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.82#
183.00	11.70	12.20
0.00	0.00	0.00