
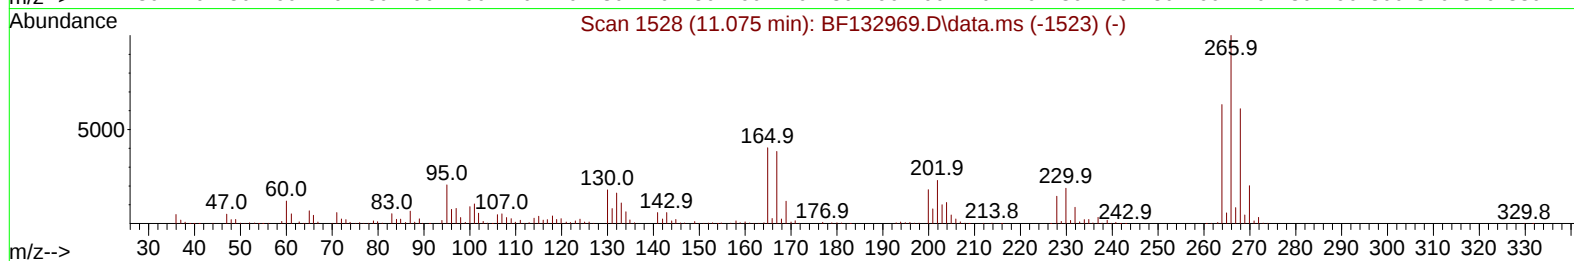
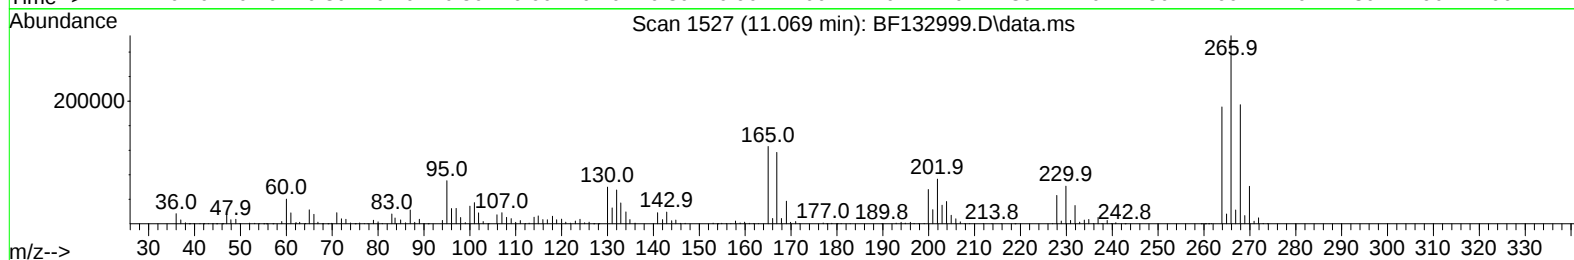


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042423\
Data File : BF132999.D
Acq On : 24 Apr 2023 17:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 06:14:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

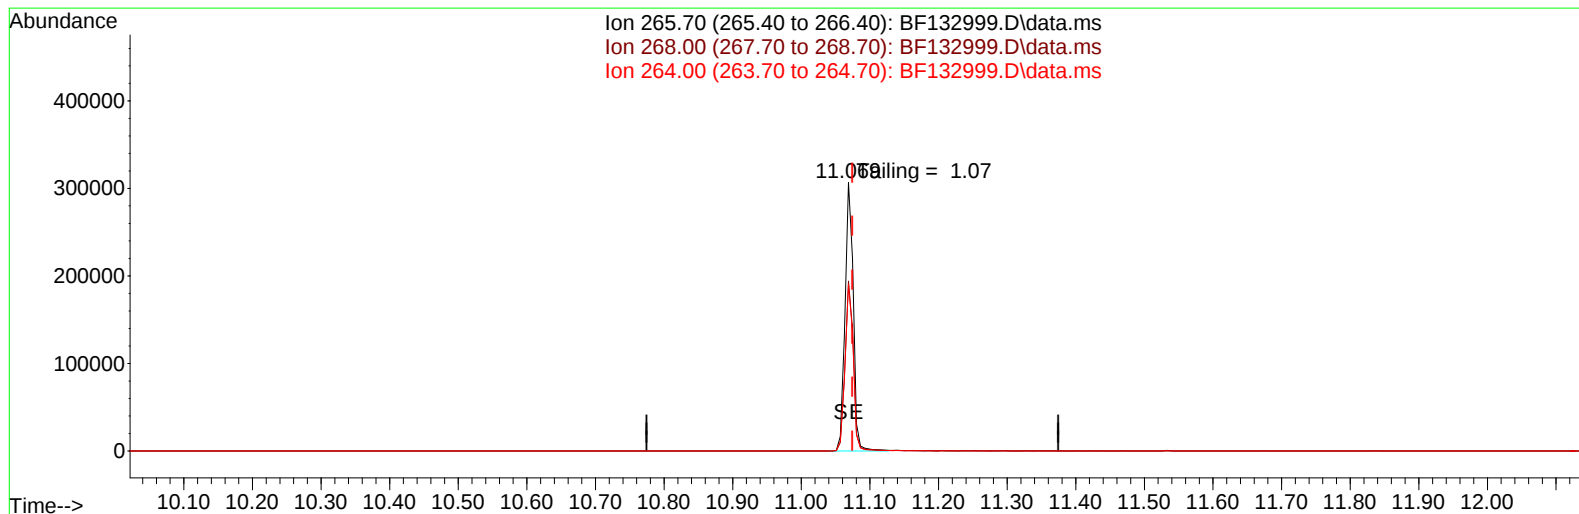

TIC: BF132999.D\data.ms

(70) Pentachlorophenol (C)




11.069min (-0.006) 35166.94 ng

response 255517

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.35
264.00	63.30	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042423\
Data File : BF132999.D
Acq On : 24 Apr 2023 17:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 06:14:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

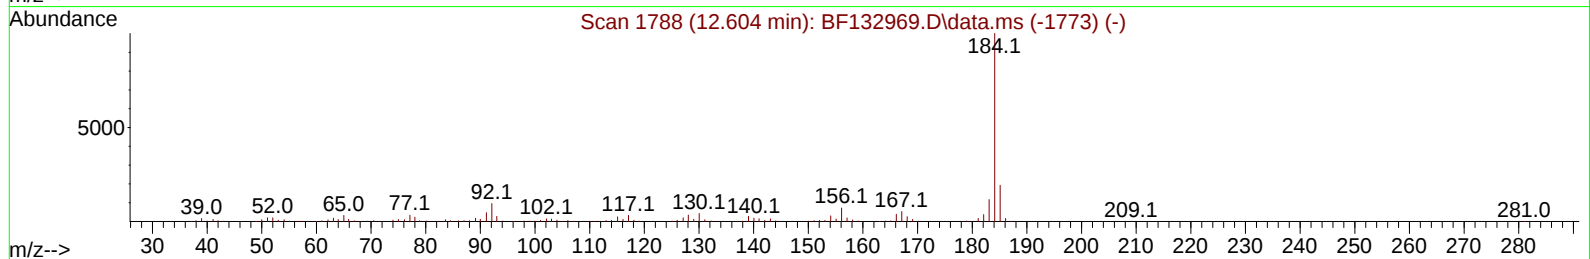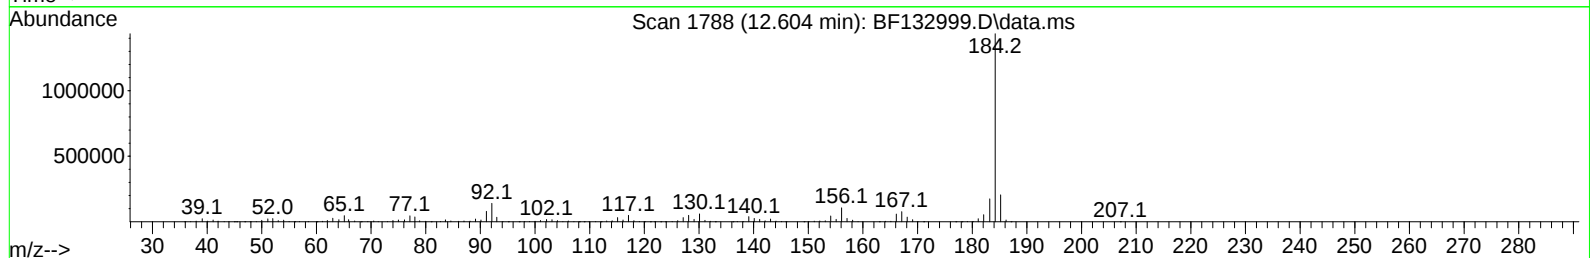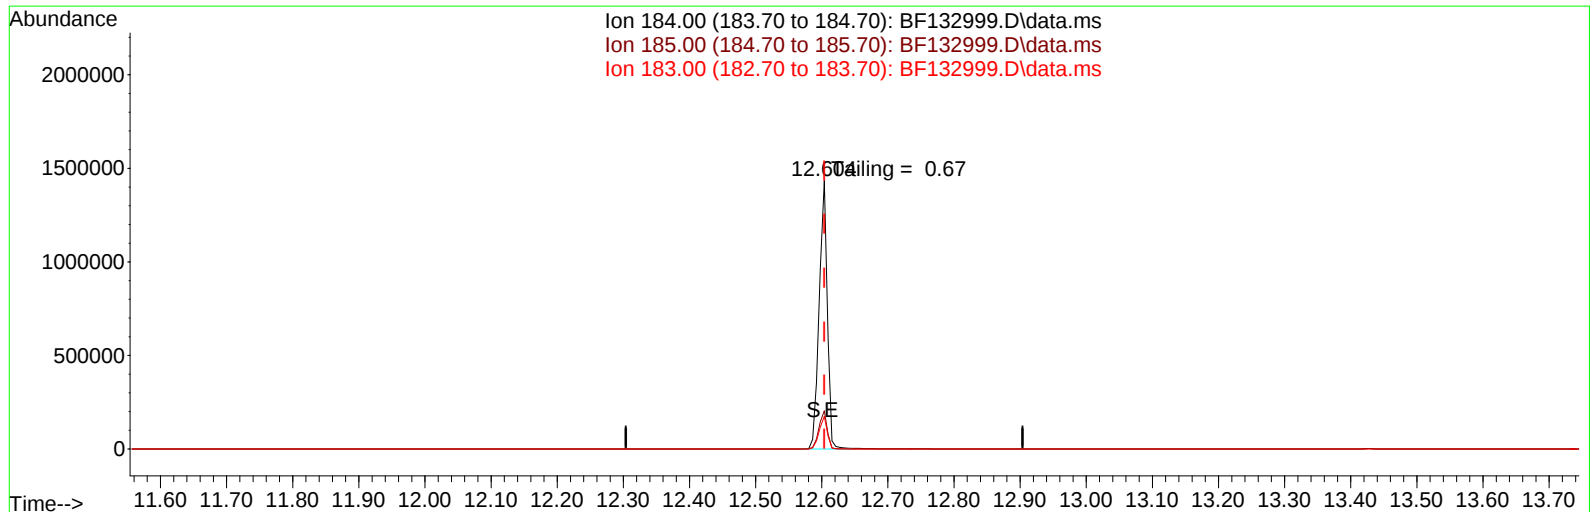

TIC: BF132999.D\data.ms

(77) Benzidine

12.604min (-0.000) 0.00 ng

response 1234836

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.29#
183.00	11.70	12.18
0.00	0.00	0.00