
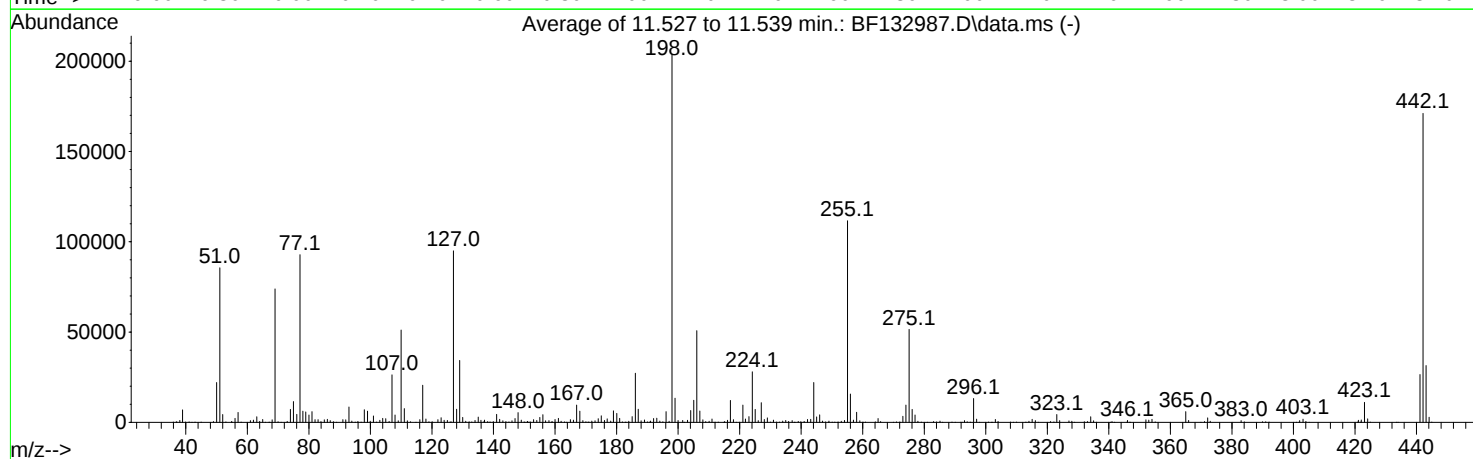


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042423\
 Data File : BF132987.D
 Acq On : 24 Apr 2023 10:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Apr 22 03:30:56 2023

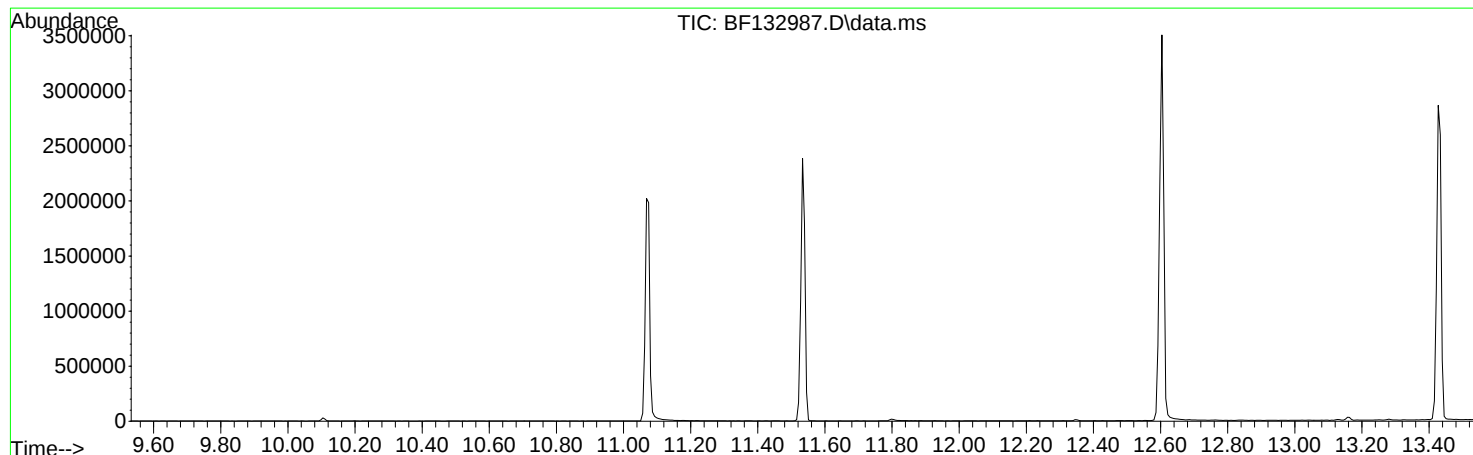

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	85579	PASS
68	69	0.00	2	1.9	1412	PASS
69	198	0.00	100	36.3	73901	PASS
70	69	0.00	2	0.5	380	PASS
127	198	10	80	46.6	95000	PASS
197	198	0.00	2	0.3	625	PASS
198	198	100	100	100.0	203712	PASS
199	198	5	9	6.6	13428	PASS
275	198	10	60	25.3	51467	PASS
365	198	1	100	2.9	5903	PASS
441	198	0.01	100	13.0	26462	PASS
442	442	50	100	100.0	171112	PASS
443	442	15	24	18.4	31482	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/24/2023	BNA_F	<u>BF132987.D</u>
Compound Name	Response	Retention Time
DDT	507625	13.433
DDD	5370	13.163
DDE	0	12.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5370	512995	1.05

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042423\
Data File : BF132987.D
Acq On : 24 Apr 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 25 06:12:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

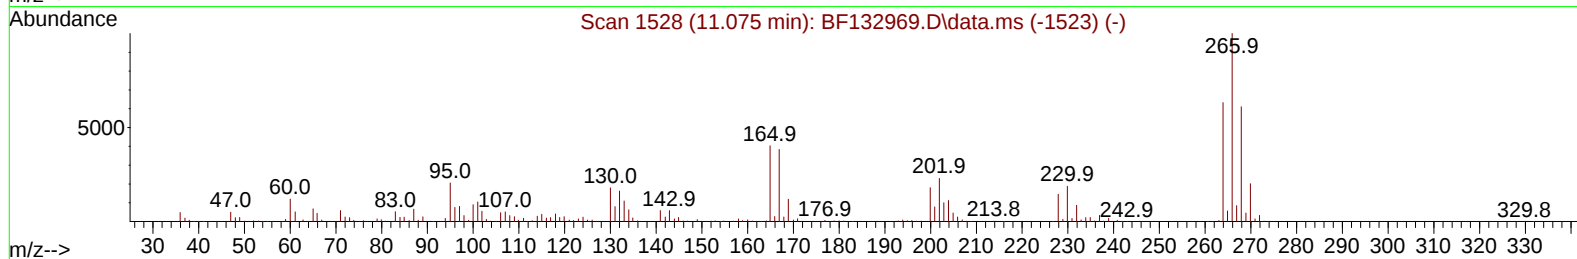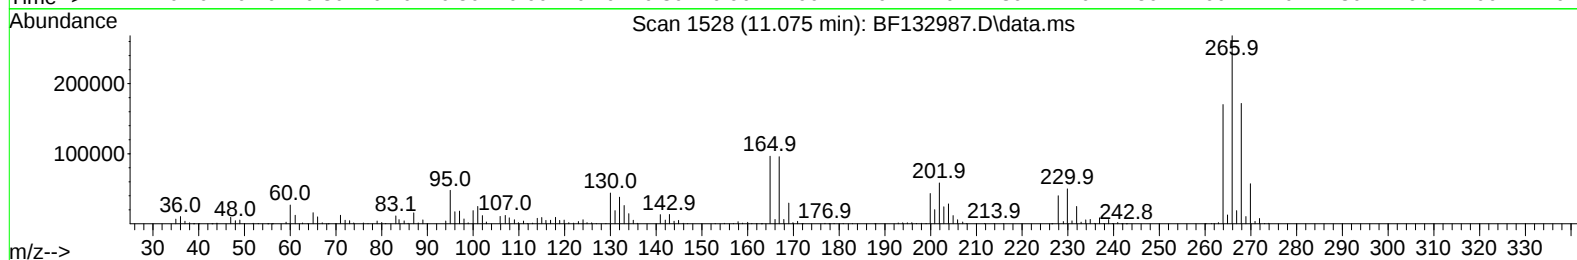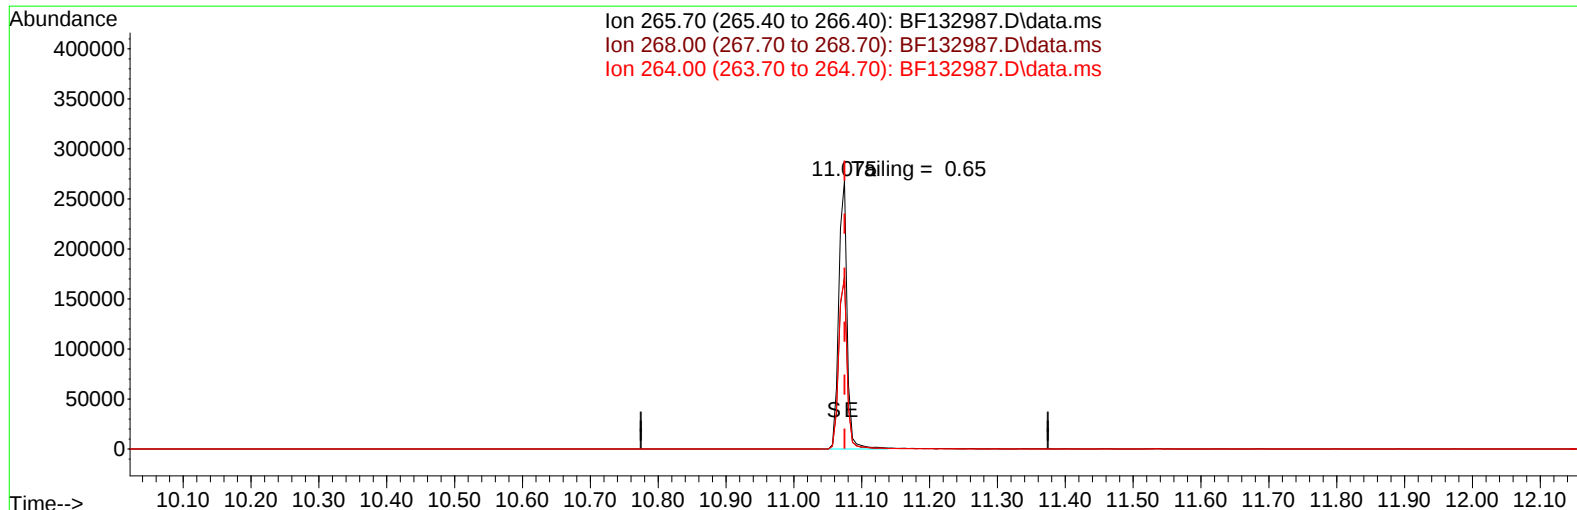

TIC: BF132987.D\data.ms

(70) Pentachlorophenol (C)

11.075min (0.000) 303360.47 ng




response 230501

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.03
264.00	63.30	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042423\
Data File : BF132987.D
Acq On : 24 Apr 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 25 06:12:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

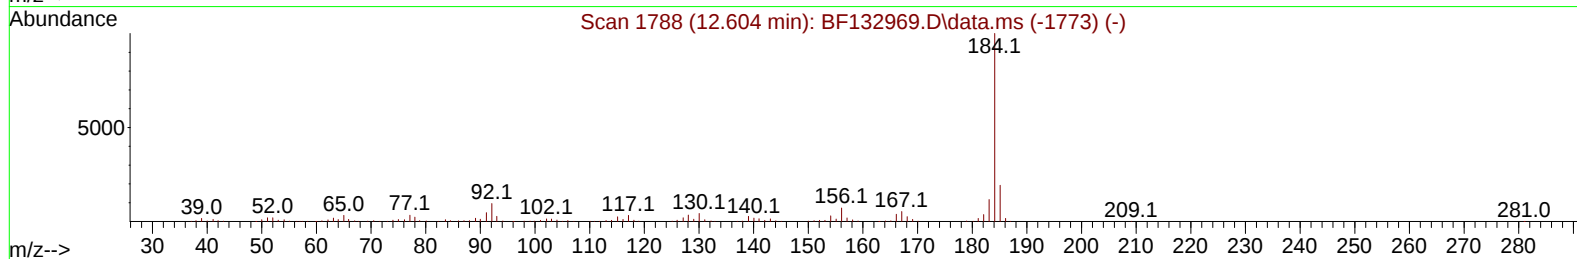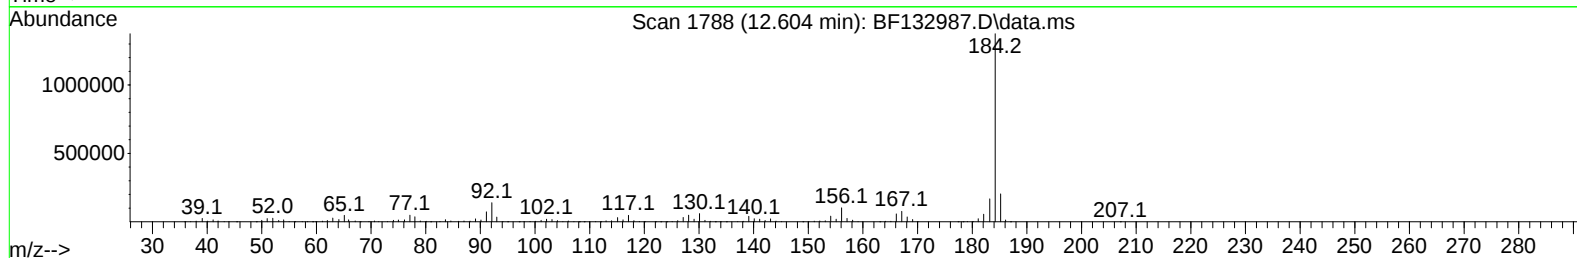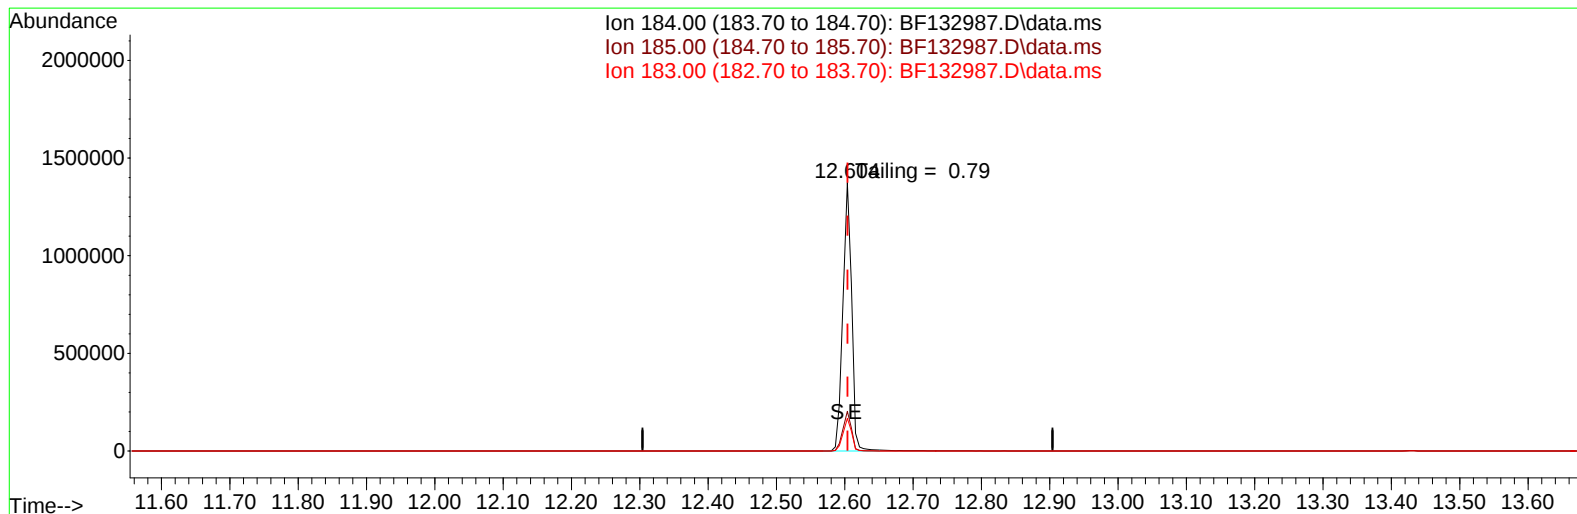

TIC: BF132987.D\data.ms

(77) Benzidine

12.604min (-0.000) 10332.41 ng

response 1226755

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.82#
183.00	11.70	12.20
0.00	0.00	0.00