
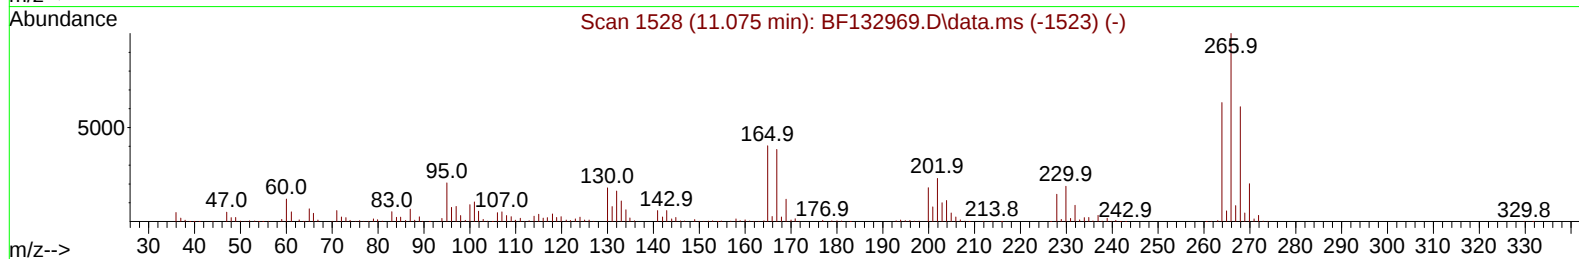
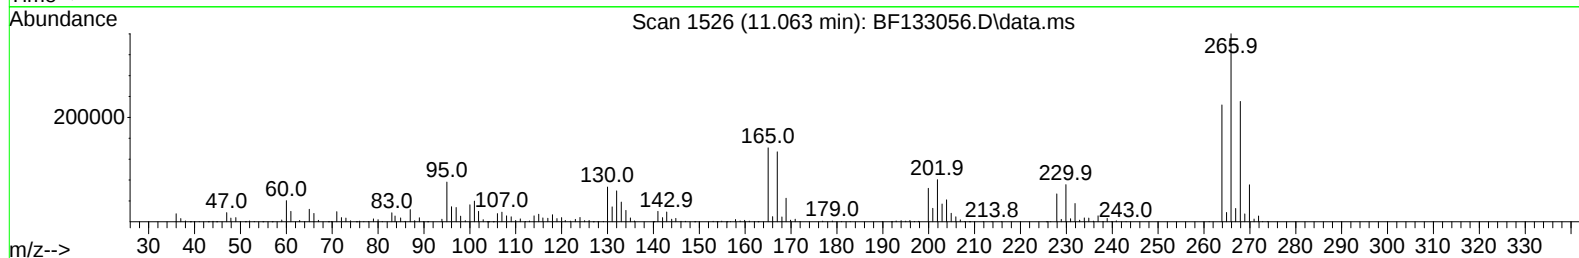


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133056.D
Acq On : 26 Apr 2023 10:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:24:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:56:03 2023
Response via : Initial Calibration

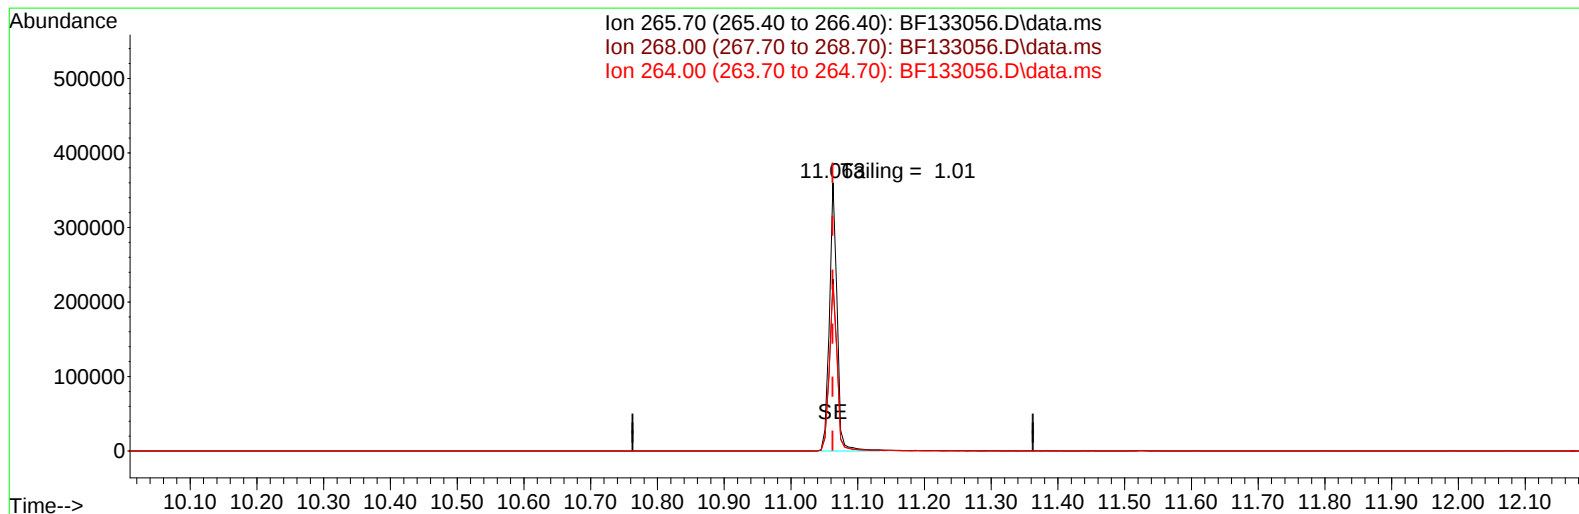

TIC: BF133056.D\data.ms

(70) Pentachlorophenol (C)




11.063min (+ 0.000) 32077.95 ng

response 291722

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.05
264.00	63.30	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133056.D
Acq On : 26 Apr 2023 10:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:24:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:56:03 2023
Response via : Initial Calibration

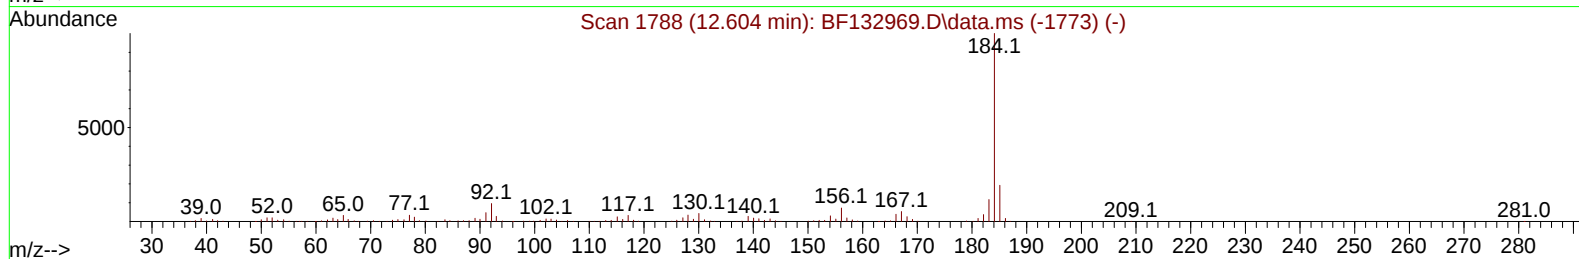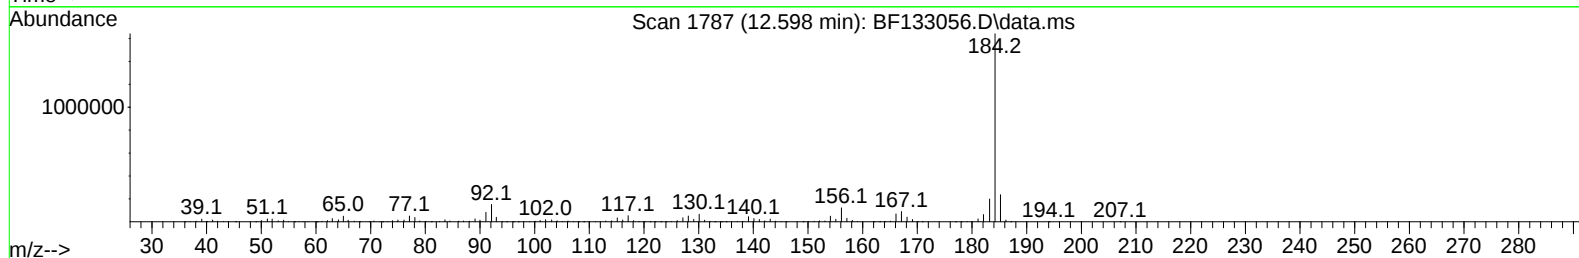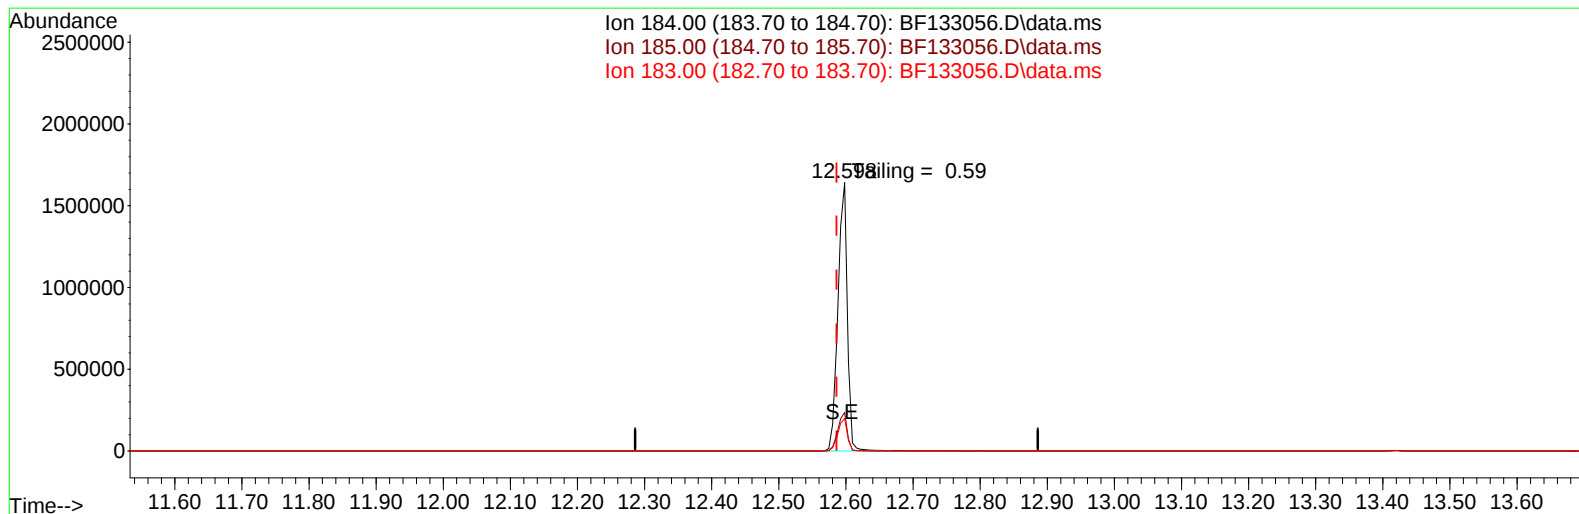

TIC: BF133056.D\data.ms

(77) Benzidine**12.598min (+ 0.012) 1715984.49 ng****response 1596001**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.39#
183.00	11.70	12.07
0.00	0.00	0.00