
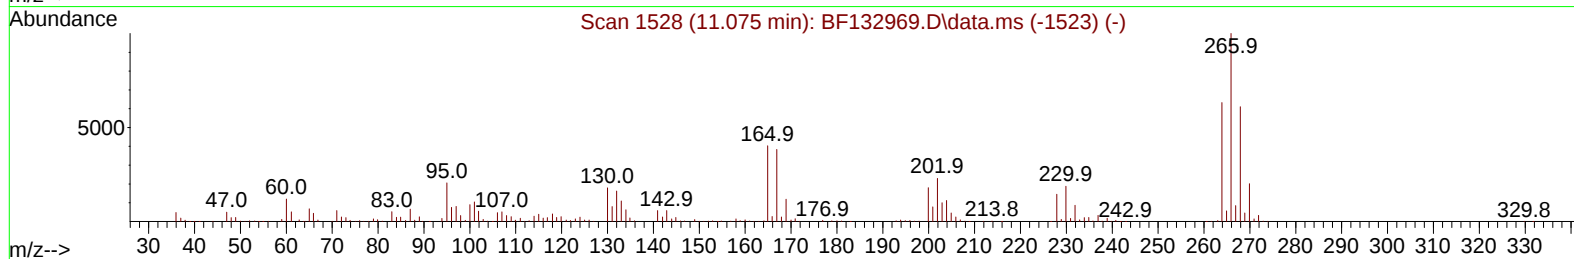
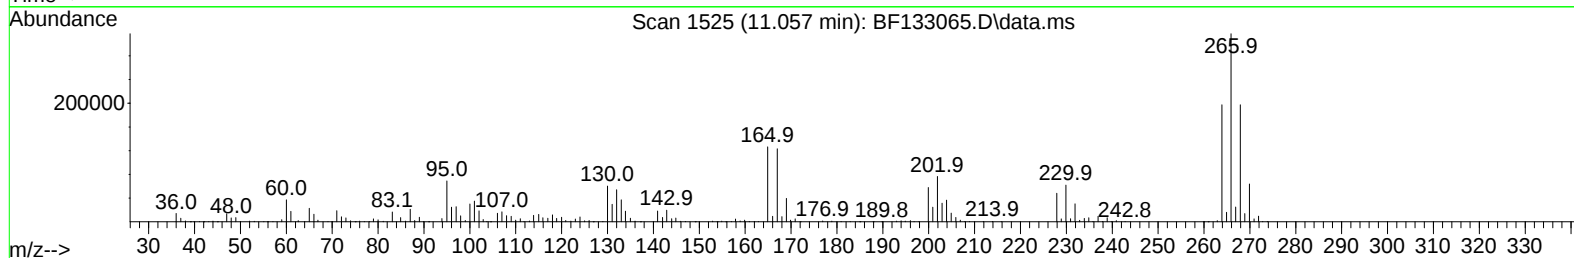


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
 Data File : BF133065.D
 Acq On : 26 Apr 2023 15:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:29:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 01:56:03 2023
 Response via : Initial Calibration

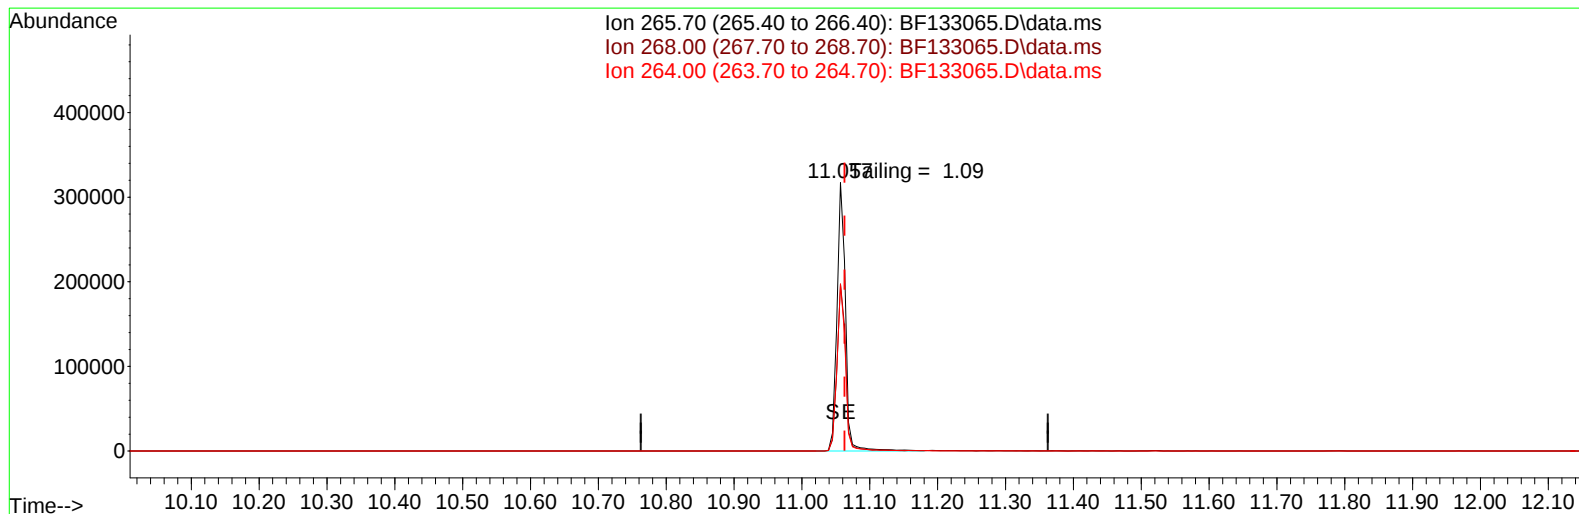

TIC: BF133065.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.006) 31605.14 ng

response 273664

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.25
264.00	63.30	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133065.D
Acq On : 26 Apr 2023 15:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:29:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:56:03 2023
Response via : Initial Calibration

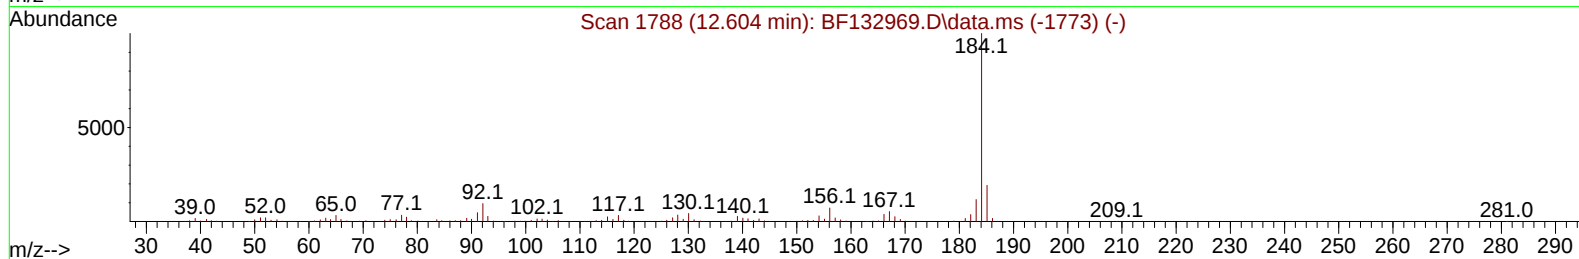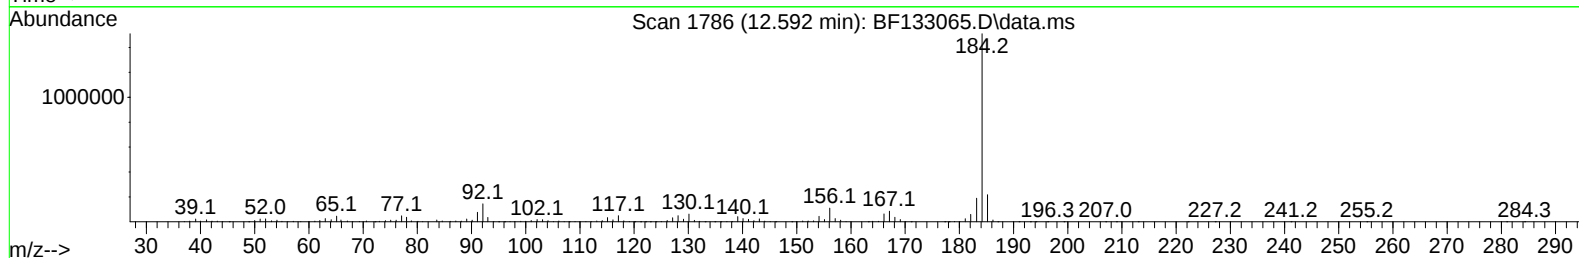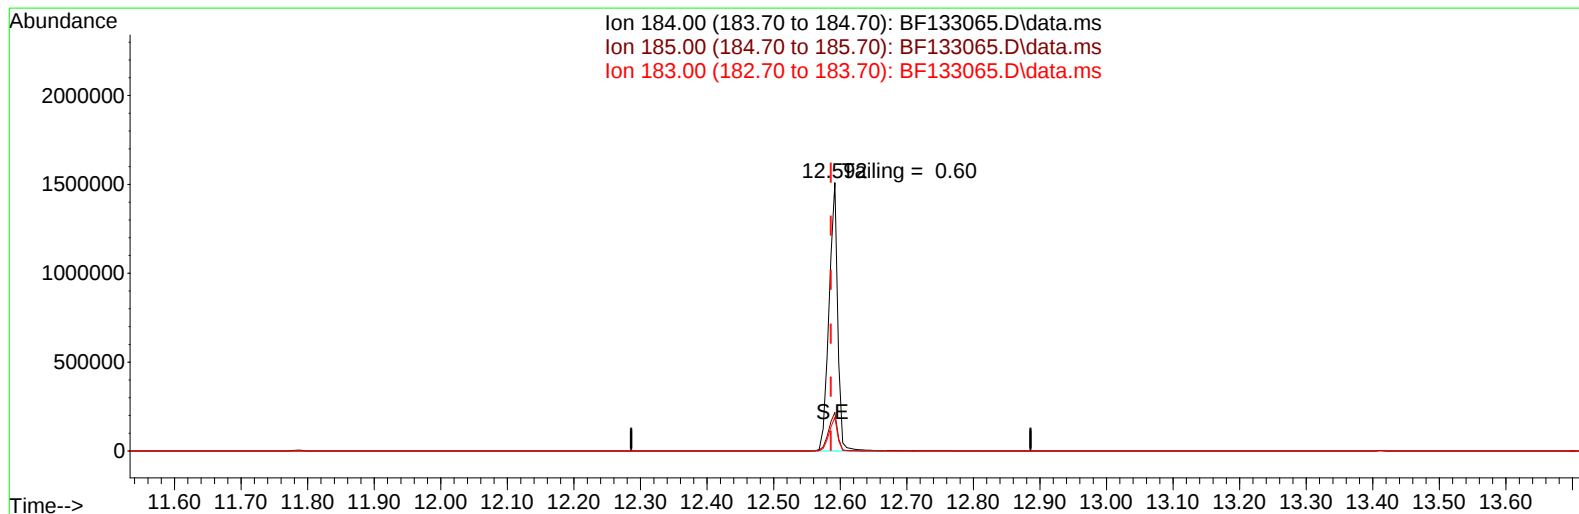

TIC: BF133065.D\data.ms

(77) Benzidine

12.592min (+ 0.006) 78724.97 ng

response 1380538

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.38#
183.00	11.70	12.55
0.00	0.00	0.00