

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
 Data File : BF133064.D
 Acq On : 26 Apr 2023 14:11
 Operator : CG\JU
 Sample : 02491-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S2S-TP4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.928	478	483	491	rVB	222504	286171	7.62%	1.019%
2	5.351	550	555	558	rBV	3574115	3386450	90.14%	12.064%
3	6.375	724	729	732	rBV	3659284	3458429	92.06%	12.320%
4	6.740	787	791	794	rBV	1325921	1135862	30.23%	4.046%
5	7.298	881	886	889	rBV	2403586	2250073	59.89%	8.016%
6	8.022	1005	1009	1012	rBV	2024362	1567545	41.72%	5.584%
7	9.098	1188	1192	1195	rVB	4578155	3717875	98.96%	13.245%
8	9.775	1303	1307	1310	rBV	2293971	1797373	47.84%	6.403%
9	10.486	1424	1428	1431	rBV	203805	169267	4.51%	0.603%
10	10.557	1436	1440	1444	rBV	2665943	2383427	63.44%	8.491%
11	11.251	1555	1558	1562	rBV	2158005	1848437	49.20%	6.585%
12	11.786	1645	1649	1653	rBV	50323	54690	1.46%	0.195%
13	12.839	1824	1828	1832	rBV	3892656	3756872	100.00%	13.384%
14	13.857	1989	2001	2002	rBV9	27880	78953	2.10%	0.281%
15	13.886	2002	2006	2010	rVB	1277327	1125812	29.97%	4.011%
16	15.310	2243	2248	2254	rBV	899054	1053357	28.04%	3.753%




Sum of corrected areas: 28070593

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133064.D
Acq On : 26 Apr 2023 14:11
Operator : CG\JU
Sample : 02491-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S2S-TP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

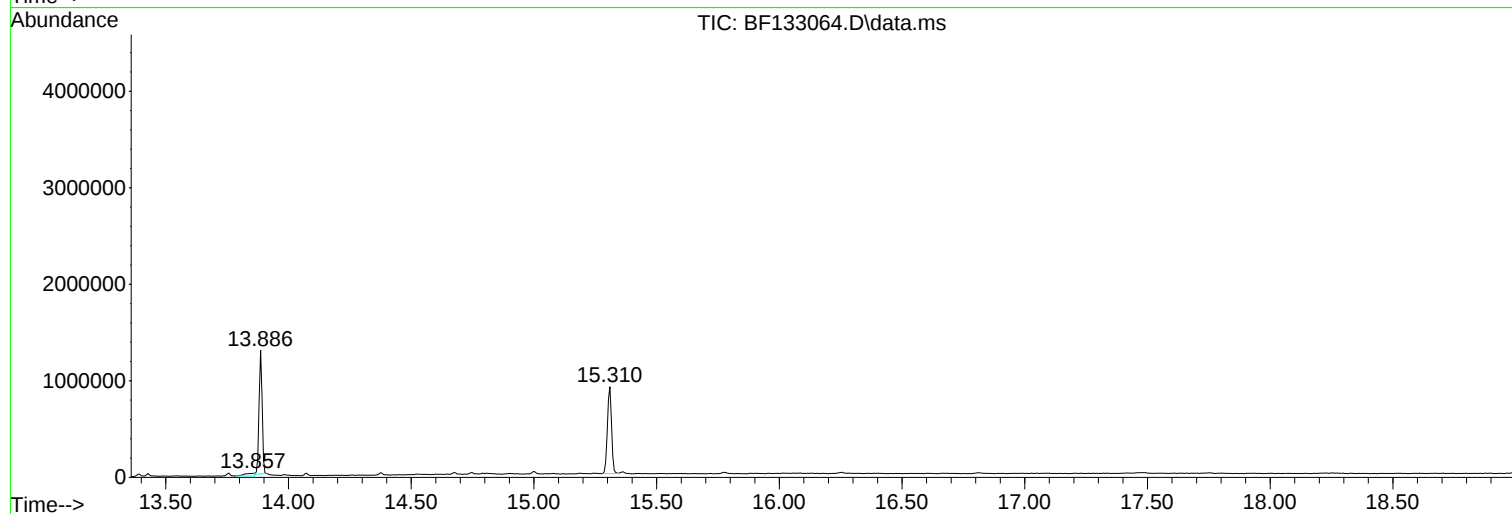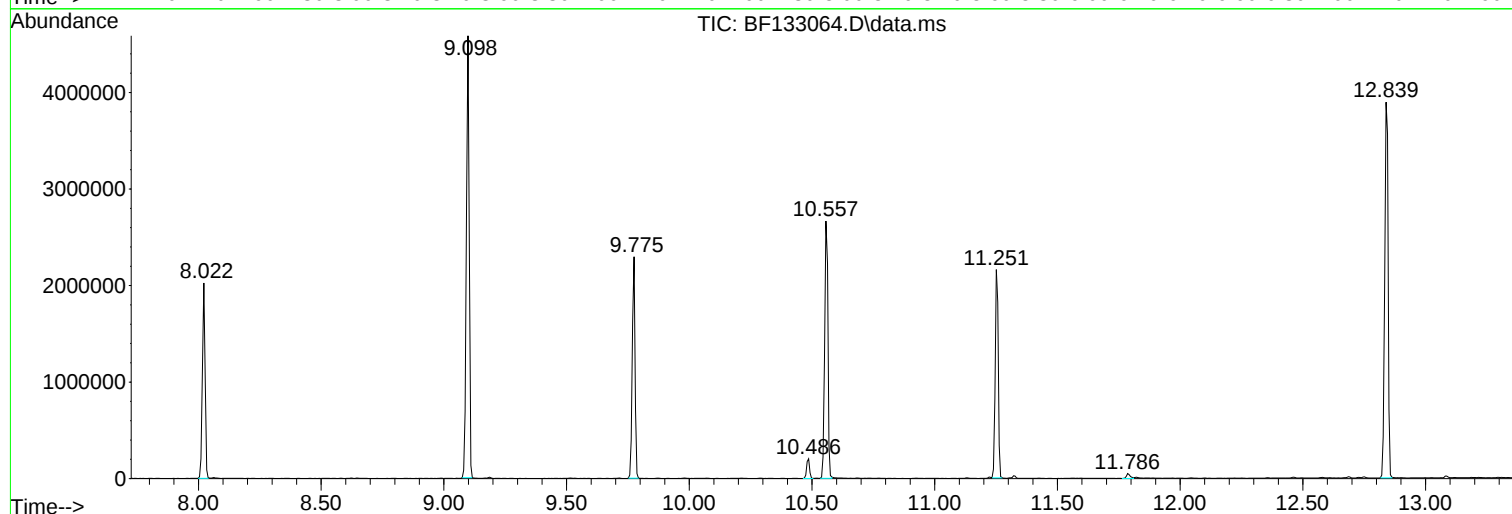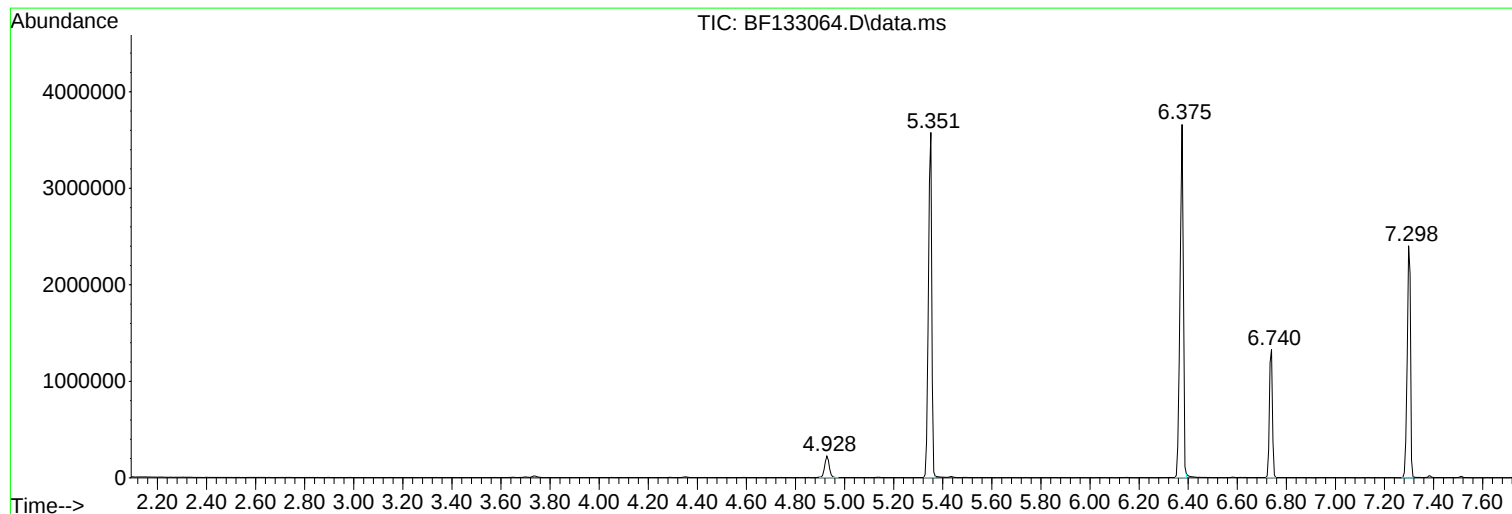

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133064.D
Acq On : 26 Apr 2023 14:11
Operator : CG\JU
Sample : 02491-03
Misc :
ALS Vial : 9 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
S2S-TP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
4.928	5.04 ng	286171	1,4-Dichlorobenzene-d4			6.740
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	59
2	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	12
3	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	9
4	4-Methoxy-1-pentene		100	C6H12O	098386-09-5	9
5	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	9

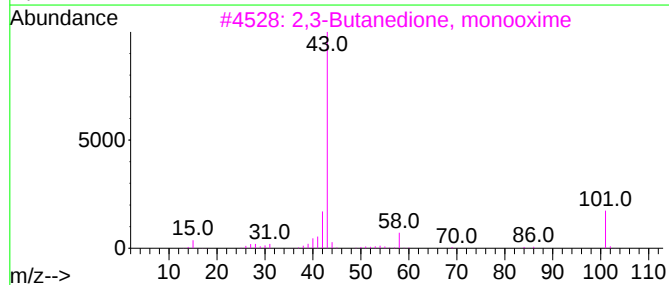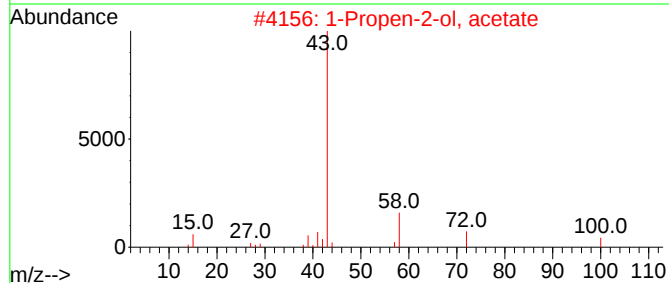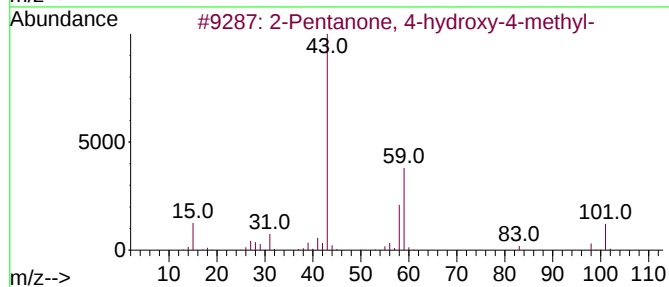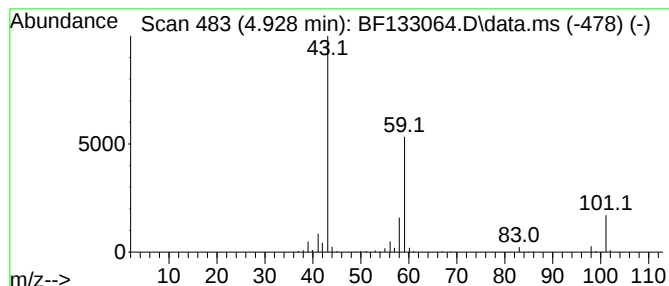

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133064.D
Acq On : 26 Apr 2023 14:11
Operator : CG\JU
Sample : 02491-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S2S-TP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.928	5.0	ng	286171	1	6.740	1135860	20.0