

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
 Data File : BF133086.D
 Acq On : 27 Apr 2023 02:07
 Operator : CG\JU
 Sample : 02423-07 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SPD-2WC-23-04-18

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.698	266	274	279	rBV	29644	40817	1.55%	0.160%
2	4.910	476	480	488	rVB	77171	79789	3.03%	0.312%
3	5.339	549	553	556	rBV	1705947	1492118	56.62%	5.834%
4	6.369	724	728	731	rBV	1952187	1604683	60.89%	6.274%
5	6.739	787	791	794	rBV	2241992	1935427	73.44%	7.567%
6	7.298	882	886	889	rBV	1182379	1010711	38.35%	3.952%
7	8.022	1005	1009	1012	rBV	3424352	2557448	97.05%	9.999%
8	9.092	1188	1191	1195	rBV	2361589	1867441	70.86%	7.301%
9	9.433	1242	1249	1251	rBV	33738	35752	1.36%	0.140%
10	9.774	1303	1307	1310	rVB	3115971	2635302	100.00%	10.304%
11	10.316	1396	1399	1406	rVB3	46428	43948	1.67%	0.172%
12	10.480	1423	1427	1431	rVB	269134	215653	8.18%	0.843%
13	10.557	1436	1440	1443	rBV	596114	540239	20.50%	2.112%
14	10.686	1458	1462	1463	rBV4	39405	44473	1.69%	0.174%
15	11.163	1539	1543	1546	rVB2	30017	44554	1.69%	0.174%
16	11.257	1555	1559	1561	rBV	2534536	2335914	88.64%	9.133%
17	11.274	1561	1562	1566	rVV	497499	317954	12.07%	1.243%
18	11.321	1566	1570	1574	rVB2	144232	162485	6.17%	0.635%
19	11.751	1641	1643	1646	rBV	58665	56706	2.15%	0.222%
20	11.786	1646	1649	1653	rVV2	118315	132256	5.02%	0.517%
21	11.827	1653	1656	1658	rVV3	46405	52116	1.98%	0.204%
22	11.863	1659	1662	1665	rVV	128607	139547	5.30%	0.546%
23	11.886	1665	1666	1669	rVB	56690	36613	1.39%	0.143%
24	12.051	1691	1694	1695	rBV	54678	45649	1.73%	0.178%
25	12.068	1695	1697	1701	rVB2	46247	42656	1.62%	0.167%
26	12.304	1734	1737	1740	rBV2	69878	70327	2.67%	0.275%
27	12.386	1748	1751	1755	rBV2	43956	45954	1.74%	0.180%
28	12.463	1761	1764	1768	rBV	1014557	832438	31.59%	3.255%
29	12.692	1797	1803	1806	rBV	869866	882103	33.47%	3.449%
30	12.810	1821	1823	1824	rBV	46455	34208	1.30%	0.134%
31	12.839	1824	1828	1831	rVV	1670165	1421103	53.93%	5.556%
32	13.021	1856	1859	1861	rVB	113007	104872	3.98%	0.410%
33	13.086	1867	1870	1872	rBV2	95072	78133	2.96%	0.305%
34	13.121	1873	1876	1879	rBV2	102575	115435	4.38%	0.451%
35	13.886	2002	2006	2009	rBV2	1935840	2224849	84.42%	8.699%
36	13.915	2009	2011	2013	rVB	341806	273862	10.39%	1.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133086.D
Acq On : 27 Apr 2023 02:07
Operator : CG\JU
Sample : 02423-07 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPD-2WC-23-04-18

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.904	2176	2179	2186	rBV	242529	457736	17.37%	1.790%
38	15.251	2235	2238	2241	rBV	193479	223672	8.49%	0.875%
39	15.315	2244	2249	2253	rBV	1129298	1341486	50.90%	5.245%




Sum of corrected areas: 25576429

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133086.D
Acq On : 27 Apr 2023 02:07
Operator : CG\JU
Sample : 02423-07 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPD-2WC-23-04-18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

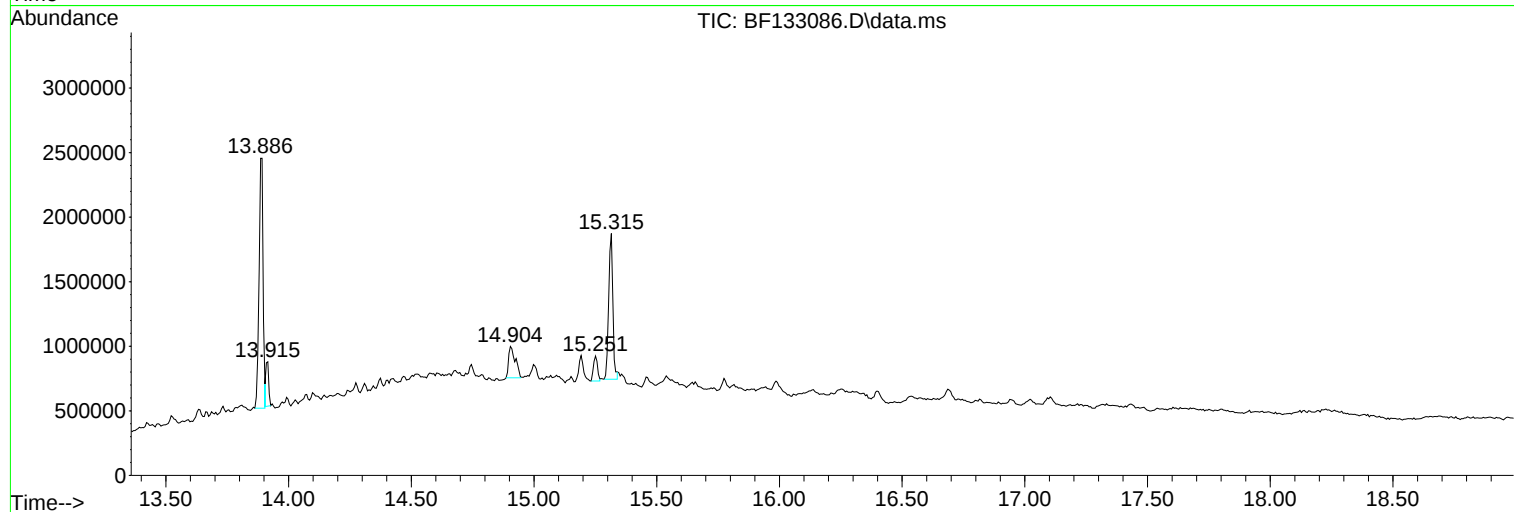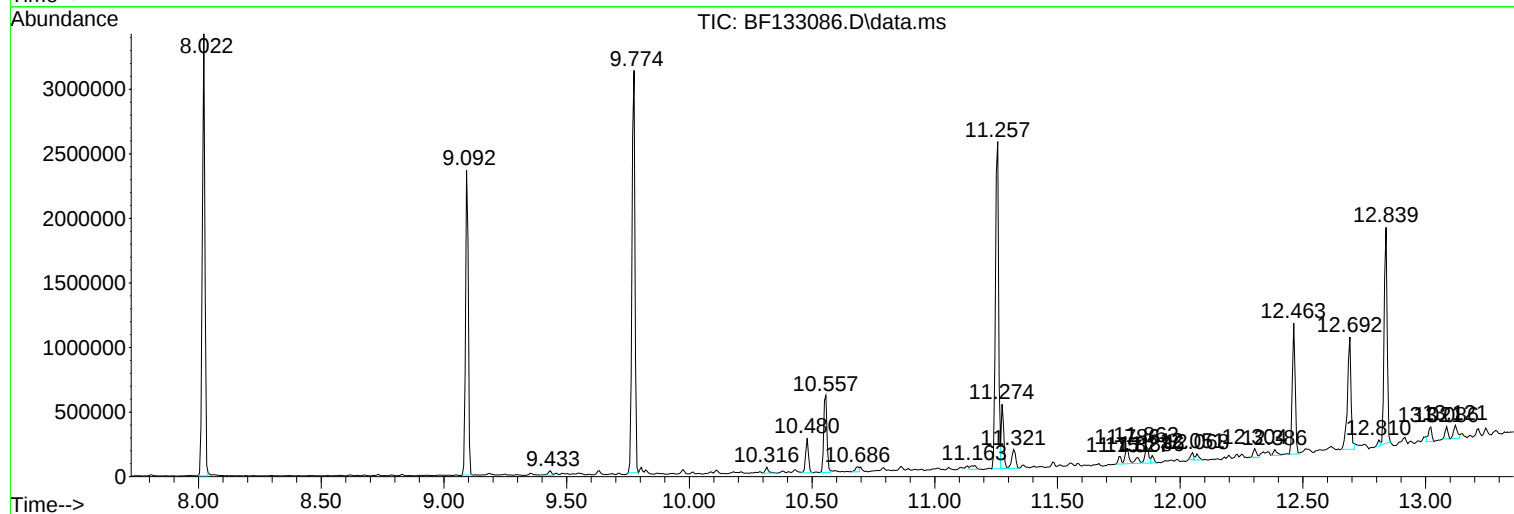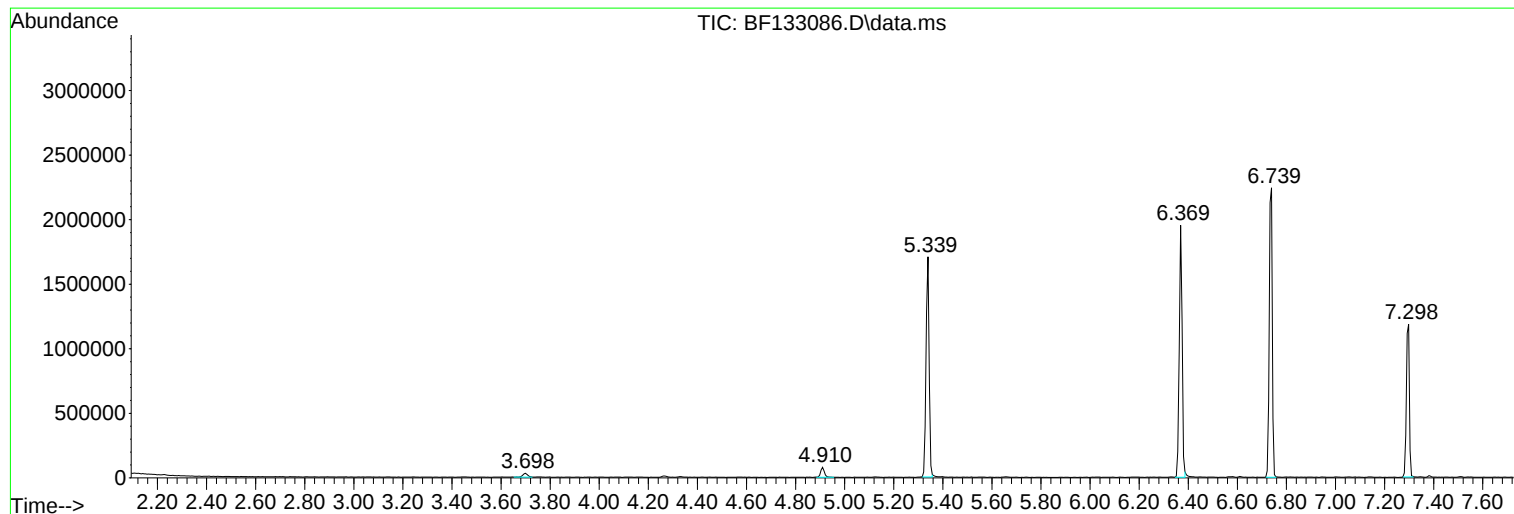

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133086.D
Acq On : 27 Apr 2023 02:07
Operator : CG\JU
Sample : 02423-07 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPD-2WC-23-04-18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133086.D
Acq On : 27 Apr 2023 02:07
Operator : CG\JU
Sample : 02423-07 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPD-2WC-23-04-18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------