

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
 Data File : BF133088.D
 Acq On : 27 Apr 2023 03:10
 Operator : CG\JU
 Sample : 02423-03 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SPD-1WC-23-04-18

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	268	273	281	rVB2	27780	42685	1.66%	0.197%
2	4.910	477	480	487	rVB	48985	50998	1.99%	0.235%
3	5.340	549	553	562	rBV	1576193	1363305	53.09%	6.276%
4	6.375	725	729	740	rBV	1625100	1429170	55.65%	6.580%
5	6.740	787	791	794	rBV	2384016	1947632	75.84%	8.967%
6	7.298	882	886	889	rBV	983644	831137	32.36%	3.826%
7	8.022	1005	1009	1012	rBV	3308375	2568141	100.00%	11.823%
8	9.092	1188	1191	1195	rBV	1863697	1562016	60.82%	7.191%
9	9.775	1303	1307	1310	rBV	3209976	2485887	96.80%	11.445%
10	10.481	1424	1427	1431	rVB	165238	133528	5.20%	0.615%
11	10.557	1436	1440	1444	rBV	736525	593826	23.12%	2.734%
12	10.686	1459	1462	1467	rVB5	24689	35559	1.38%	0.164%
13	11.257	1555	1559	1561	rBV	2663415	2205384	85.87%	10.153%
14	11.275	1561	1562	1566	rVV	235349	175452	6.83%	0.808%
15	11.328	1566	1571	1574	rVB	59101	67788	2.64%	0.312%
16	11.757	1641	1644	1646	rBV	33529	32466	1.26%	0.149%
17	11.786	1646	1649	1653	rVB	118027	115571	4.50%	0.532%
18	11.869	1659	1663	1665	rBV	68045	78475	3.06%	0.361%
19	12.051	1691	1694	1696	rBV	45411	43950	1.71%	0.202%
20	12.304	1735	1737	1740	rBV	44264	38625	1.50%	0.178%
21	12.463	1761	1764	1767	rBV	584143	489948	19.08%	2.256%
22	12.692	1798	1803	1806	rBV	532586	493996	19.24%	2.274%
23	12.839	1825	1828	1831	rBV	1614032	1285363	50.05%	5.918%
24	13.022	1857	1859	1863	rVB	78782	64057	2.49%	0.295%
25	13.892	2002	2007	2009	rBV	2170429	2081385	81.05%	9.582%
26	13.916	2009	2011	2013	rVB	217083	159615	6.22%	0.735%
27	15.316	2245	2249	2253	rBV	1168664	1344855	52.37%	6.192%




Sum of corrected areas: 21720814

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133088.D
Acq On : 27 Apr 2023 03:10
Operator : CG\JU
Sample : 02423-03 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPD-1WC-23-04-18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

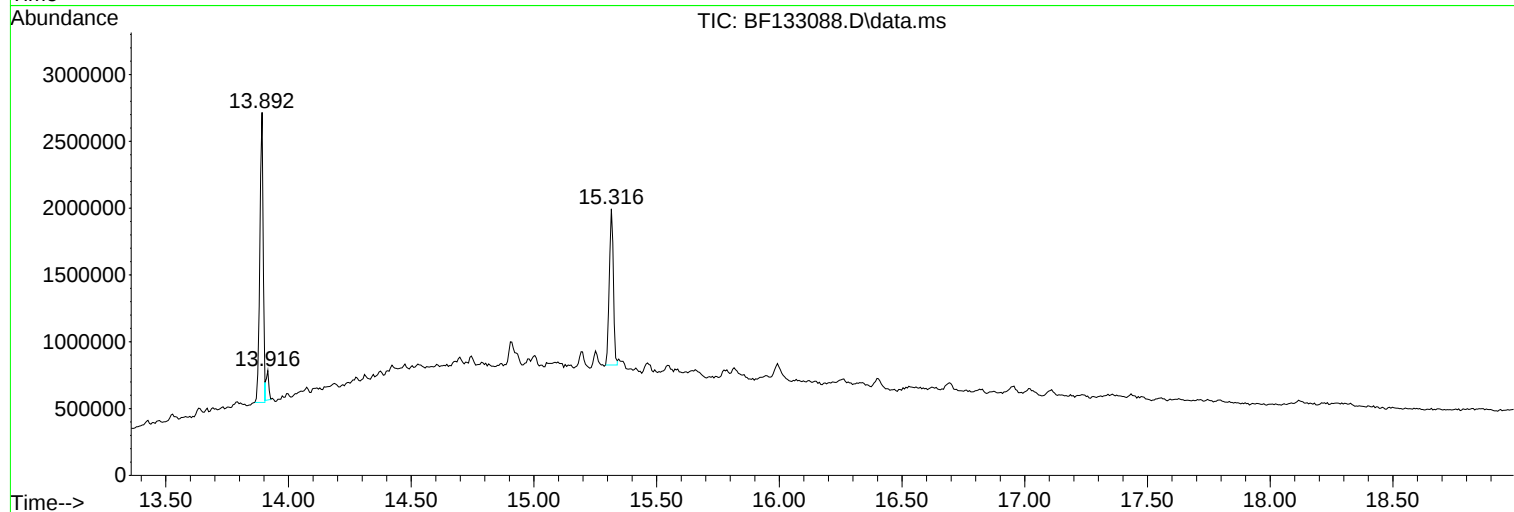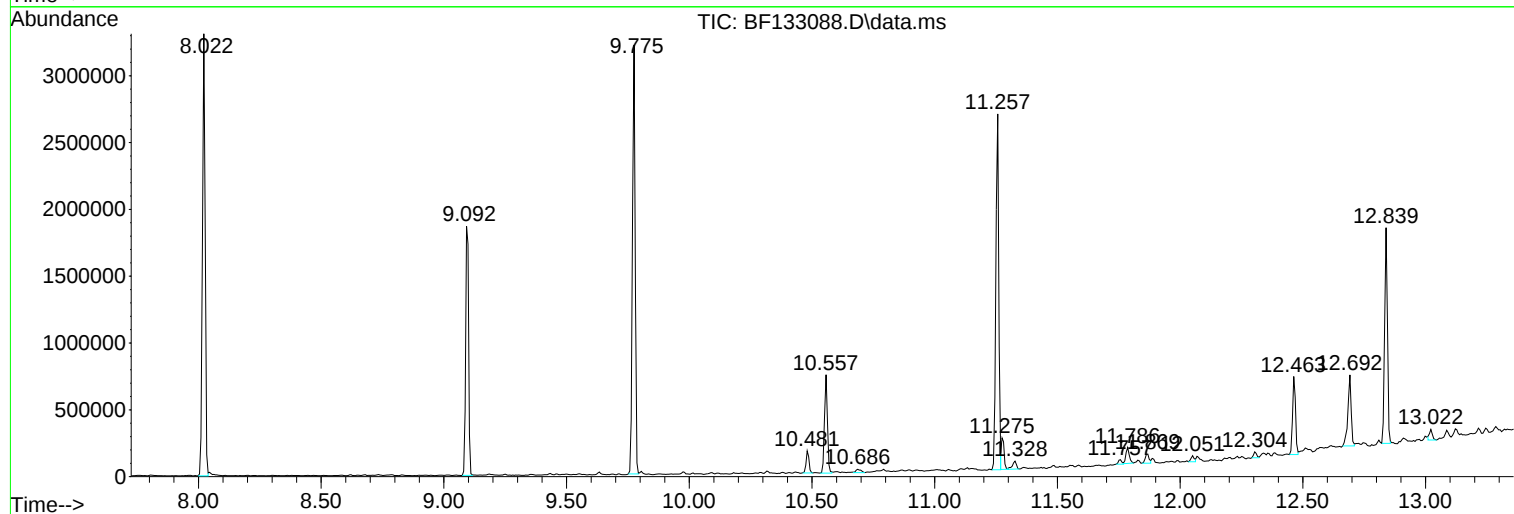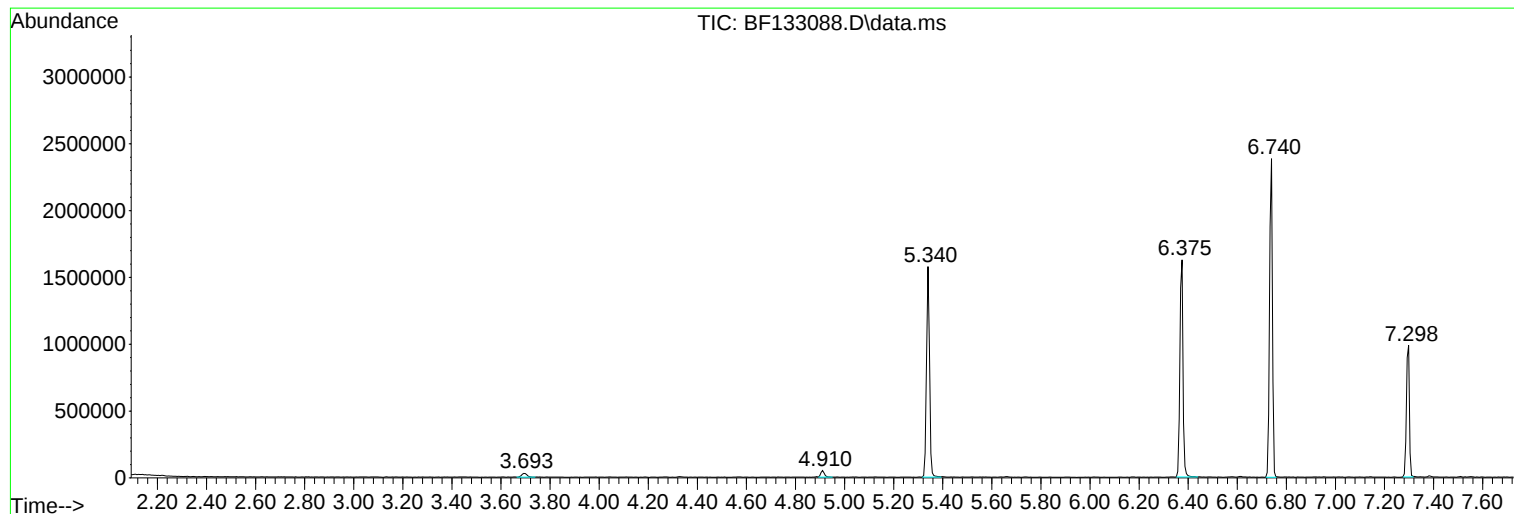

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133088.D
Acq On : 27 Apr 2023 03:10
Operator : CG\JU
Sample : 02423-03 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPD-1WC-23-04-18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133088.D
Acq On : 27 Apr 2023 03:10
Operator : CG\JU
Sample : 02423-03 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPD-1WC-23-04-18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------