
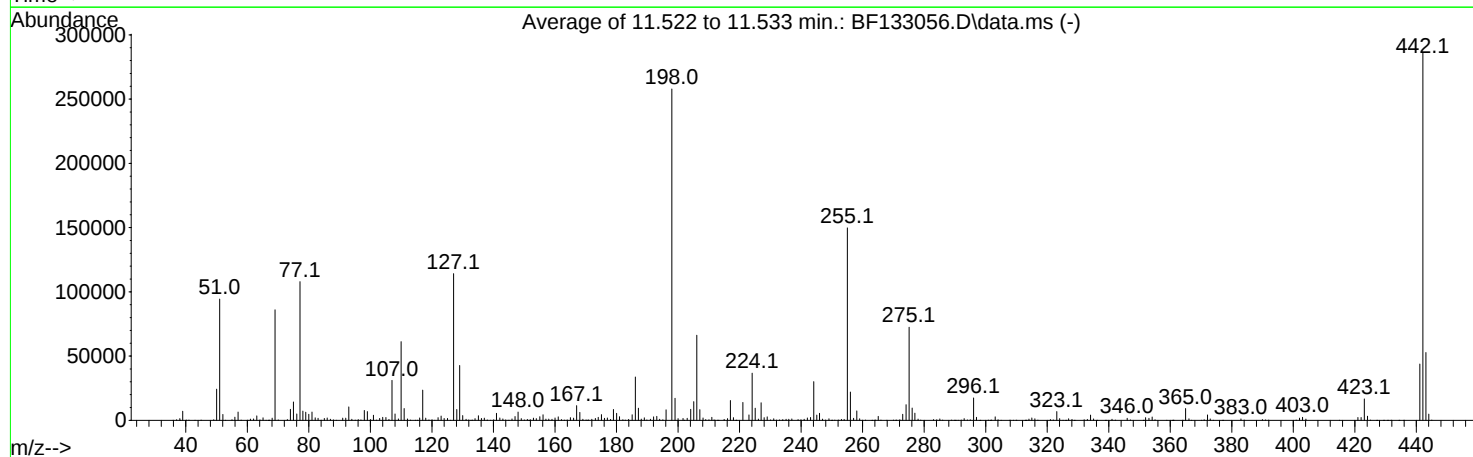


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133056.D
Acq On : 26 Apr 2023 10:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 27 01:56:03 2023

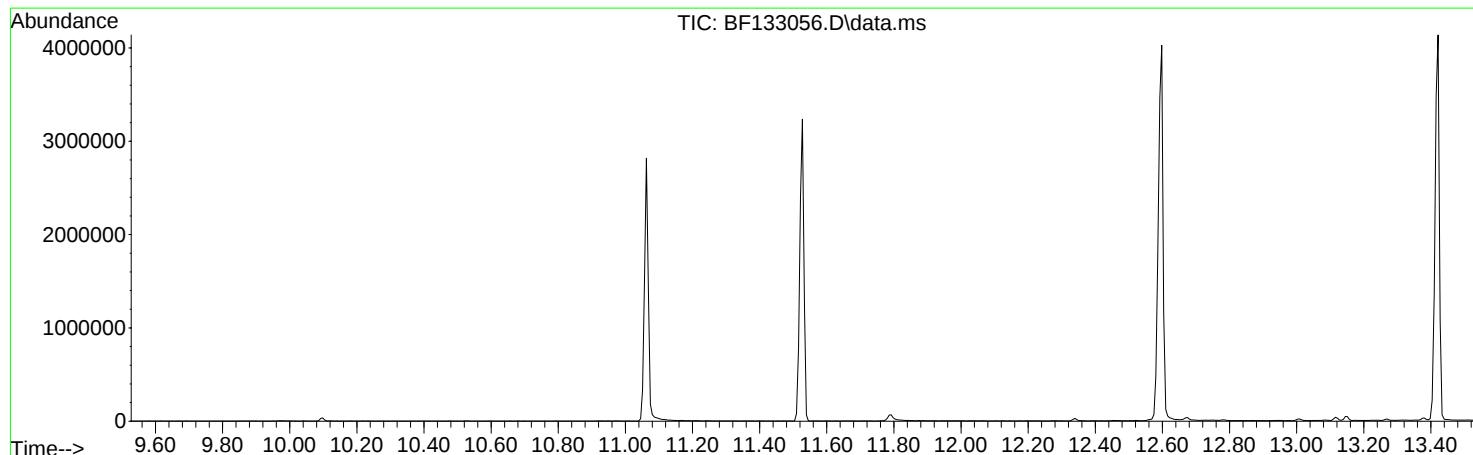

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	94359	PASS
68	69	0.00	2	2.0	1696	PASS
69	198	0.00	100	33.4	86075	PASS
70	69	0.00	2	0.5	416	PASS
127	198	10	80	44.3	114173	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	257861	PASS
199	198	5	9	6.7	17208	PASS
275	198	10	60	28.1	72437	PASS
365	198	1	100	3.6	9216	PASS
441	198	0.01	100	17.0	43891	PASS
442	442	50	100	100.0	286272	PASS
443	442	15	24	18.4	52776	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/26/2023	BNA_F	<u>BF133056.D</u>
Compound Name	Response	Retention Time
DDT	735465	13.421
DDD	12841	13.151
DDE	1187	12.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14028	749493	1.87

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133056.D
Acq On : 26 Apr 2023 10:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:24:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:56:03 2023
Response via : Initial Calibration

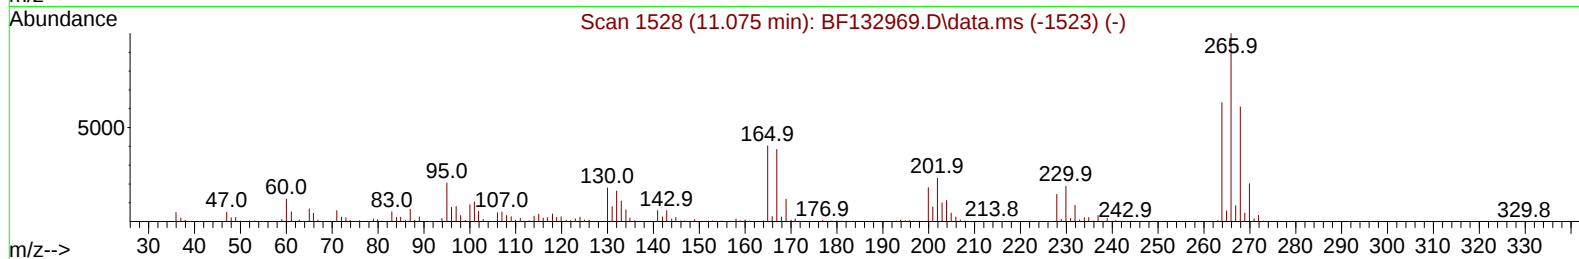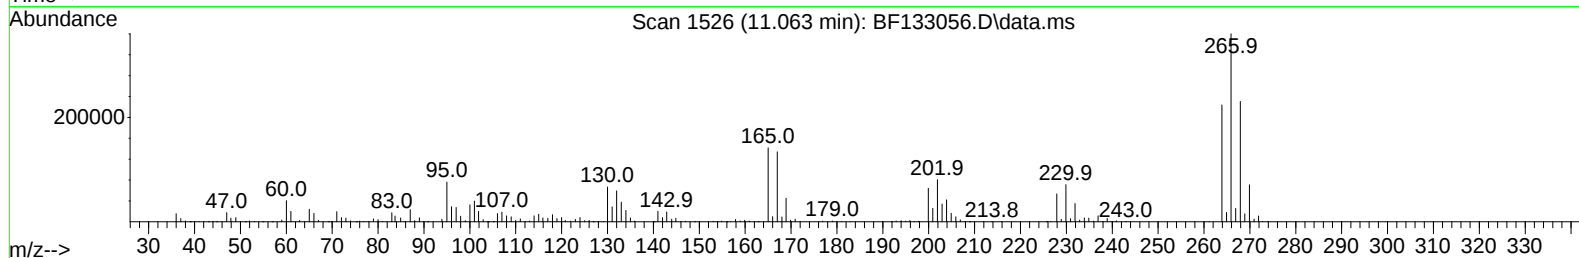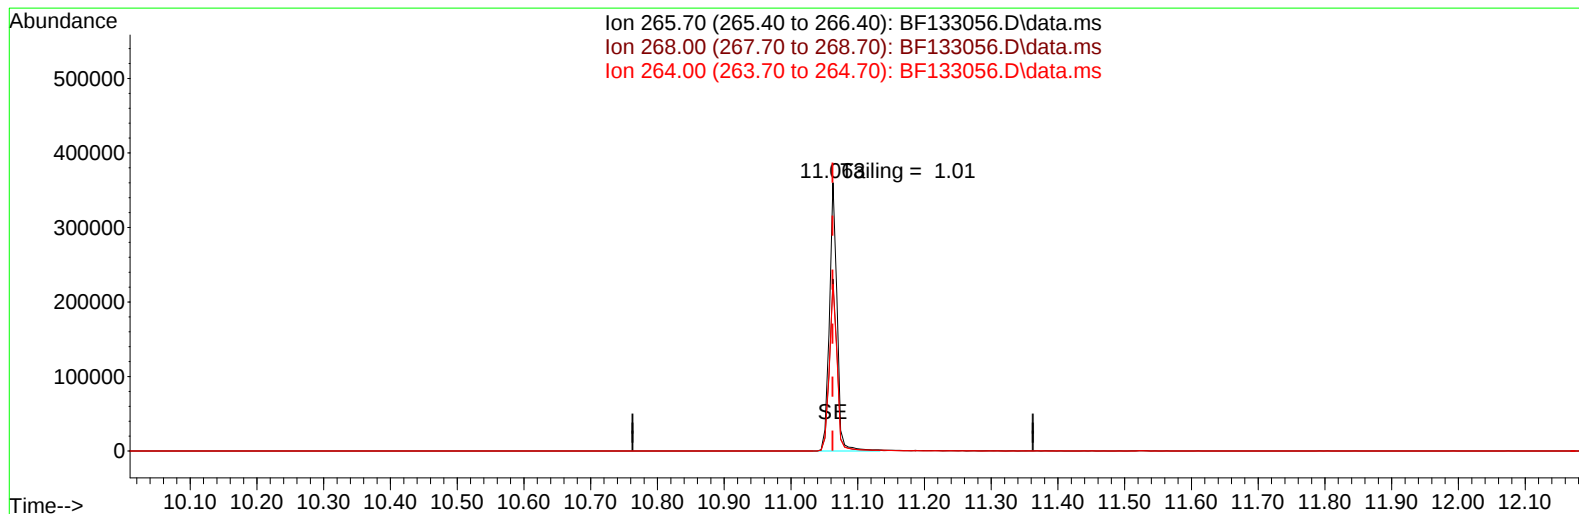

TIC: BF133056.D\data.ms

(70) Pentachlorophenol (C)

11.063min (+ 0.000) 32077.95 ng




response 291722

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.05
264.00	63.30	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133056.D
Acq On : 26 Apr 2023 10:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:24:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:56:03 2023
Response via : Initial Calibration

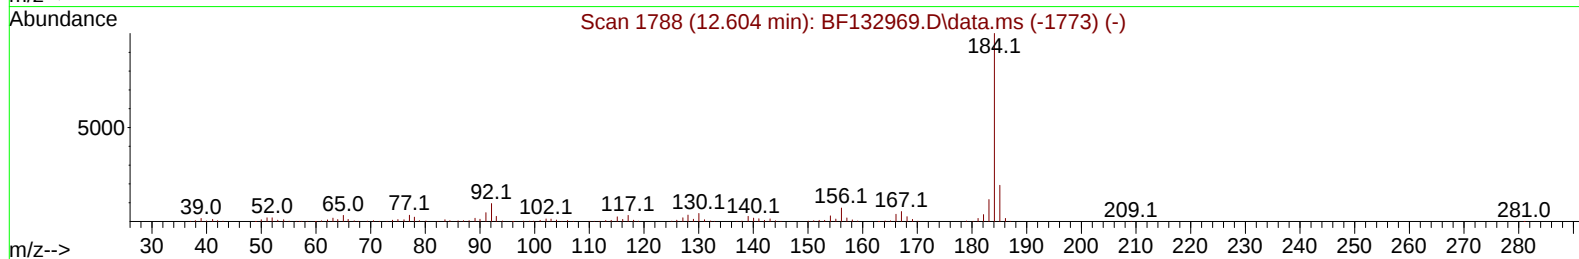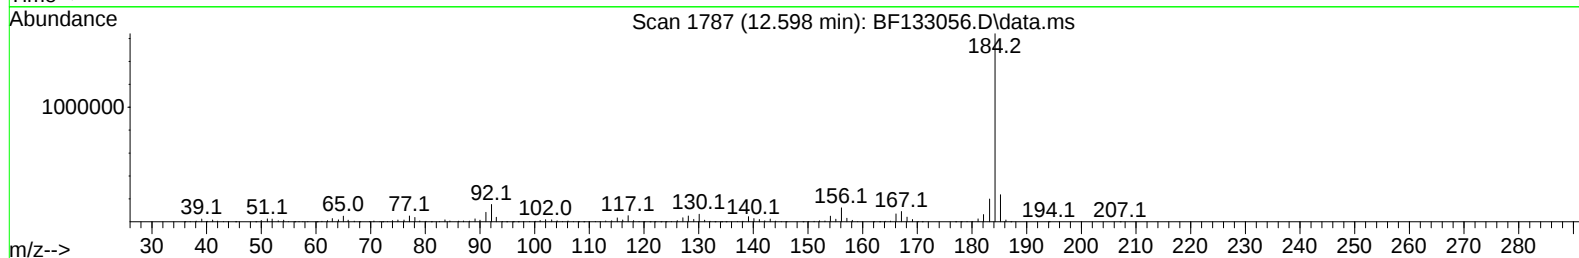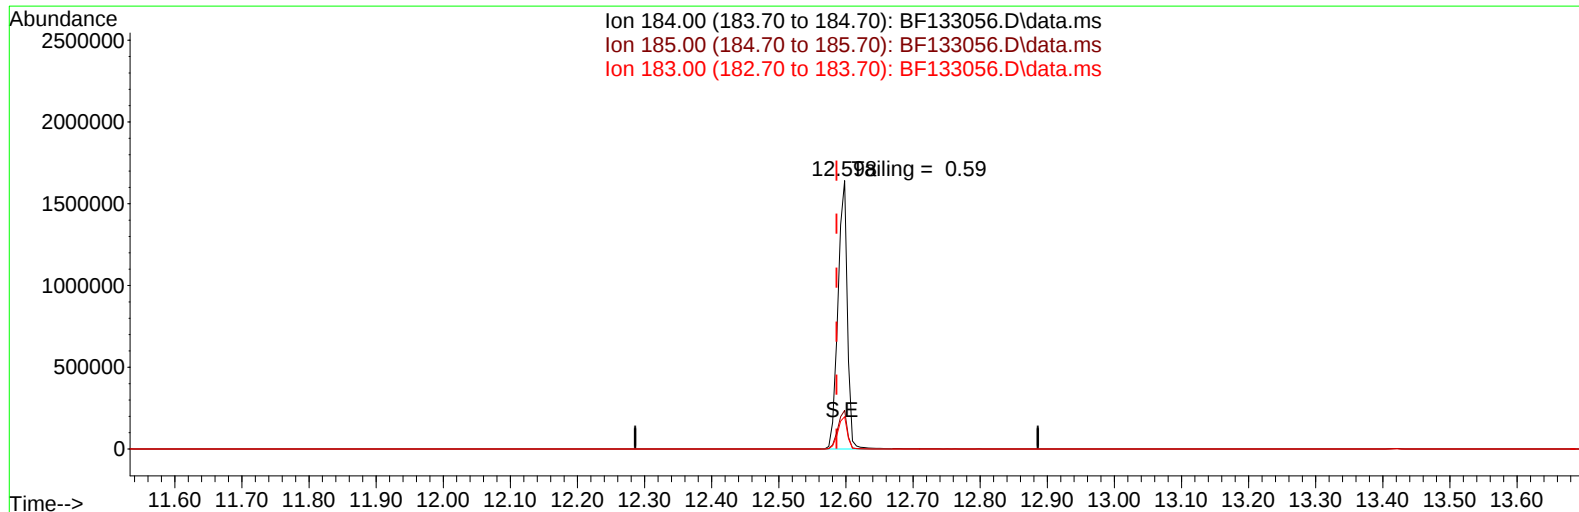

TIC: BF133056.D\data.ms

(77) Benzidine

12.598min (+ 0.012) 1715984.49 ng

response 1596001

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.39#
183.00	11.70	12.07
0.00	0.00	0.00