


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133065.D
Acq On : 26 Apr 2023 15:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 27 01:56:03 2023

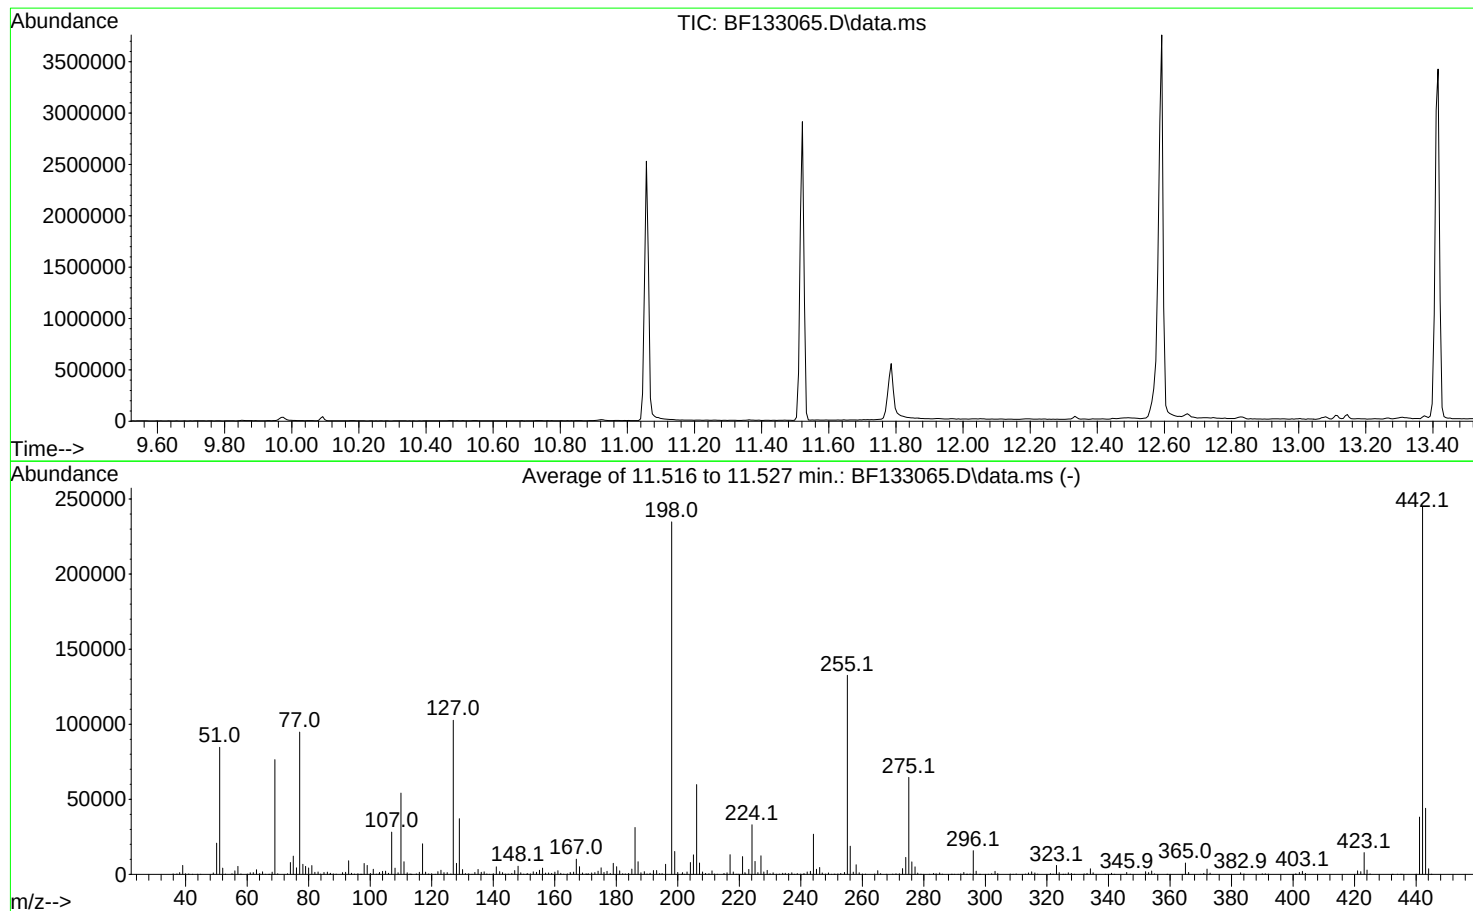

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	84645	PASS
68	69	0.00	2	1.9	1472	PASS
69	198	0.00	100	32.6	76435	PASS
70	69	0.00	2	0.6	435	PASS
127	198	10	80	43.7	102592	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	234800	PASS
199	198	5	9	6.5	15247	PASS
275	198	10	60	27.5	64555	PASS
365	198	1	100	3.2	7598	PASS
441	198	0.01	100	16.3	38163	PASS
442	442	50	100	100.0	245013	PASS
443	442	15	24	18.0	44016	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/26/2023	BNA_F	<u>BF133065.D</u>
Compound Name	Response	Retention Time
DDT	609708	13.415
DDD	12538	13.145
DDE	314	12.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12852	622560	2.06

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133065.D
Acq On : 26 Apr 2023 15:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:29:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:56:03 2023
Response via : Initial Calibration

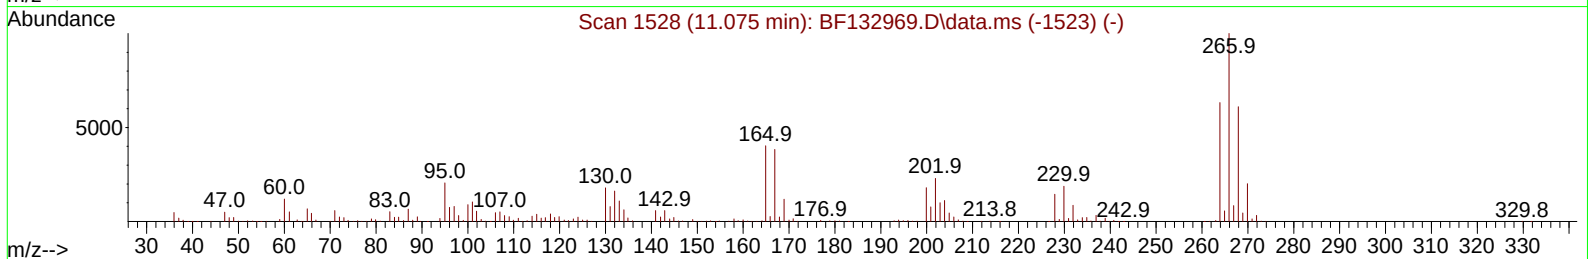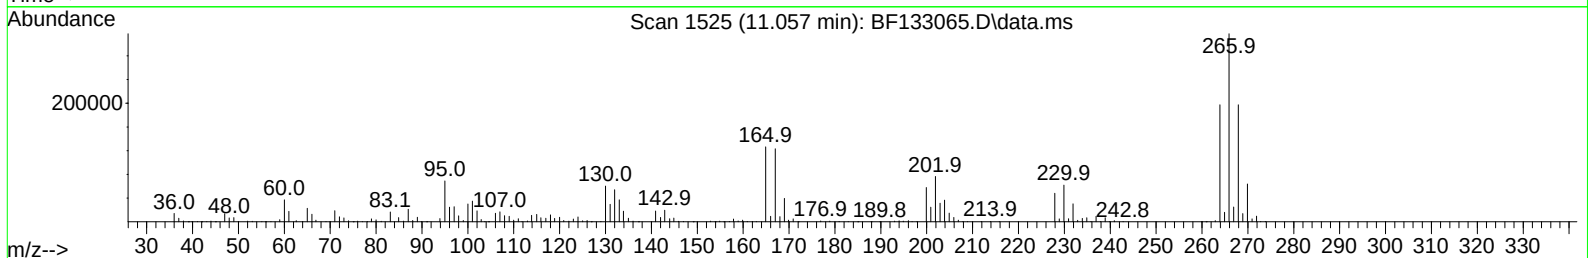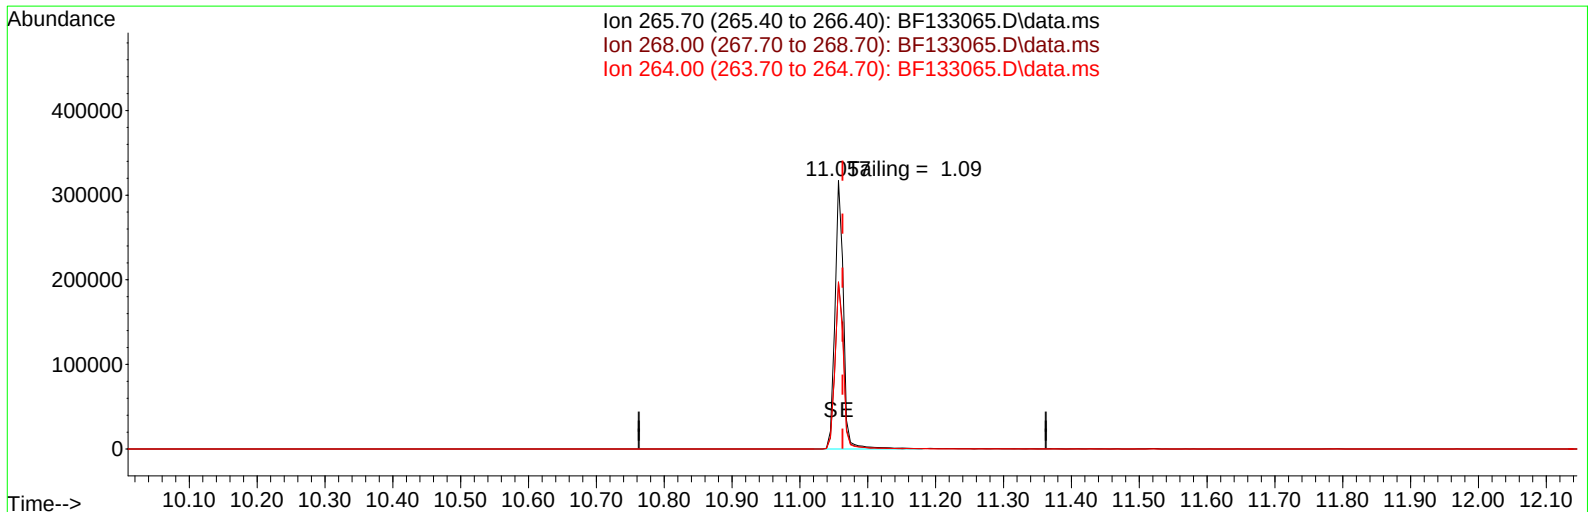

TIC: BF133065.D\data.ms

(70) Pentachlorophenol (C)

11.057min (-0.006) 31605.14 ng




response 273664

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.25
264.00	63.30	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042623\
Data File : BF133065.D
Acq On : 26 Apr 2023 15:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:29:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:56:03 2023
Response via : Initial Calibration

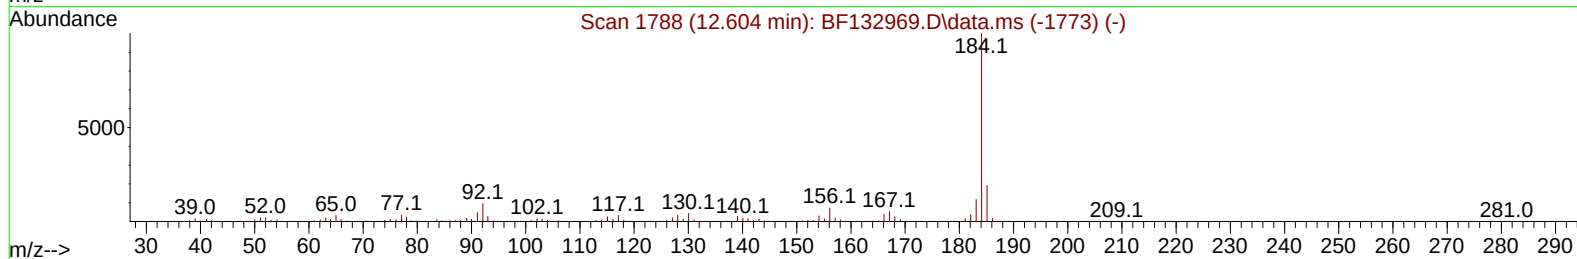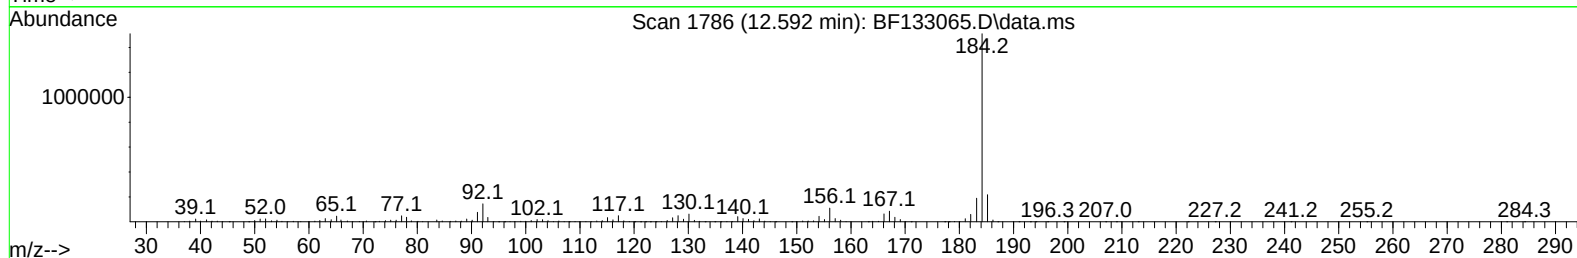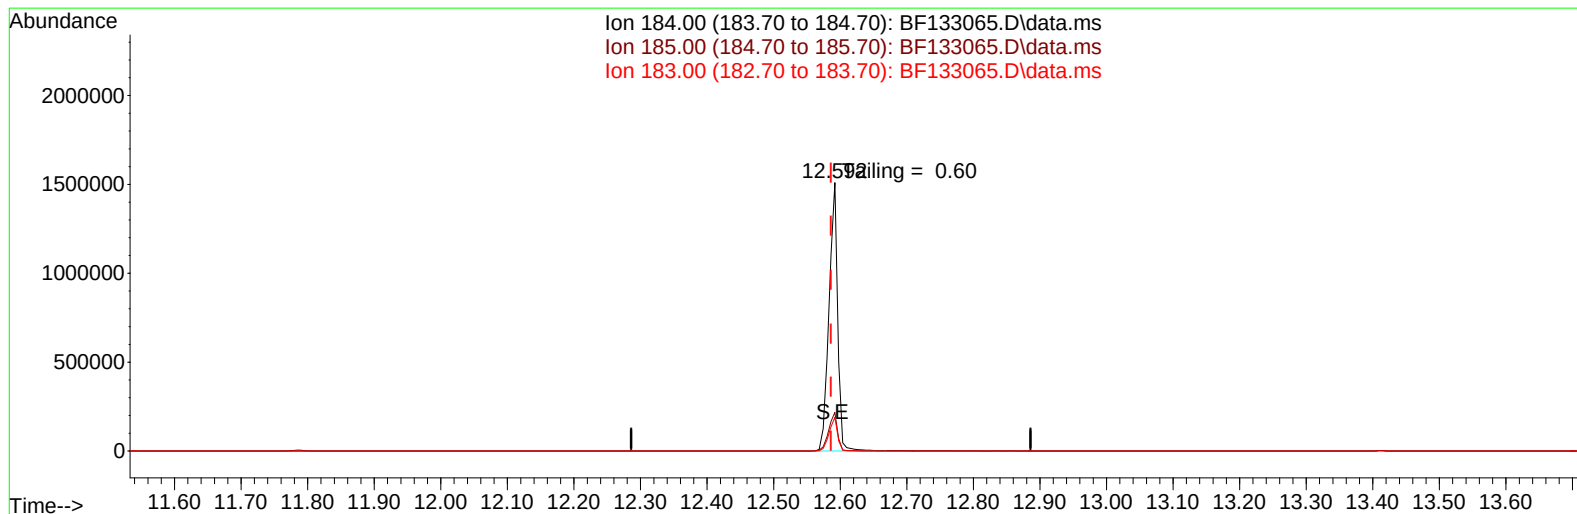

TIC: BF133065.D\data.ms

(77) Benzidine

12.592min (+ 0.006) 78724.97 ng

response 1380538

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.38#
183.00	11.70	12.55
0.00	0.00	0.00