
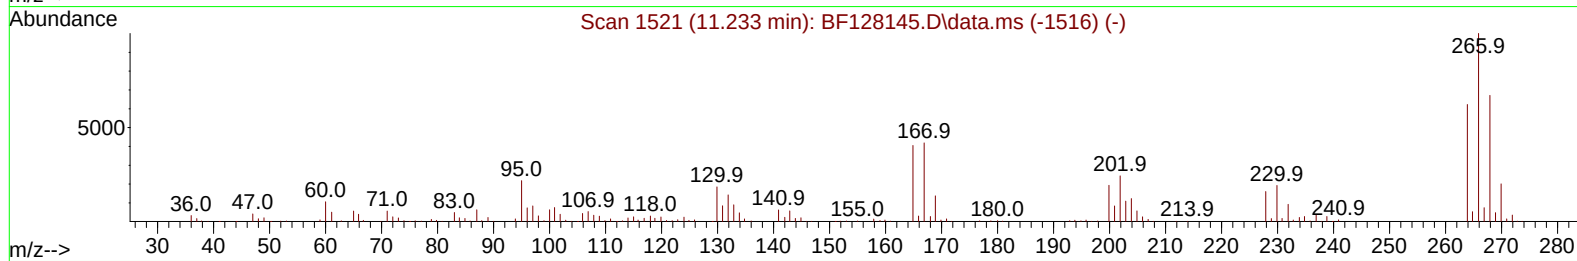
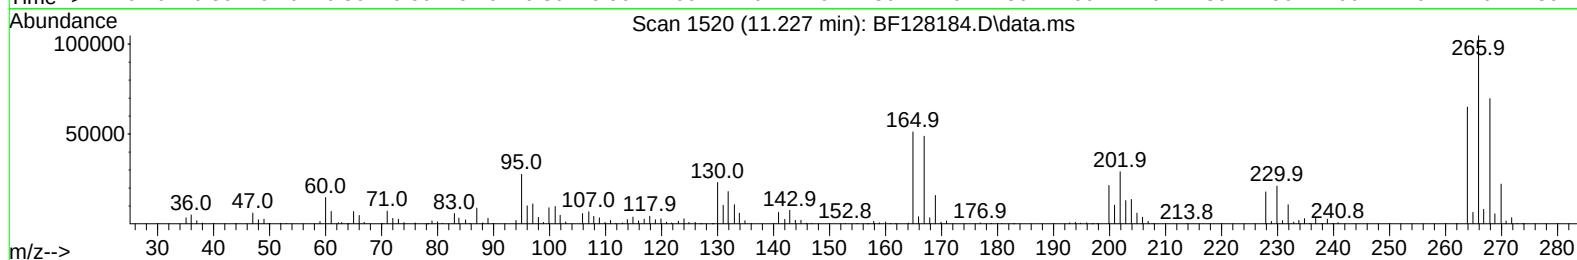


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
 Data File : BF128184.D
 Acq On : 11 May 2022 09:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 09:42:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 09 15:30:11 2022
 Response via : Initial Calibration

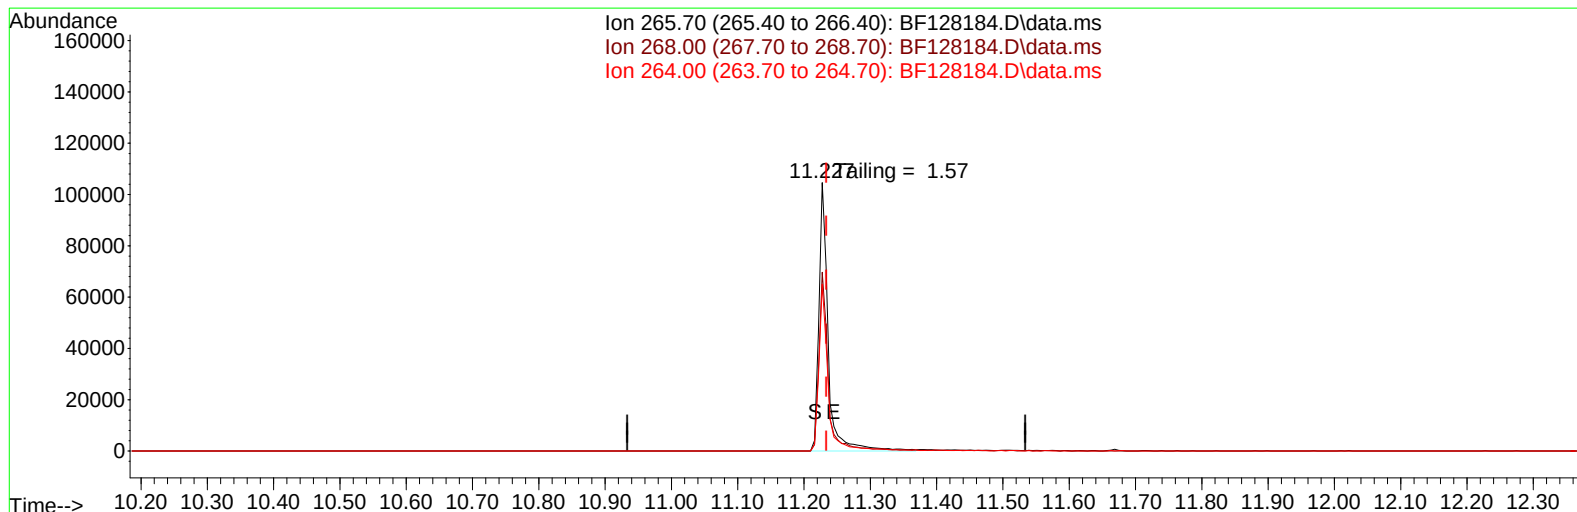

TIC: BF128184.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.006) 300514.24 ng

response 102986

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.59
264.00	66.40	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128184.D
Acq On : 11 May 2022 09:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 09:42:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 15:30:11 2022
Response via : Initial Calibration

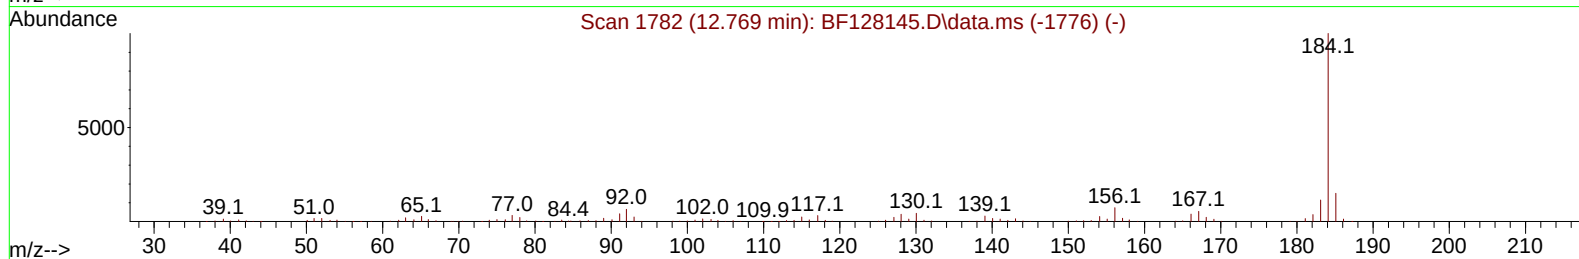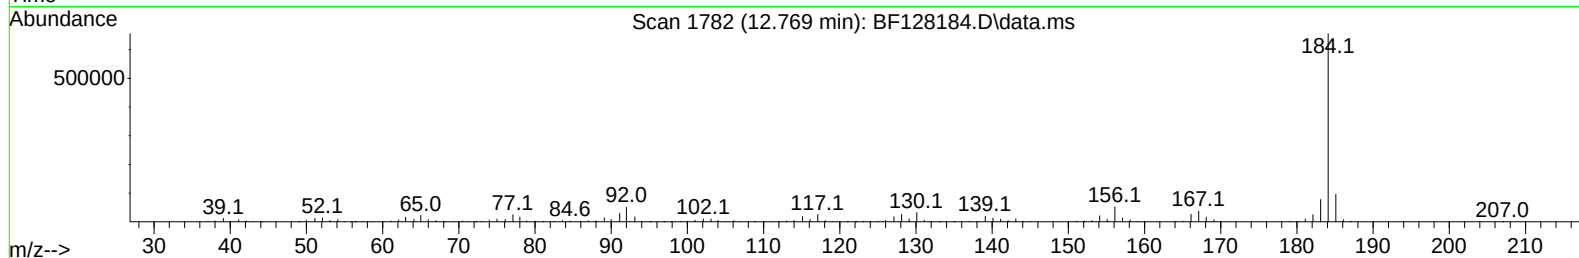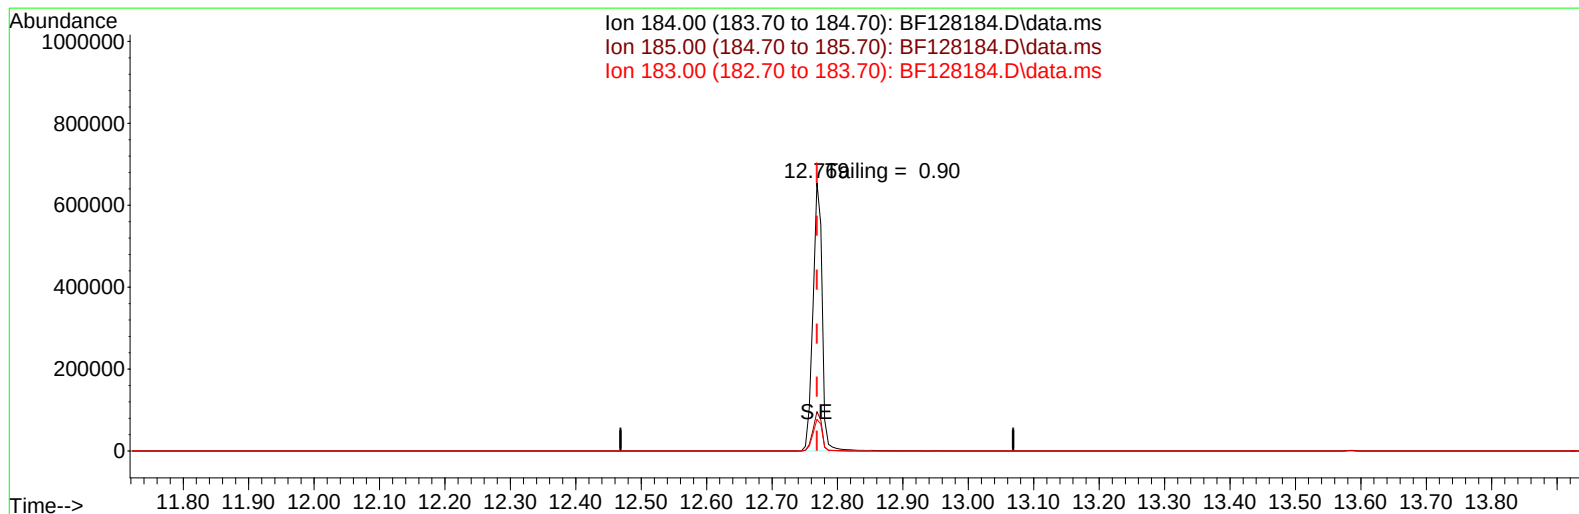

TIC: BF128184.D\data.ms

(77) Benzidine

12.769min (-0.000) 217070.12 ng

response 644088

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.68
183.00	11.20	11.83
0.00	0.00	0.00