

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
 Data File : BF128188.D
 Acq On : 11 May 2022 11:33
 Operator : CG\JU
 Sample : PB144653TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144653TB

Quant Time: May 12 05:59:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 09 15:30:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.892	152	95012	20.000	ng	0.00
21) Naphthalene-d8	8.175	136	377058	20.000	ng	0.00
39) Acenaphthene-d10	9.933	164	218531	20.000	ng	0.00
64) Phenanthrene-d10	11.421	188	407794	20.000	ng	0.00
76) Chrysene-d12	14.068	240	323097	20.000	ng	-0.01
86) Perylene-d12	15.568	264	265282	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.534	112	756837	126.984	ng	0.02
7) Phenol-d6	6.528	99	993459	126.023	ng	0.00
23) Nitrobenzene-d5	7.457	82	724036	86.404	ng	0.00
42) 2,4,6-Tribromophenol	10.727	330	312658	124.750	ng	0.00
45) 2-Fluorobiphenyl	9.251	172	1205916	86.344	ng	0.00
79) Terphenyl-d14	13.015	244	1489558	86.507	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128188.D
Acq On : 11 May 2022 11:33
Operator : CG\JU
Sample : PB144653TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144653TB

Quant Time: May 12 05:59:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 15:30:11 2022
Response via : Initial Calibration




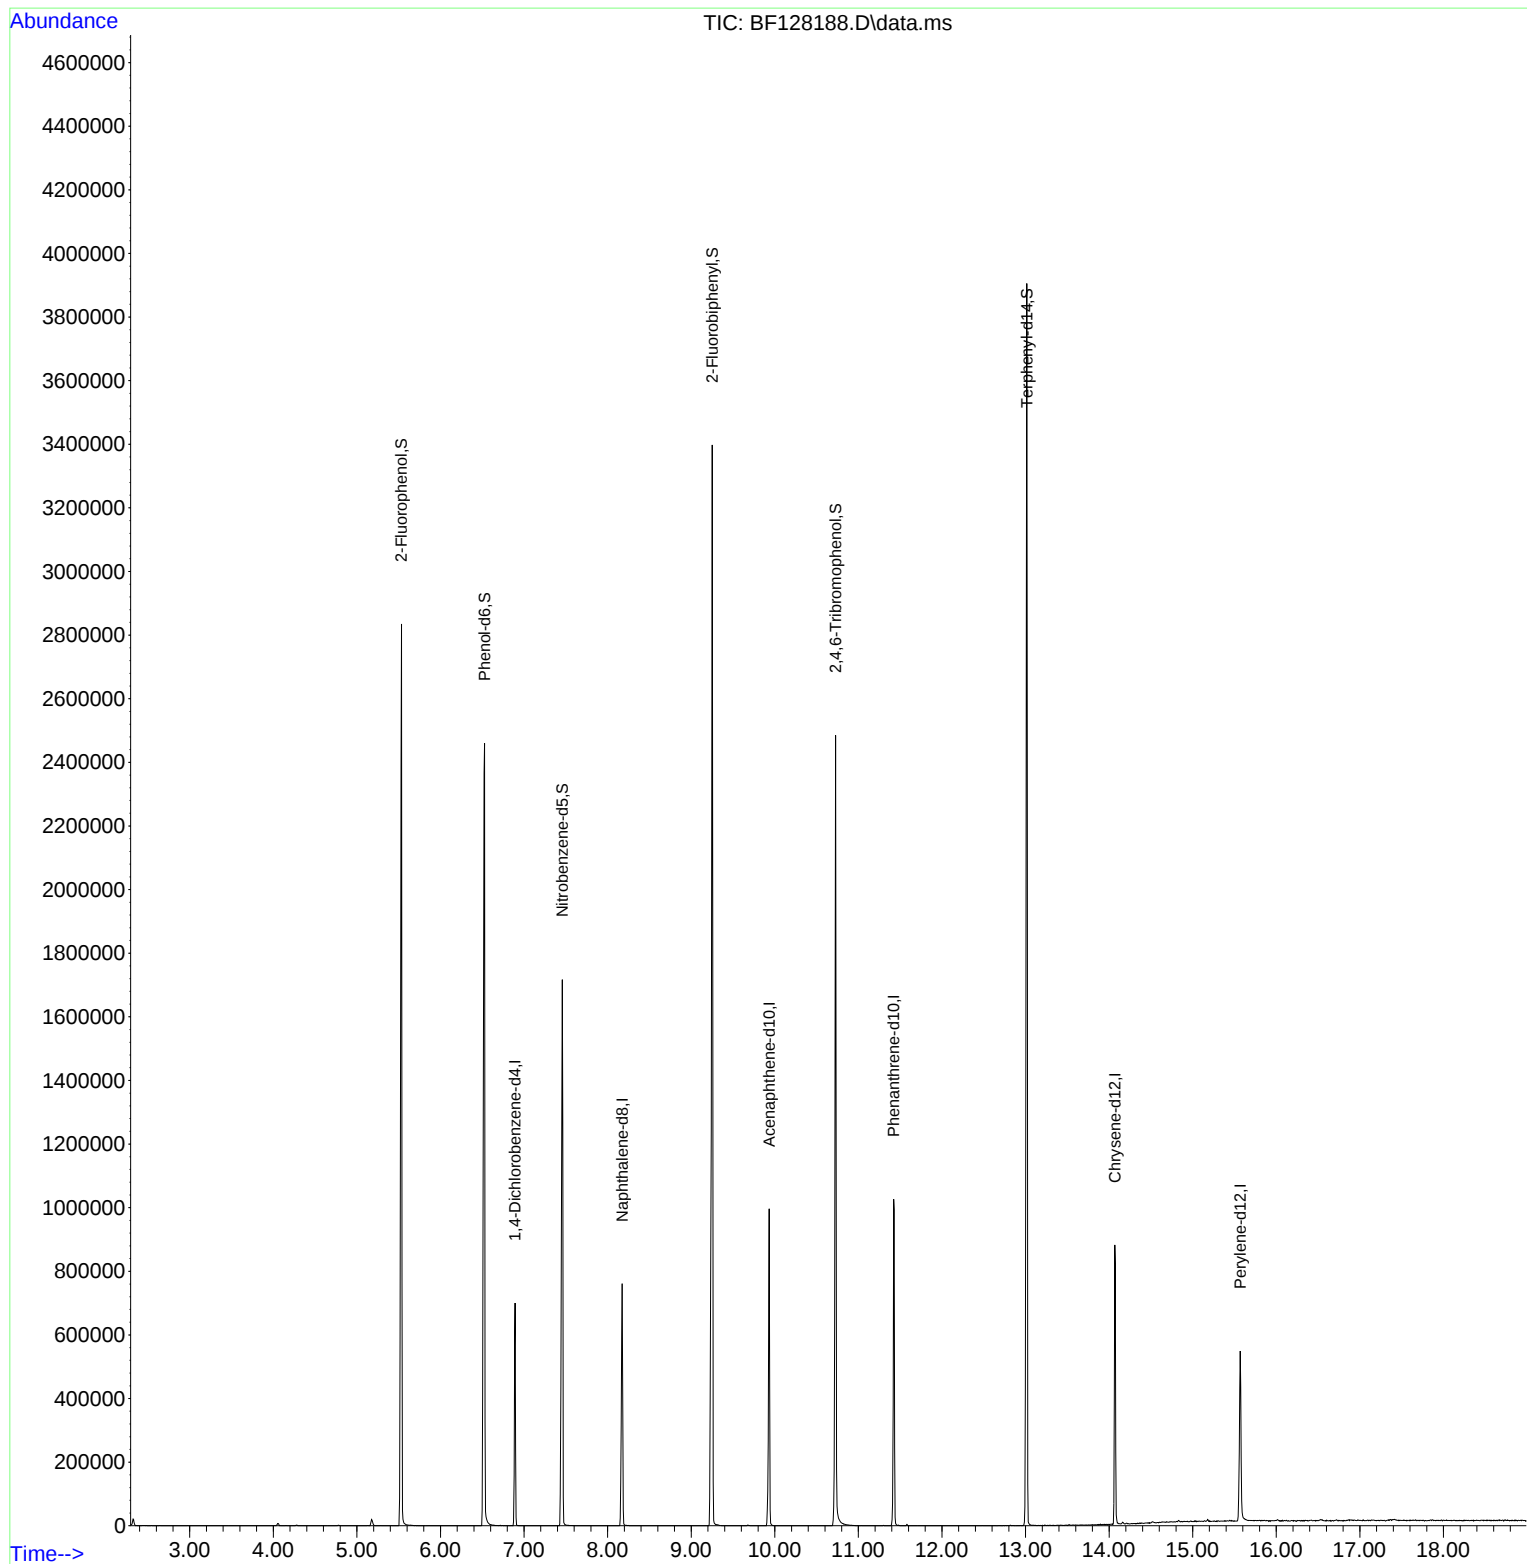




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.892 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33




Instrument :
BNA_F
ClientSampleId :
PB144653TB


Tgt Ion:152 Resp: 95012
Ion Ratio Lower Upper
152 100
150 155.7 125.3 187.9
115 66.0 48.8 73.2

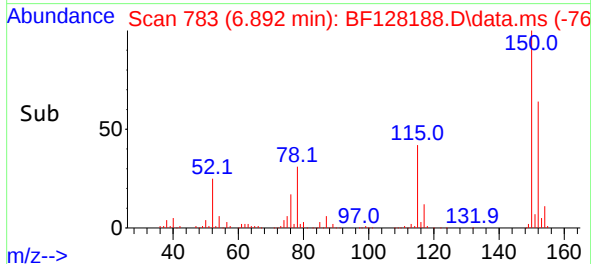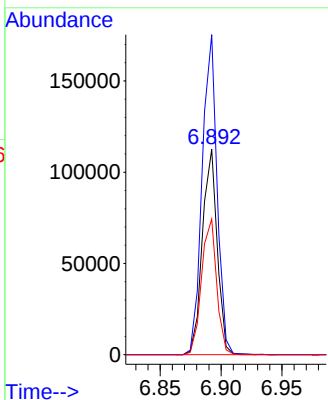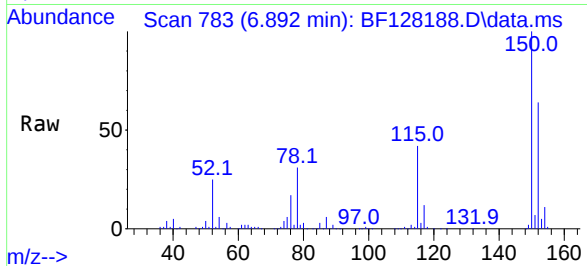

#5
2-Fluorophenol
Concen: 126.984 ng
RT: 5.534 min Scan# 552
Delta R.T. 0.017 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33

Tgt Ion:112 Resp: 756837
Ion Ratio Lower Upper
112 100
64 65.2 49.5 74.3
63 36.3 26.3 39.5

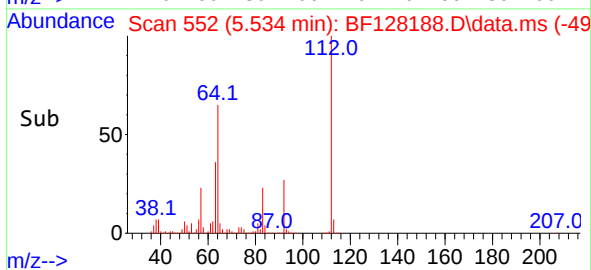
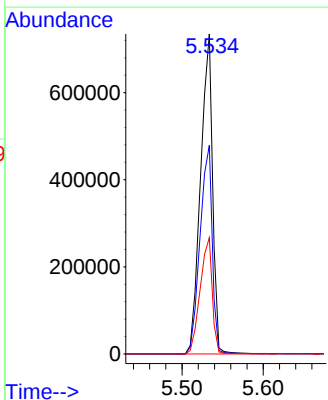
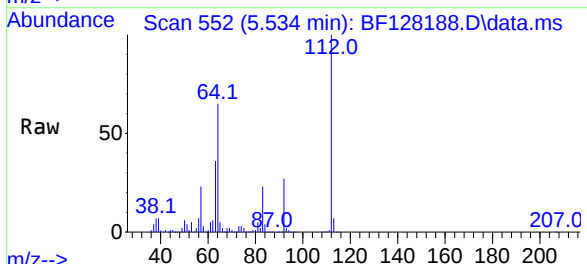




#7
Phenol-d6
Concen: 126.023 ng
RT: 6.528 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33




Instrument :
BNA_F
ClientSampleId :
PB144653TB


Tgt Ion: 99 Resp: 993459
Ion Ratio Lower Upper
99 100
42 20.8 16.6 24.8
71 40.4 30.0 45.0

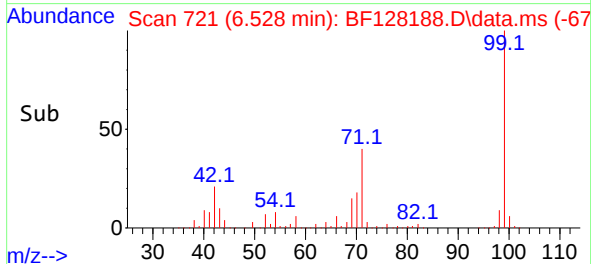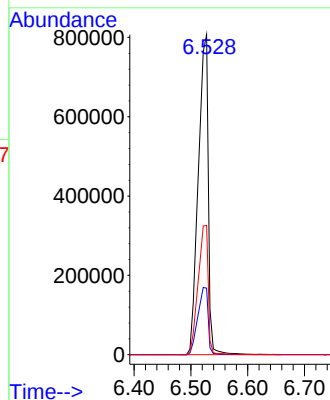

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.175 min Scan# 1001
Delta R.T. -0.006 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33

Tgt Ion: 136 Resp: 377058
Ion Ratio Lower Upper
136 100
137 10.6 8.6 13.0
54 7.9 6.8 10.2
68 5.6 5.1 7.7


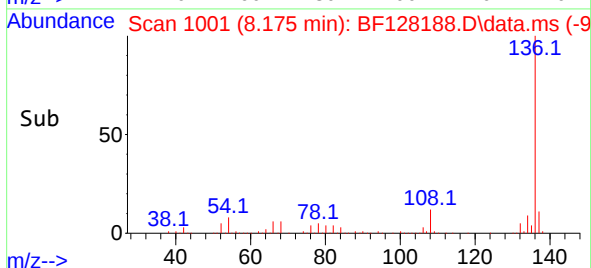
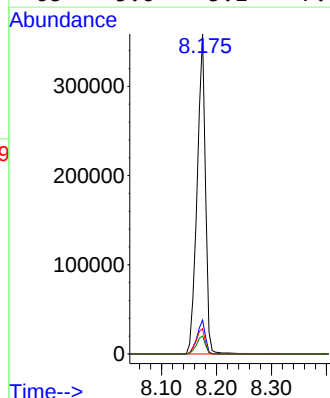
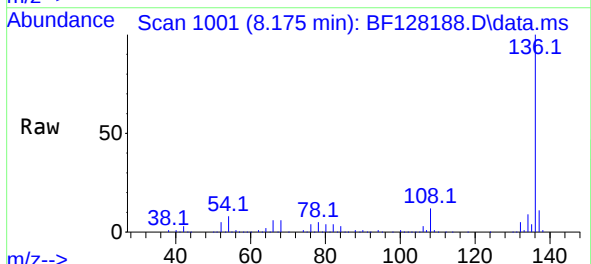




#23
Nitrobenzene-d5
Concen: 86.404 ng
RT: 7.457 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33




Instrument :
BNA_F
ClientSampleId :
PB144653TB


Tgt Ion: 82 Resp: 724036
Ion Ratio Lower Upper
82 100
128 35.7 30.0 45.0
54 51.8 41.3 61.9

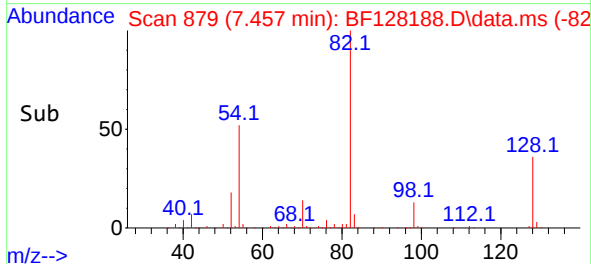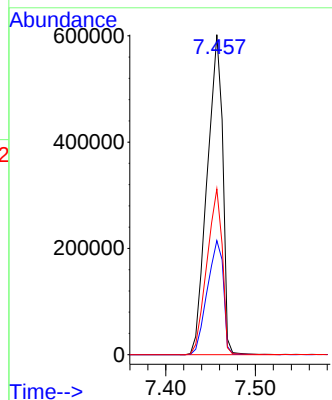

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.933 min Scan# 1300
Delta R.T. -0.006 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33


Tgt Ion:164 Resp: 218531
Ion Ratio Lower Upper
164 100
162 95.5 76.0 114.0
160 43.5 34.8 52.2

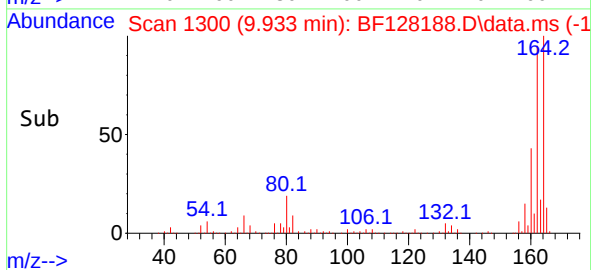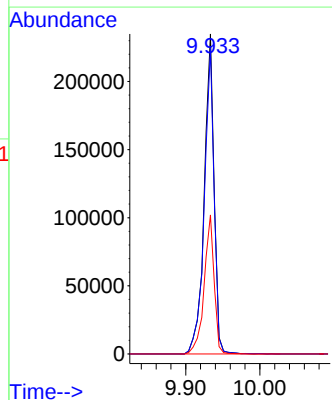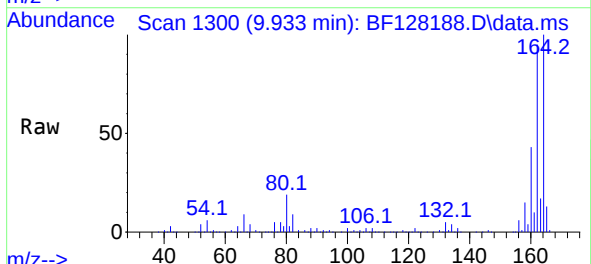



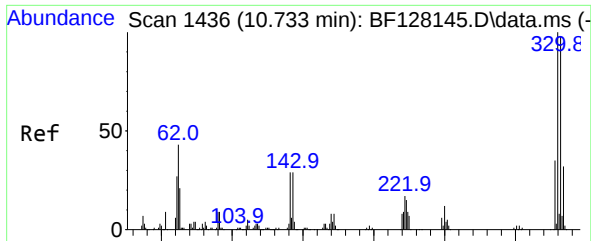


#42
2,4,6-Tribromophenol
Concen: 124.750 ng
RT: 10.727 min Scan# 1435
Delta R.T. -0.006 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33

Instrument :
BNA_F
ClientSampleId :
PB144653TB



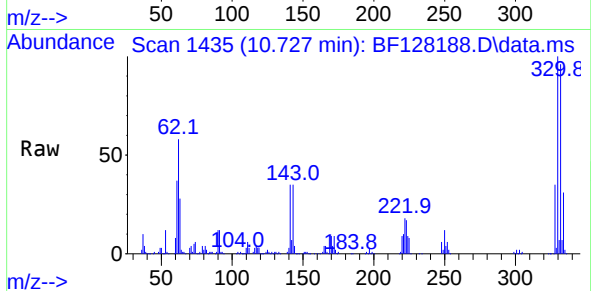


Tgt Ion:330 Resp: 312658
Ion Ratio Lower Upper
330 100
332 96.4 79.0 118.4
141 32.4 28.9 43.3

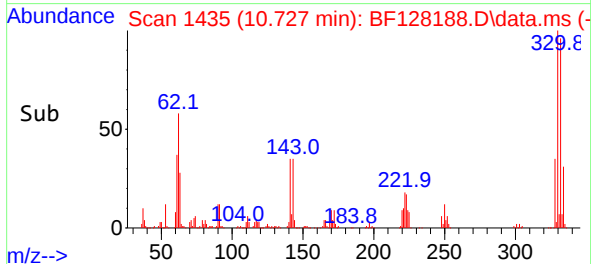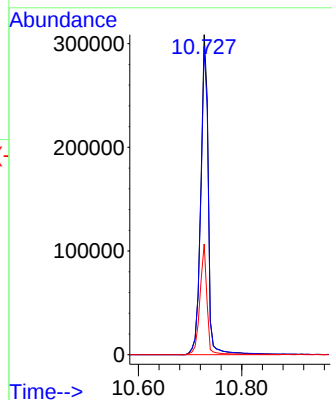

#45
2-Fluorobiphenyl
Concen: 86.344 ng
RT: 9.251 min Scan# 1184
Delta R.T. -0.006 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33

Tgt Ion:172 Resp: 1205916
Ion Ratio Lower Upper
172 100
171 34.7 28.6 42.8
170 23.7 19.1 28.7


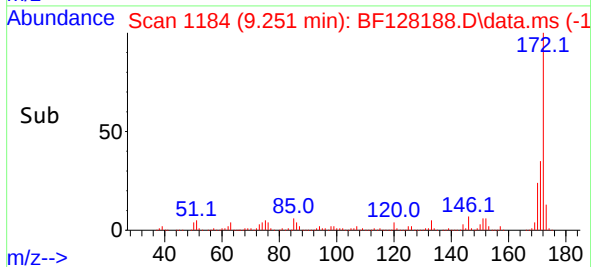
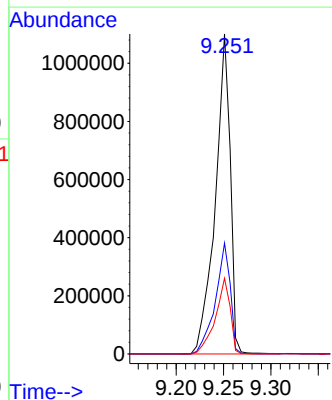
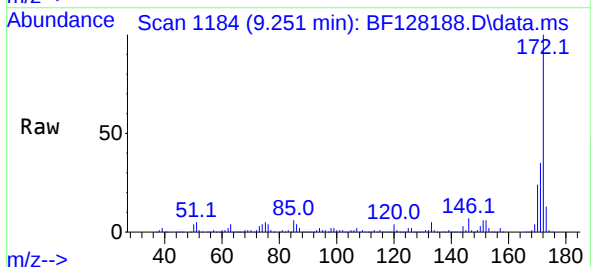




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.421 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33




Instrument :
BNA_F
ClientSampleId :
PB144653TB

Tgt Ion:188 Resp: 407794
Ion Ratio Lower Upper
188 100
94 9.0 8.0 12.0
80 10.5 8.9 13.3

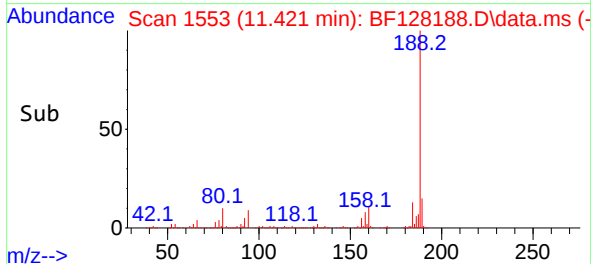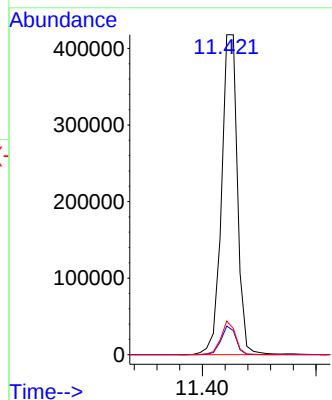

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.068 min Scan# 2003
Delta R.T. -0.012 min
Lab File: BF128188.D
Acq: 11 May 2022 11:33

Tgt Ion:240 Resp: 323097
Ion Ratio Lower Upper
240 100
120 9.5 7.0 10.6
236 26.3 20.3 30.5


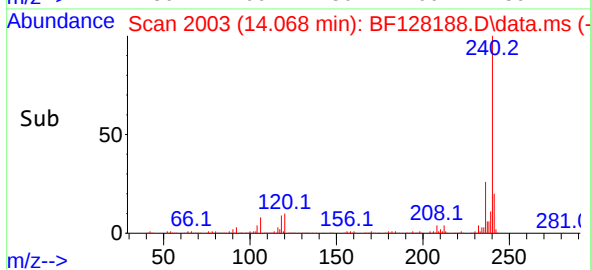
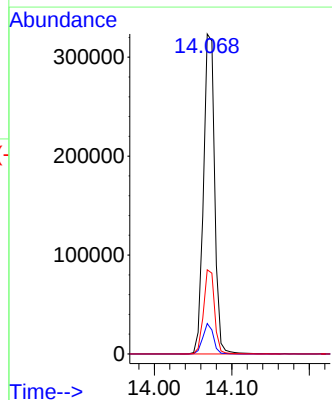
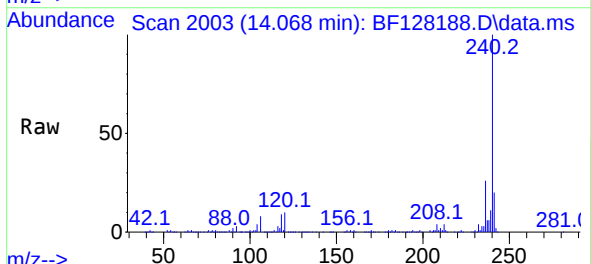




#79
 Terphenyl-d14
 Concen: 86.507 ng
 RT: 13.015 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BF128188.D
 Acq: 11 May 2022 11:33

Instrument :
 BNA_F
 ClientSampleId :
 PB144653TB

Tgt Ion:244 Resp: 1489558
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.2 9.4
 122 10.3 8.6 12.8

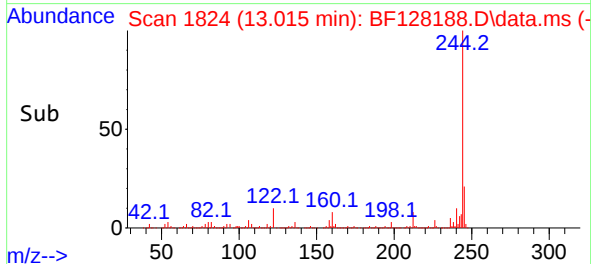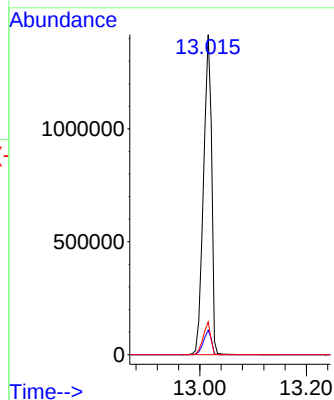

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.568 min Scan# 2258
 Delta R.T. -0.006 min
 Lab File: BF128188.D
 Acq: 11 May 2022 11:33

Tgt Ion:264 Resp: 265282
 Ion Ratio Lower Upper
 264 100
 260 24.0 20.1 30.1
 265 21.5 17.5 26.3

