

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
 Data File : BF128205.D
 Acq On : 11 May 2022 20:16
 Operator : CG\JU
 Sample : N2762-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB18

Quant Time: May 12 06:01:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 09 15:30:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.892	152	85348	20.000	ng	0.00
21) Naphthalene-d8	8.175	136	329801	20.000	ng	0.00
39) Acenaphthene-d10	9.933	164	182148	20.000	ng	0.00
64) Phenanthrene-d10	11.422	188	314836	20.000	ng	0.00
76) Chrysene-d12	14.068	240	186734	20.000	ng	-0.01
86) Perylene-d12	15.562	264	173332	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	494434	92.351	ng	0.00
7) Phenol-d6	6.522	99	645718	91.186	ng	0.00
23) Nitrobenzene-d5	7.457	82	463920	63.295	ng	0.00
42) 2,4,6-Tribromophenol	10.727	330	186149	89.108	ng	0.00
45) 2-Fluorobiphenyl	9.251	172	727834	62.523	ng	0.00
79) Terphenyl-d14	13.010	244	657057	66.025	ng	0.00
Target Compounds						
						Qvalue
75) Fluoranthene	12.639	202	38250	2.251	ng	96
78) Pyrene	12.868	202	34969	2.583	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128205.D
Acq On : 11 May 2022 20:16
Operator : CG\JU
Sample : N2762-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB18

Quant Time: May 12 06:01:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 15:30:11 2022
Response via : Initial Calibration




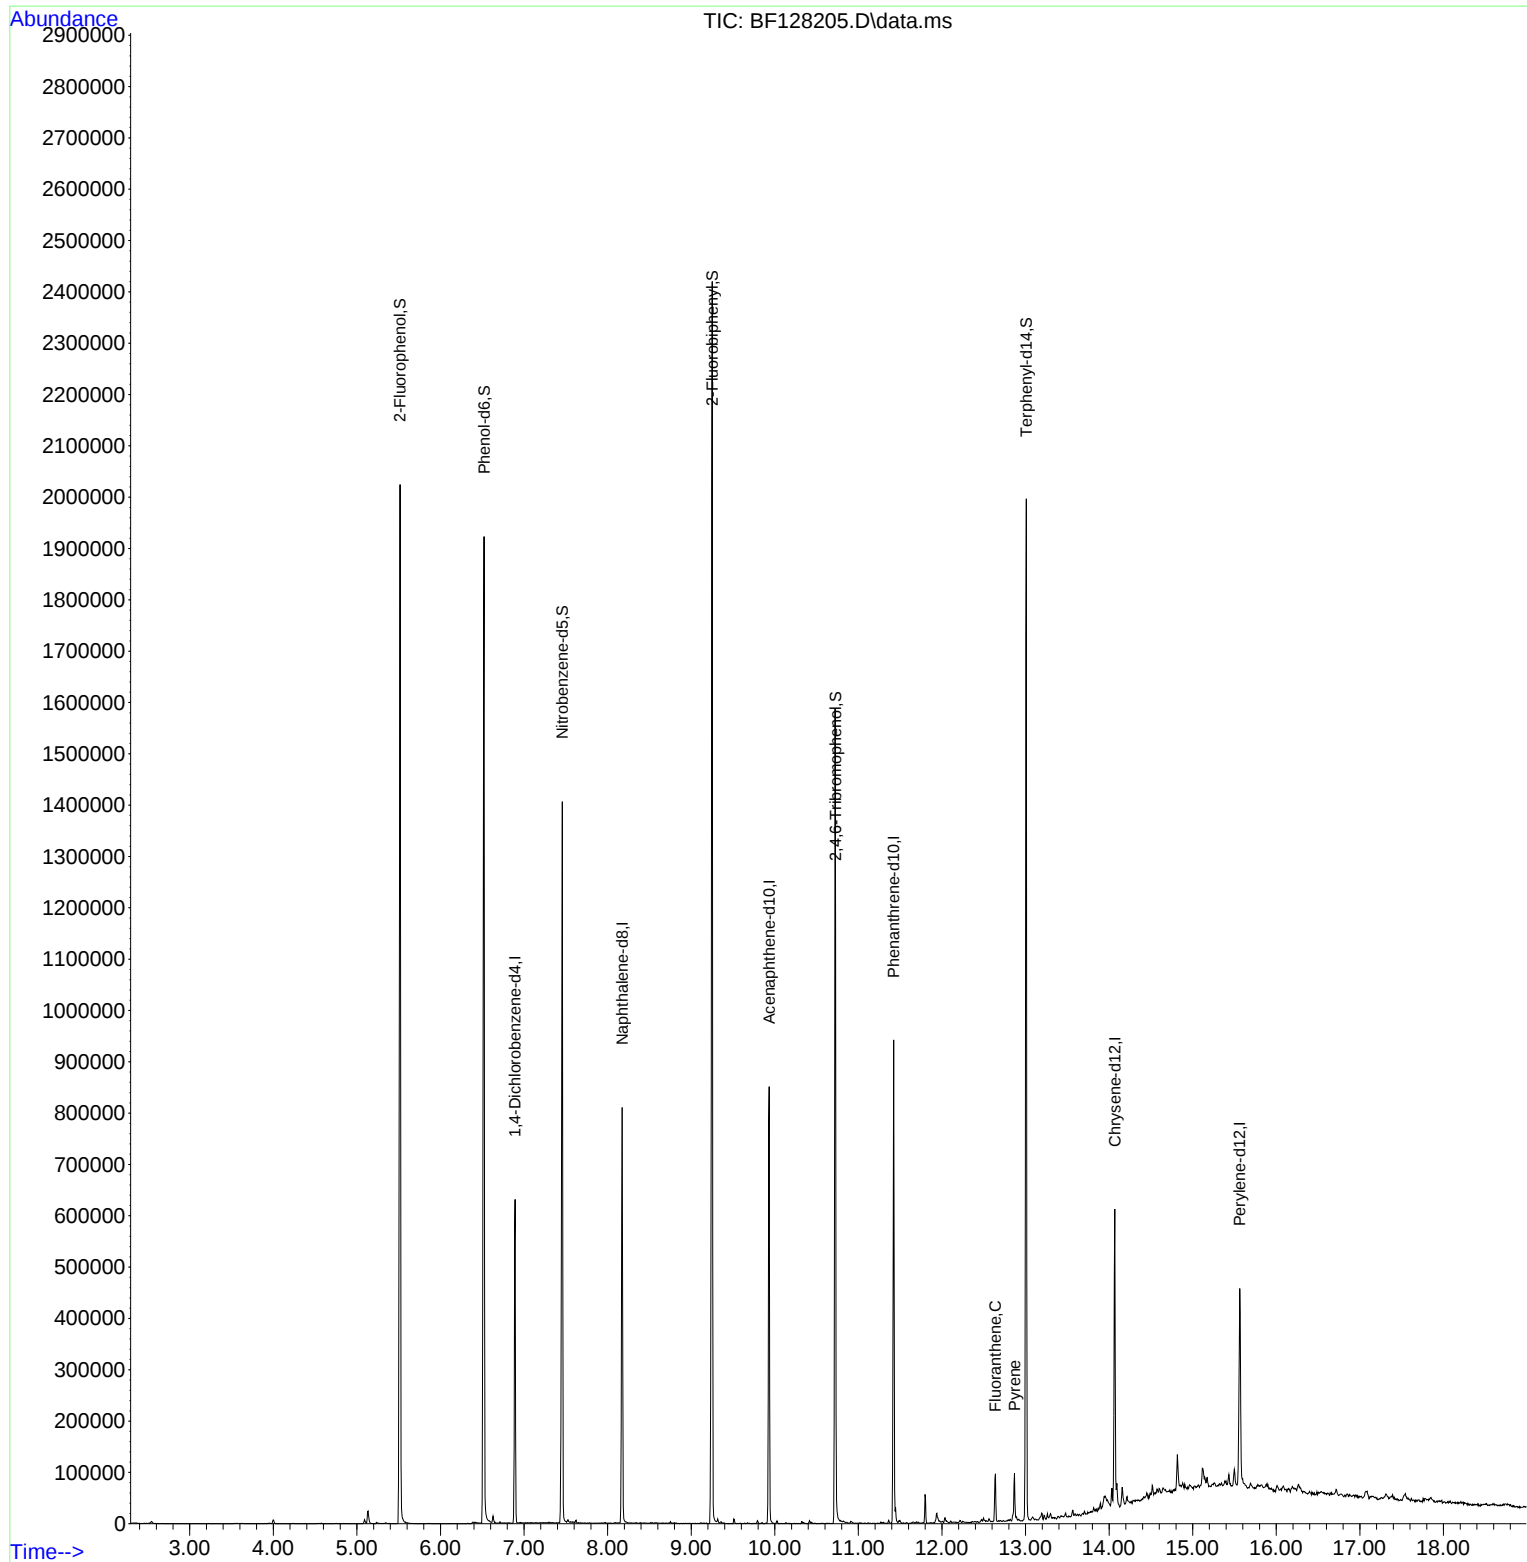




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.892 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16




Instrument :
BNA_F
ClientSampleId :
SB18


Tgt Ion:152 Resp: 85348
Ion Ratio Lower Upper
152 100
150 156.9 125.3 187.9
115 65.4 48.8 73.2

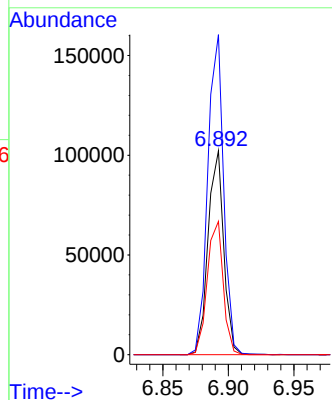

#5
2-Fluorophenol
Concen: 92.351 ng
RT: 5.516 min Scan# 549
Delta R.T. -0.000 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16

Tgt Ion:112 Resp: 494434
Ion Ratio Lower Upper
112 100
64 67.2 49.5 74.3
63 36.8 26.3 39.5


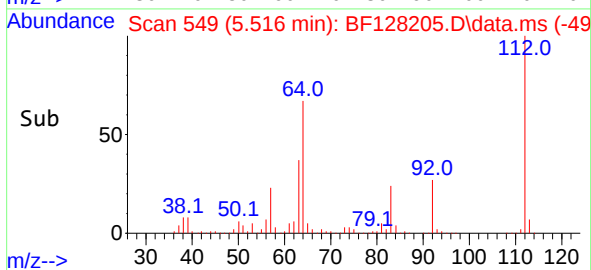
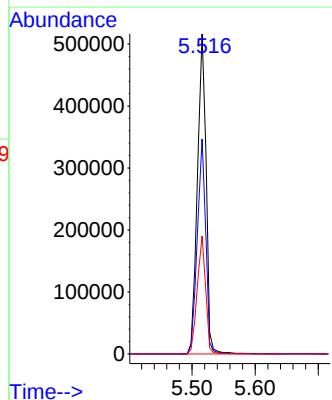





#7
Phenol-d6
Concen: 91.186 ng
RT: 6.522 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16




Instrument :
BNA_F
ClientSampleId :
SB18


Tgt Ion: 99 Resp: 645718
Ion Ratio Lower Upper
99 100
42 21.3 16.6 24.8
71 40.1 30.0 45.0

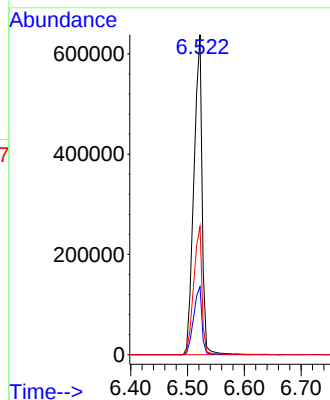

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.175 min Scan# 1001
Delta R.T. -0.006 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16

Tgt Ion: 136 Resp: 329801
Ion Ratio Lower Upper
136 100
137 10.9 8.6 13.0
54 8.2 6.8 10.2
68 5.6 5.1 7.7


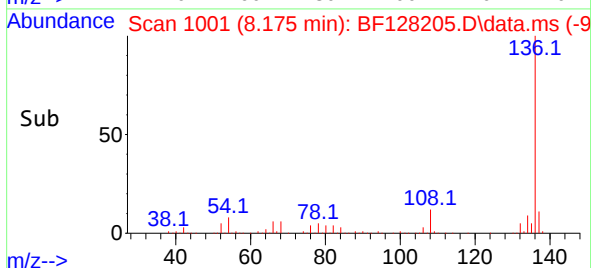
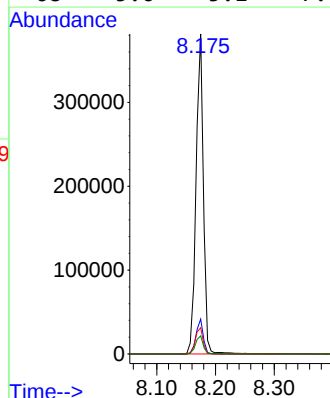





#23
Nitrobenzene-d5
Concen: 63.295 ng
RT: 7.457 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16




Instrument :
BNA_F
ClientSampleId :
SB18


Tgt Ion: 82 Resp: 463920
Ion Ratio Lower Upper
82 100
128 35.5 30.0 45.0
54 50.7 41.3 61.9

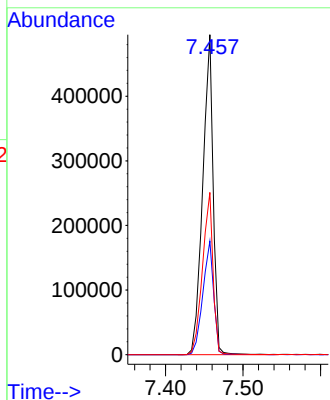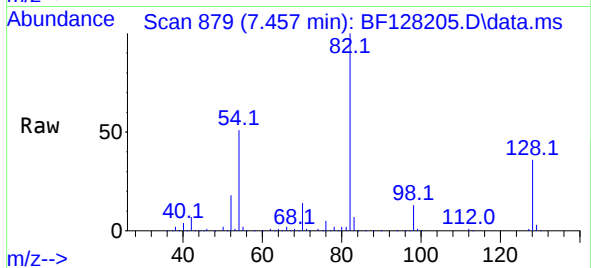

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.933 min Scan# 1300
Delta R.T. -0.006 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16

Tgt Ion:164 Resp: 182148
Ion Ratio Lower Upper
164 100
162 97.1 76.0 114.0
160 43.4 34.8 52.2

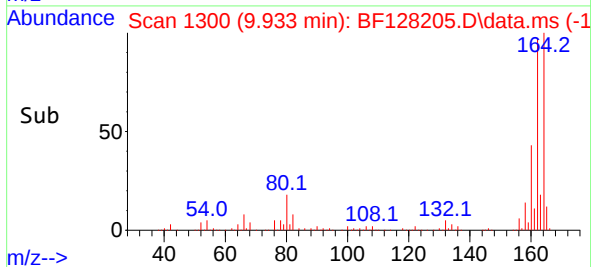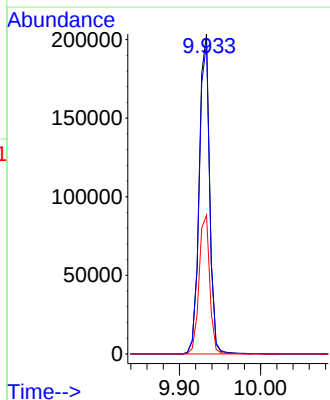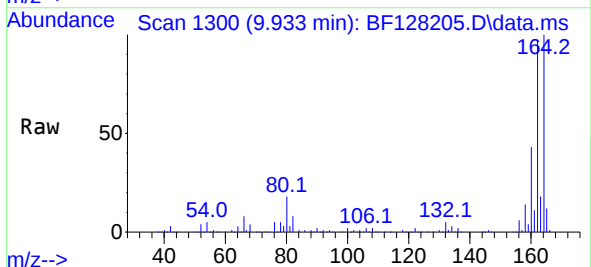

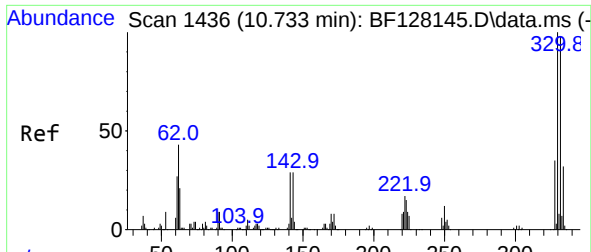

#42

2,4,6-Tribromophenol

Concen: 89.108 ng

RT: 10.727 min Scan# 1435

Delta R.T. -0.006 min

Lab File: BF128205.D

Acq: 11 May 2022 20:16

Instrument :

BNA_F

ClientSampleId :

SB18





Tgt Ion:330 Resp: 186149

Ion Ratio Lower Upper

330 100

332 96.4 79.0 118.4

141 34.0 28.9 43.3

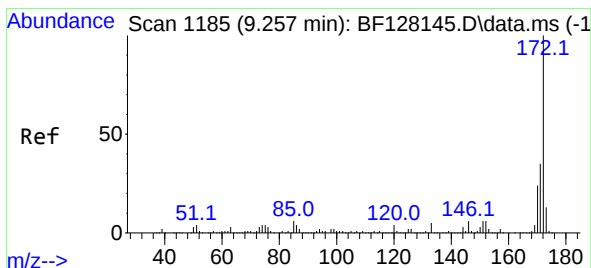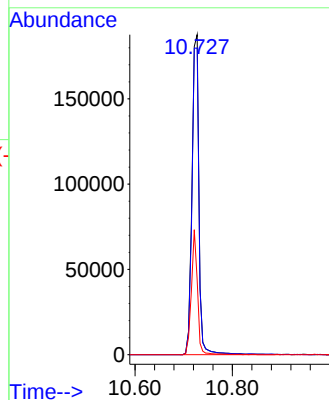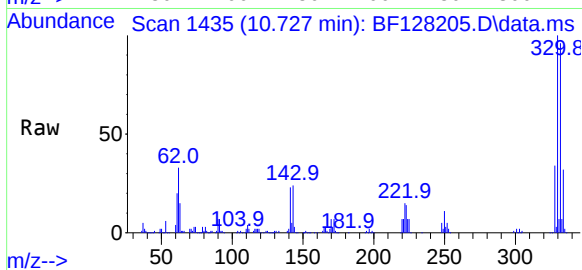

#45

2-Fluorobiphenyl

Concen: 62.523 ng

RT: 9.251 min Scan# 1184

Delta R.T. -0.006 min

Lab File: BF128205.D

Acq: 11 May 2022 20:16




Tgt Ion:172 Resp: 727834


Ion Ratio Lower Upper

172 100

171 35.2 28.6 42.8

170 23.5 19.1 28.7


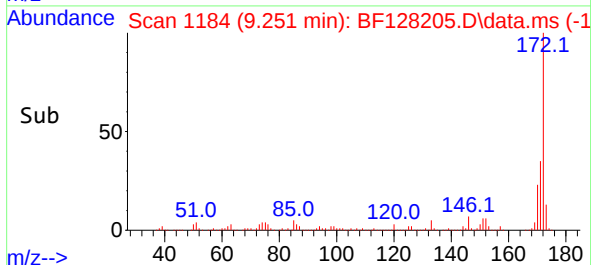
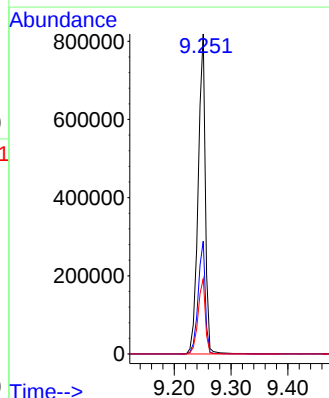
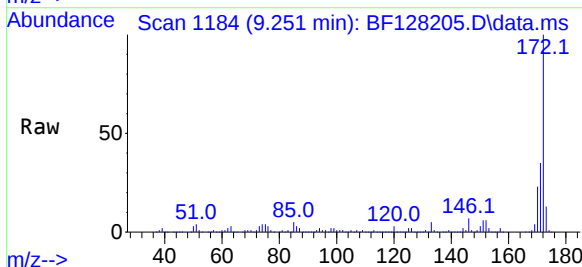




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.422 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16




Instrument :
BNA_F
ClientSampleId :
SB18


Tgt Ion:188 Resp: 314836
Ion Ratio Lower Upper
188 100
94 8.6 8.0 12.0
80 9.4 8.9 13.3

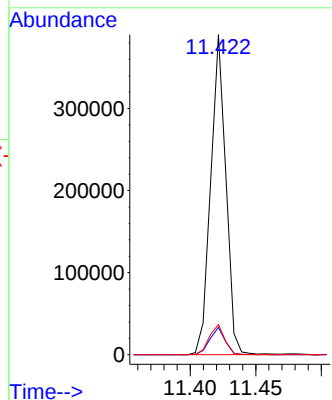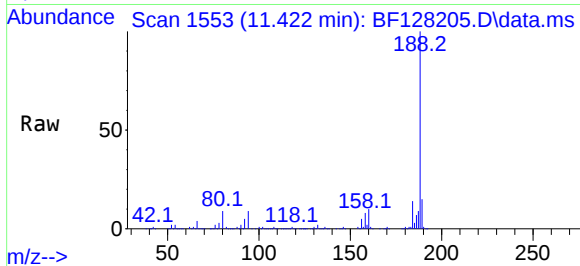

#75
Fluoranthene
Concen: 2.251 ng
RT: 12.639 min Scan# 1760
Delta R.T. -0.006 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16

Tgt Ion:202 Resp: 38250
Ion Ratio Lower Upper
202 100
101 8.8 0.0 31.6
203 17.5 0.0 38.1


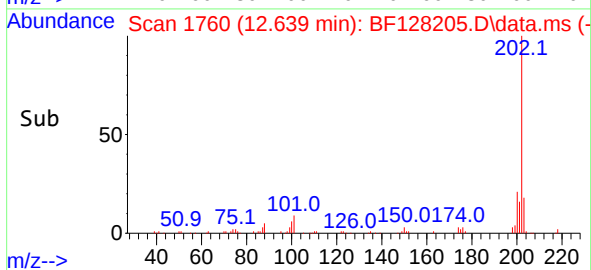
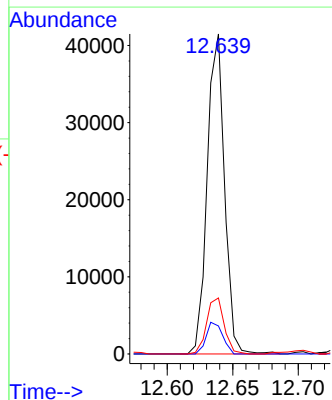
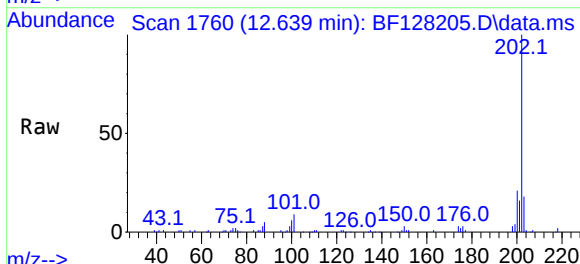




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.068 min Scan# 20
Delta R.T. -0.012 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16




Instrument :
BNA_F
ClientSampleId :
SB18


Tgt Ion:240 Resp: 186734
Ion Ratio Lower Upper
240 100
120 8.5 7.0 10.6
236 25.2 20.3 30.5

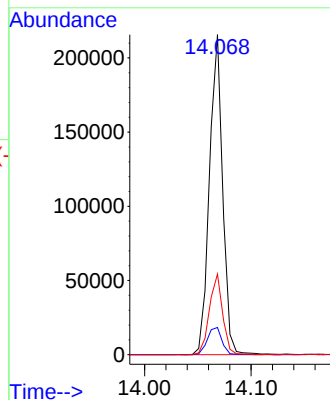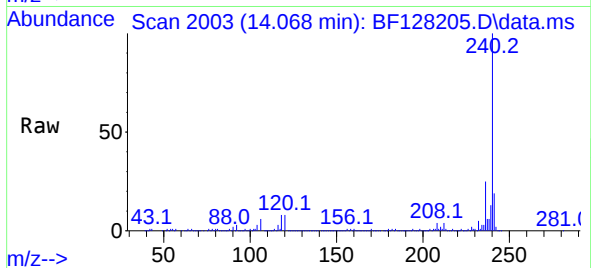

#78
Pyrene
Concen: 2.583 ng
RT: 12.868 min Scan# 1799
Delta R.T. -0.012 min
Lab File: BF128205.D
Acq: 11 May 2022 20:16

Tgt Ion:202 Resp: 34969
Ion Ratio Lower Upper
202 100
200 22.3 17.4 26.2
203 17.8 14.0 21.0


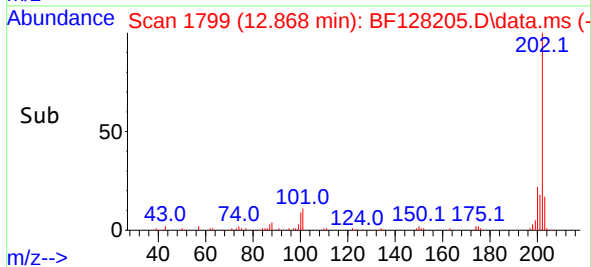
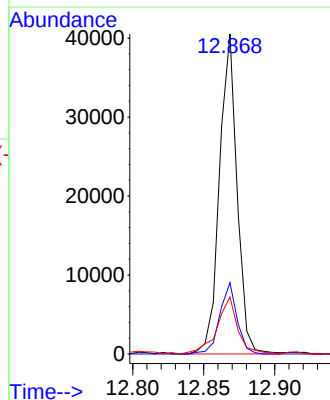
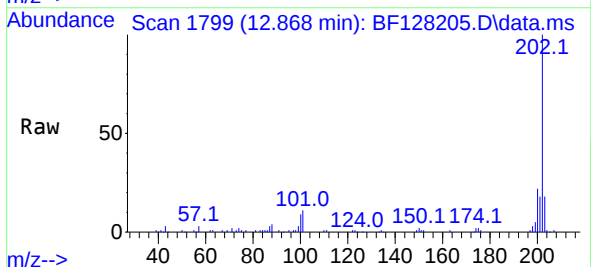




#79
 Terphenyl-d14
 Concen: 66.025 ng
 RT: 13.010 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF128205.D
 Acq: 11 May 2022 20:16

Instrument :
 BNA_F
 ClientSampleId :
 SB18

Tgt Ion:244 Resp: 657057
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.2 9.4
 122 8.0 8.6 12.8#

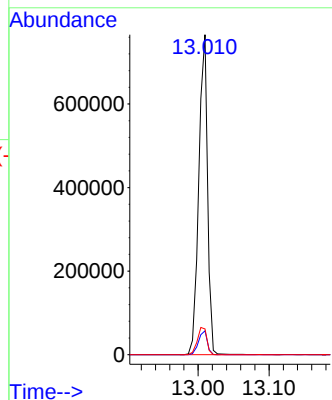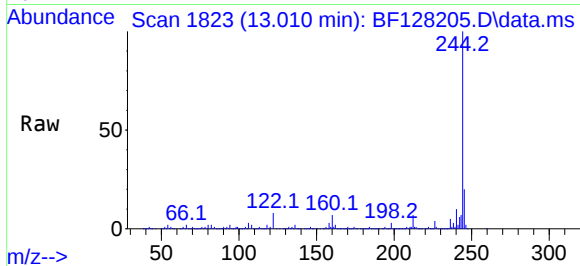

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.562 min Scan# 2257
 Delta R.T. -0.012 min
 Lab File: BF128205.D
 Acq: 11 May 2022 20:16

Tgt Ion:264 Resp: 173332
 Ion Ratio Lower Upper
 264 100
 260 23.2 20.1 30.1
 265 21.1 17.5 26.3

