

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
 Data File : BF128192.D
 Acq On : 11 May 2022 13:52
 Operator : CG\JU
 Sample : PB144720BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144720BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	546	551	554	rBV	2756755	2910412	75.06%	12.798%
2	6.522	714	720	723	rBV	2459651	2994711	77.23%	13.169%
3	6.892	779	783	786	rBV	705248	624994	16.12%	2.748%
4	7.457	873	879	882	rBV	1777341	2065435	53.26%	9.082%
5	8.175	995	1001	1004	rBV	821517	812326	20.95%	3.572%
6	9.251	1177	1184	1187	rBV	3453963	3622903	93.43%	15.931%
7	9.933	1293	1300	1303	rBV	1025235	943588	24.33%	4.149%
8	10.727	1429	1435	1438	rBV	2469041	2284681	58.92%	10.047%
9	11.422	1547	1553	1557	rBV	1063627	999094	25.77%	4.393%
10	13.016	1818	1824	1827	rBV	3984797	3877686	100.00%	17.051%
11	14.068	1999	2003	2014	rVB	952906	857303	22.11%	3.770%
12	15.568	2252	2258	2268	rBV	515838	693620	17.89%	3.050%
13	17.374	2555	2565	2566	rBV5	22365	54305	1.40%	0.239%




Sum of corrected areas: 22741058

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128192.D
Acq On : 11 May 2022 13:52
Operator : CG\JU
Sample : PB144720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144720BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

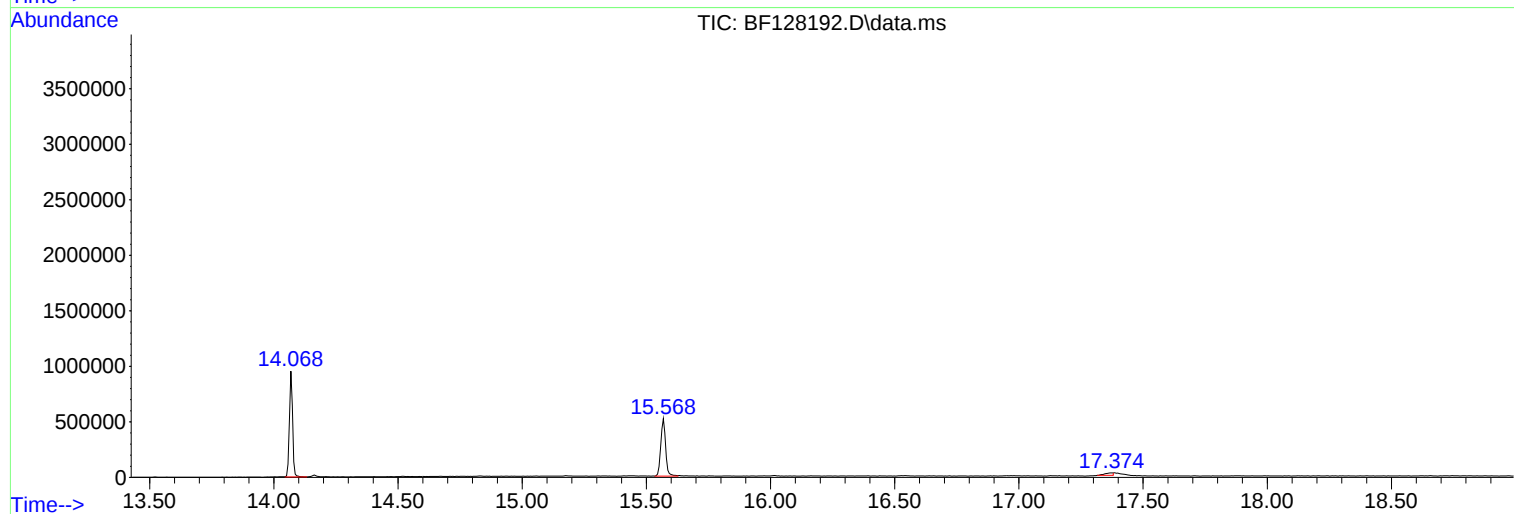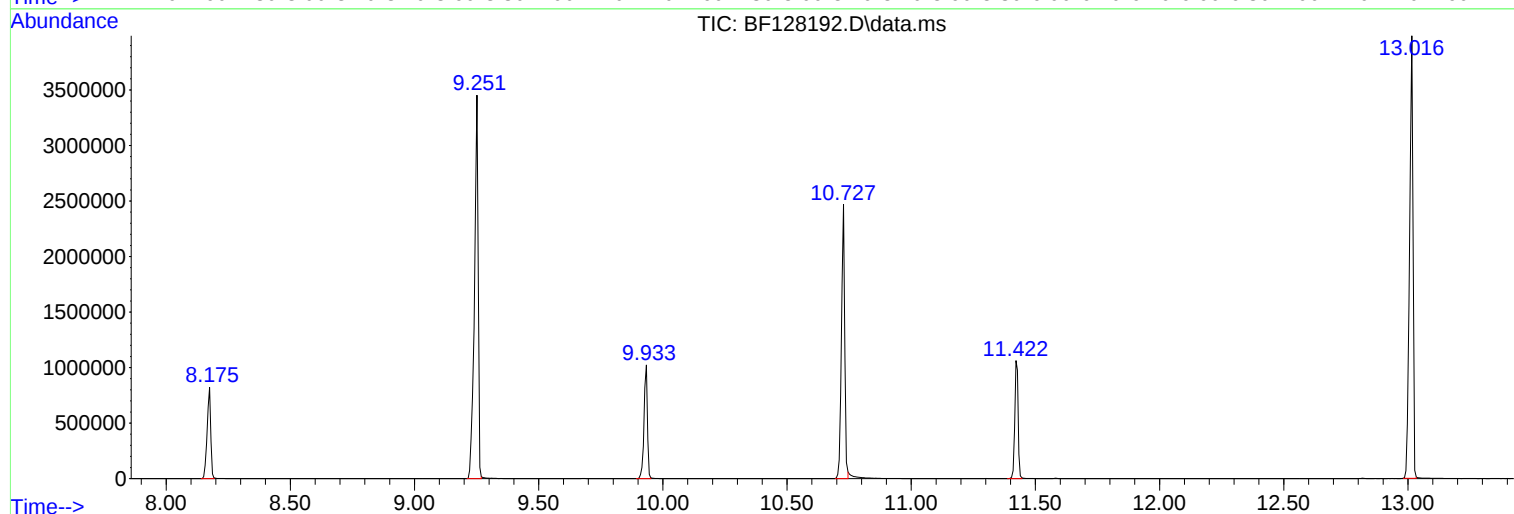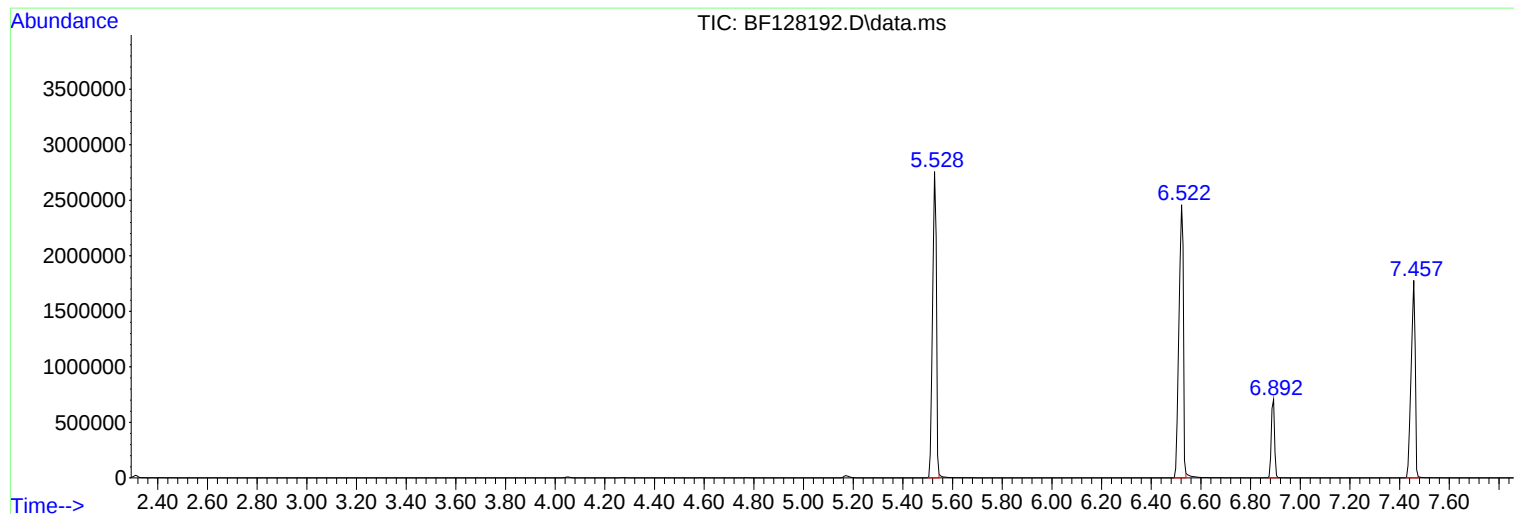

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128192.D
Acq On : 11 May 2022 13:52
Operator : CG\JU
Sample : PB144720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144720BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128192.D
Acq On : 11 May 2022 13:52
Operator : CG\JU
Sample : PB144720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144720BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------