

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
 Data File : BF128193.D
 Acq On : 11 May 2022 14:20
 Operator : CG\JU
 Sample : PB144740BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144740BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	546	551	554	rBV	2349688	2173223	53.51%	10.130%
2	6.522	714	720	723	rBV	2086552	2224934	54.79%	10.371%
3	6.892	779	783	786	rBV	678244	623249	15.35%	2.905%
4	7.457	873	879	882	rBV	1850329	2223700	54.76%	10.365%
5	8.175	995	1001	1004	rBV	822822	851502	20.97%	3.969%
6	9.251	1177	1184	1187	rBV	3672309	3864947	95.17%	18.015%
7	9.933	1293	1300	1303	rBV	1060883	985834	24.28%	4.595%
8	10.727	1429	1435	1460	rBV	1646313	1765824	43.48%	8.231%
9	11.422	1547	1553	1557	rBV	1148889	1040793	25.63%	4.851%
10	13.016	1818	1824	1827	rBV	4136278	4060975	100.00%	18.929%
11	14.068	1999	2003	2007	rBV	973344	883238	21.75%	4.117%
12	15.568	2252	2258	2271	rBV	562779	755482	18.60%	3.521%




Sum of corrected areas: 21453701

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128193.D
Acq On : 11 May 2022 14:20
Operator : CG\JU
Sample : PB144740BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144740BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

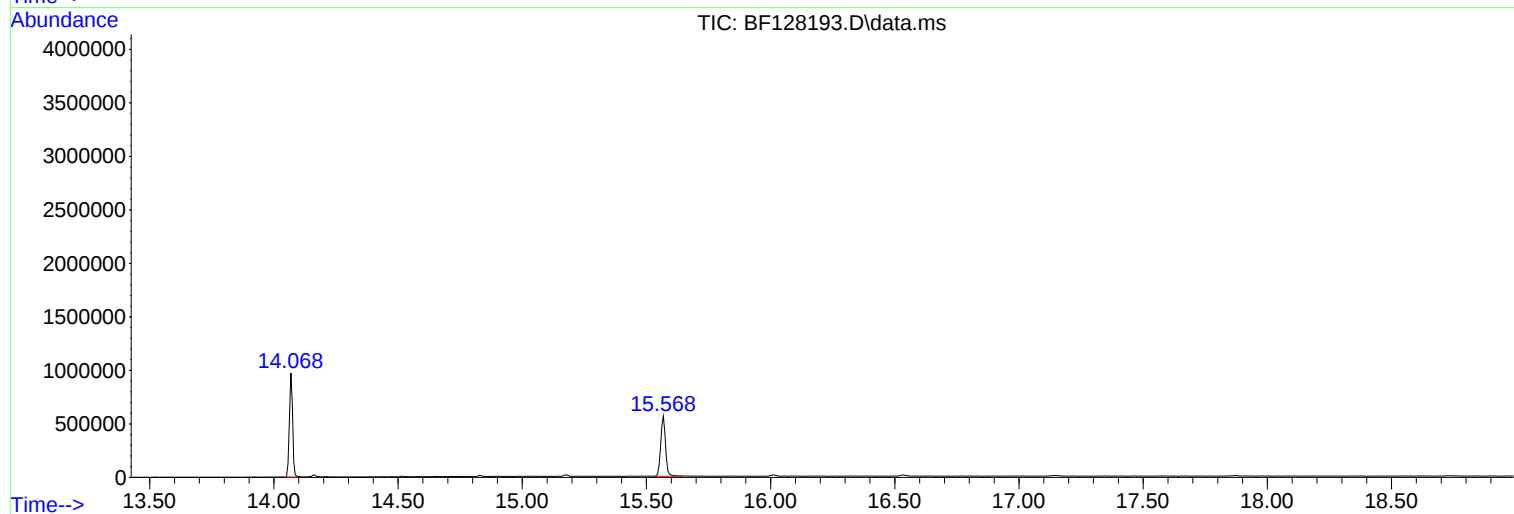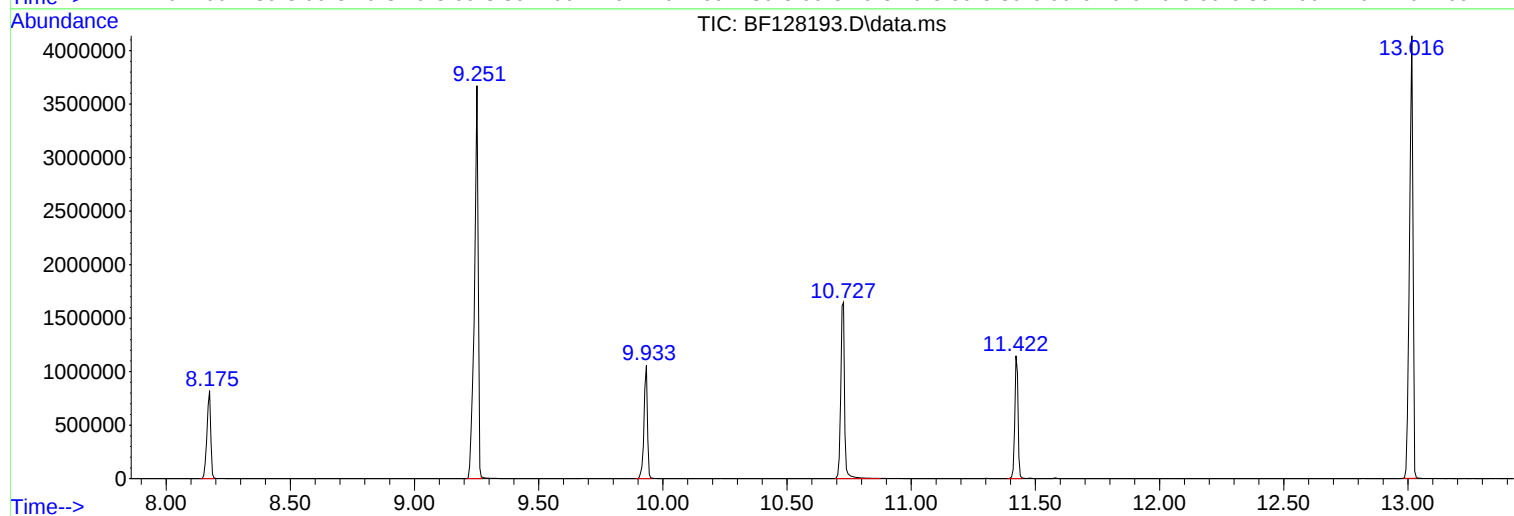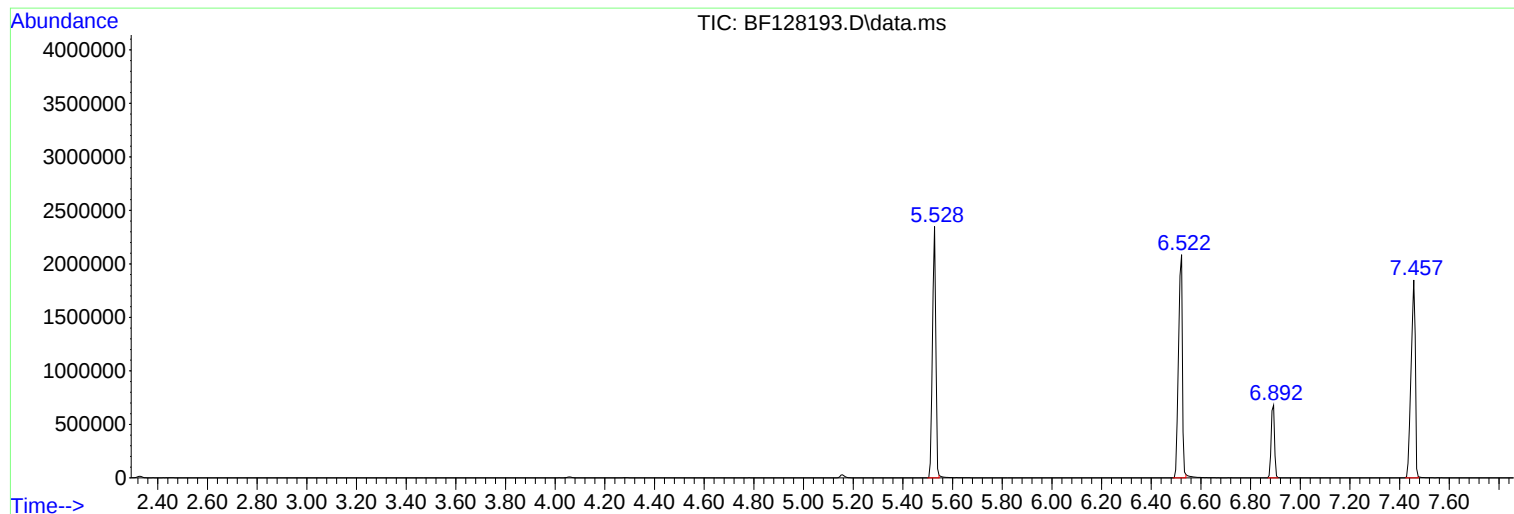

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128193.D
Acq On : 11 May 2022 14:20
Operator : CG\JU
Sample : PB144740BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144740BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128193.D
Acq On : 11 May 2022 14:20
Operator : CG\JU
Sample : PB144740BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144740BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------